

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042516.D
 Acq On : 24 Jul 2024 14:41
 Operator : JC/MD
 Sample : P3327-24 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	32	rBV2	4846	8328	1.58%	0.177%
2	1.368	43	46	63	rVB	38881	52807	9.99%	1.122%
3	1.483	63	65	67	rBV2	259	189	0.04%	0.004%
4	1.648	88	92	101	rVB	34454	43979	8.32%	0.934%
5	1.935	137	139	141	rBV	321	229	0.04%	0.005%
6	2.032	151	155	157	rBV2	180	203	0.04%	0.004%
7	2.227	185	187	189	rBV2	205	217	0.04%	0.005%
8	2.294	192	198	210	rVV	96868	156997	29.71%	3.336%
9	2.502	231	232	239	rVB	233	179	0.03%	0.004%
10	2.587	245	246	248	rBV2	118	90	0.02%	0.002%
11	2.715	259	267	269	rBV2	198	389	0.07%	0.008%
12	2.788	273	279	288	rVV3	1542	3130	0.59%	0.067%
13	2.940	295	304	317	rBV	7703	17825	3.37%	0.379%
14	3.062	321	324	326	rBV2	104	152	0.03%	0.003%
15	3.081	326	327	332	rVB2	343	401	0.08%	0.009%
16	3.172	340	342	343	rBV	145	132	0.02%	0.003%
17	3.215	346	349	350	rBV	129	118	0.02%	0.003%
18	3.288	360	361	366	rVB	146	105	0.02%	0.002%
19	3.325	366	367	370	rBV	102	90	0.02%	0.002%
20	3.367	370	374	377	rVB	102	110	0.02%	0.002%
21	3.398	377	379	383	rBV	123	150	0.03%	0.003%
22	3.434	383	385	389	rVB2	124	154	0.03%	0.003%
23	3.489	389	394	396	rBV2	105	201	0.04%	0.004%
24	3.611	407	414	419	rBV	2061	3965	0.75%	0.084%
25	3.672	423	424	427	rBV2	132	158	0.03%	0.003%
26	3.770	439	440	442	rBV2	135	112	0.02%	0.002%
27	3.843	448	452	454	rVB2	118	171	0.03%	0.004%
28	3.861	454	455	457	rBV	156	142	0.03%	0.003%
29	3.910	460	463	464	rVB	164	150	0.03%	0.003%
30	4.391	540	542	544	rVB	128	89	0.02%	0.002%
31	4.477	546	556	572	rBV2	60428	198602	37.58%	4.220%
32	4.885	621	623	624	rBB	157	102	0.02%	0.002%
33	4.965	633	636	638	rBV2	141	200	0.04%	0.004%
34	5.056	640	651	672	rVV	68543	213969	40.49%	4.547%
35	5.342	693	698	702	rBV2	99	176	0.03%	0.004%
36	5.391	702	706	707	rBV2	349	486	0.09%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042516.D
 Acq On : 24 Jul 2024 14:41
 Operator : JC/MD
 Sample : P3327-24 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.477	718	720	725	rBV2	109	214	0.04%	0.005%
38	5.550	729	732	737	rBV2	401	846	0.16%	0.018%
39	5.702	754	757	758	rBV2	124	148	0.03%	0.003%
40	5.873	784	785	786	rBV	157	104	0.02%	0.002%
41	5.964	790	800	817	rVV2	179676	528421	100.00%	11.228%
42	6.251	846	847	851	rBV2	200	256	0.05%	0.005%
43	6.458	880	881	882	rBV	169	73	0.01%	0.002%
44	6.611	905	906	908	rBV	111	79	0.01%	0.002%
45	6.763	922	931	942	rBV	161692	389351	73.68%	8.273%
46	7.019	971	973	976	rVB2	229	165	0.03%	0.004%
47	7.123	982	990	1007	rBV	176884	394076	74.58%	8.374%
48	7.306	1012	1020	1035	rVV	107849	238926	45.22%	5.077%
49	7.537	1057	1058	1061	rVB	169	76	0.01%	0.002%
50	7.641	1074	1075	1080	rBV	150	161	0.03%	0.003%
51	7.720	1086	1088	1090	rBV	84	89	0.02%	0.002%
52	7.903	1115	1118	1120	rBV2	121	181	0.03%	0.004%
53	8.116	1151	1153	1155	rBV2	92	78	0.01%	0.002%
54	8.238	1169	1173	1174	rBV2	148	170	0.03%	0.004%
55	8.324	1181	1187	1200	rBV	63245	107341	20.31%	2.281%
56	8.507	1215	1217	1218	rBV2	256	225	0.04%	0.005%
57	8.647	1233	1240	1255	rBV	264418	425388	80.50%	9.039%
58	8.952	1285	1290	1305	rBV	45222	71038	13.44%	1.509%
59	9.238	1335	1337	1339	rBV	152	136	0.03%	0.003%
60	9.281	1339	1344	1348	rBV3	1478	2151	0.41%	0.046%
61	9.330	1351	1352	1356	rVB	127	73	0.01%	0.002%
62	9.391	1356	1362	1378	rBV	172168	270671	51.22%	5.751%
63	9.604	1394	1397	1398	rBV2	187	194	0.04%	0.004%
64	9.701	1409	1413	1419	rVB	1492	1751	0.33%	0.037%
65	9.860	1437	1439	1442	rVB	157	116	0.02%	0.002%
66	9.903	1445	1446	1447	rBV	188	94	0.02%	0.002%
67	10.006	1462	1463	1465	rVB	139	90	0.02%	0.002%
68	10.055	1465	1471	1487	rBV	332377	456716	86.43%	9.705%
69	10.275	1506	1507	1508	rBV	213	85	0.02%	0.002%
70	10.317	1511	1514	1519	rVB2	420	579	0.11%	0.012%
71	10.500	1542	1544	1545	rBV	154	103	0.02%	0.002%
72	10.598	1558	1560	1561	rBV	97	88	0.02%	0.002%
73	10.713	1576	1579	1582	rVB2	119	130	0.02%	0.003%
74	10.738	1582	1583	1586	rBV2	93	86	0.02%	0.002%
75	10.787	1589	1591	1595	rVB2	216	272	0.05%	0.006%
76	10.817	1595	1596	1598	rBV2	109	107	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042516.D
 Acq On : 24 Jul 2024 14:41
 Operator : JC/MD
 Sample : P3327-24 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	10.842	1598	1600	1602	rVV2	110	94	0.02%	0.002%
78	11.067	1635	1637	1638	rBV	114	101	0.02%	0.002%
79	11.189	1652	1657	1667	rBV	219463	293973	55.63%	6.247%
80	11.317	1674	1678	1682	rBV2	569	789	0.15%	0.017%
81	11.537	1711	1714	1717	rVB2	119	130	0.02%	0.003%
82	11.707	1740	1742	1744	rBV2	100	99	0.02%	0.002%
83	11.762	1750	1751	1754	rBV	170	111	0.02%	0.002%
84	11.860	1765	1767	1768	rVB	150	79	0.01%	0.002%
85	11.982	1783	1787	1788	rBV	259	312	0.06%	0.007%
86	12.024	1789	1794	1805	rVV	331020	415068	78.55%	8.820%
87	12.317	1837	1842	1857	rBV	300646	396271	74.99%	8.420%
88	12.762	1912	1915	1919	rVB2	980	1140	0.22%	0.024%
89	12.927	1940	1942	1943	rVB	165	84	0.02%	0.002%
90	12.951	1944	1946	1948	rVV	128	98	0.02%	0.002%
91	12.987	1950	1952	1955	rVB2	102	96	0.02%	0.002%
92	13.085	1966	1968	1971	rVB2	126	103	0.02%	0.002%
93	13.365	2012	2014	2016	rVB	142	76	0.01%	0.002%
94	13.390	2016	2018	2021	rVB2	114	112	0.02%	0.002%
95	13.567	2044	2047	2048	rBV2	127	112	0.02%	0.002%
96	14.128	2136	2139	2146	rVB2	1008	1371	0.26%	0.029%
97	14.268	2160	2162	2164	rBV2	111	107	0.02%	0.002%
98	14.463	2192	2194	2195	rBV2	199	186	0.04%	0.004%
99	14.701	2232	2233	2235	rBV	298	167	0.03%	0.004%
100	14.743	2239	2240	2242	rVB	330	177	0.03%	0.004%




Sum of corrected areas: 4706201

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042516.D
Acq On : 24 Jul 2024 14:41
Operator : JC/MD
Sample : P3327-24 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

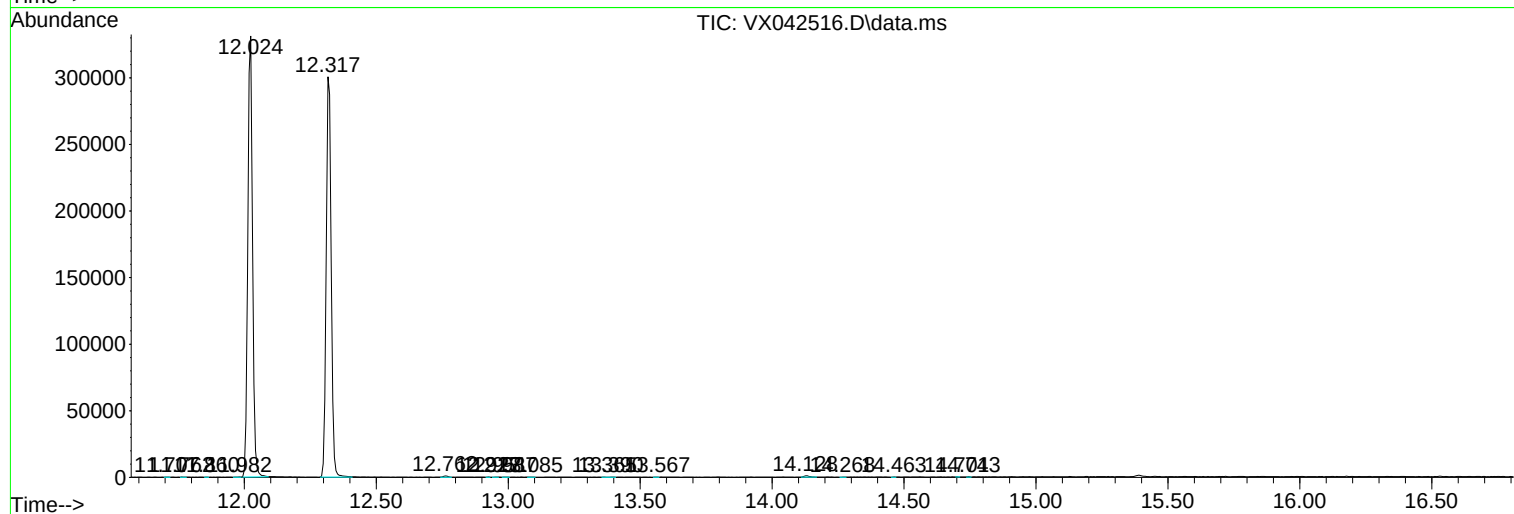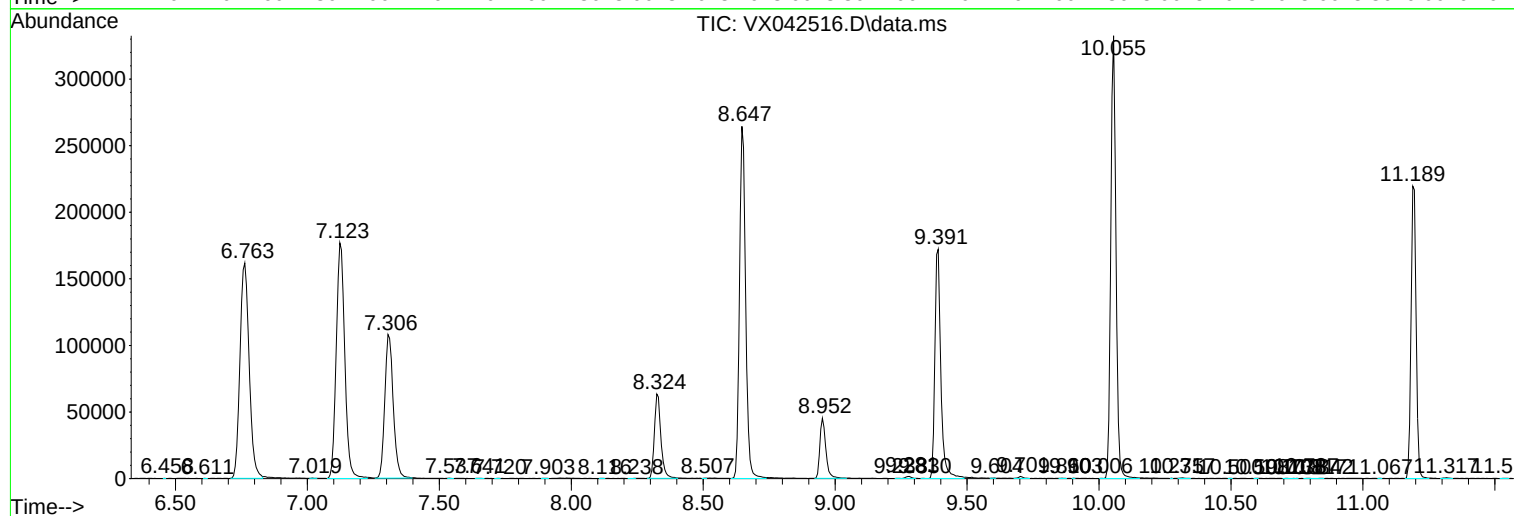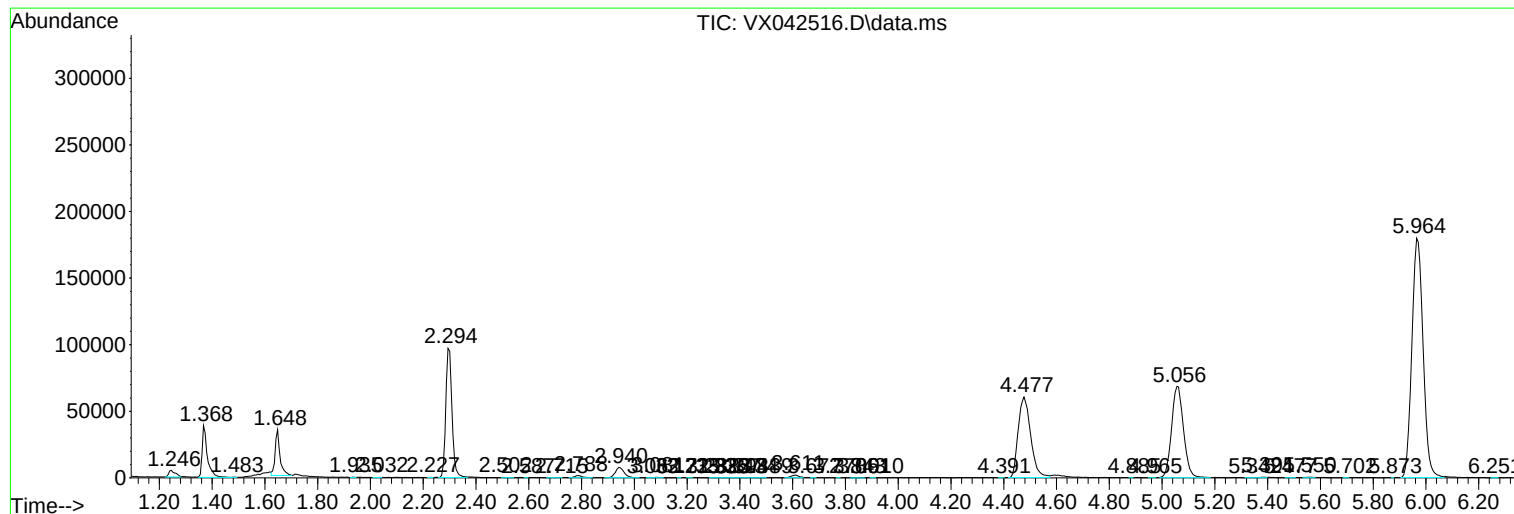

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042516.D
Acq On : 24 Jul 2024 14:41
Operator : JC/MD
Sample : P3327-24 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042516.D
Acq On : 24 Jul 2024 14:41
Operator : JC/MD
Sample : P3327-24 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc