

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042517.D
 Acq On : 24 Jul 2024 15:04
 Operator : JC/MD
 Sample : P3327-25 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	4748	5477	0.99%	0.113%
2	1.295	33	34	36	rVB	440	176	0.03%	0.004%
3	1.368	43	46	59	rVB	41989	53818	9.77%	1.115%
4	1.502	66	68	69	rBV2	249	190	0.03%	0.004%
5	1.563	69	78	79	rBV2	1744	3378	0.61%	0.070%
6	1.581	79	81	82	rVV2	2113	2040	0.37%	0.042%
7	1.605	83	85	86	rVV	2994	2908	0.53%	0.060%
8	1.648	88	92	101	rVB	34906	46344	8.41%	0.960%
9	1.837	121	123	125	rVV	176	156	0.03%	0.003%
10	1.862	125	127	129	rVB	307	251	0.05%	0.005%
11	1.929	135	138	140	rBV	245	244	0.04%	0.005%
12	2.044	154	157	158	rBV3	194	237	0.04%	0.005%
13	2.142	172	173	175	rBV3	266	177	0.03%	0.004%
14	2.294	192	198	211	rBV	102138	161779	29.36%	3.351%
15	2.563	240	242	246	rVB2	213	246	0.04%	0.005%
16	2.605	246	249	251	rVB2	142	158	0.03%	0.003%
17	2.654	254	257	258	rBV2	149	159	0.03%	0.003%
18	2.782	273	278	286	rBV2	1821	3938	0.71%	0.082%
19	2.941	296	304	316	rVB	9710	23281	4.23%	0.482%
20	3.069	319	325	326	rBV2	132	158	0.03%	0.003%
21	3.087	326	328	332	rVB3	294	377	0.07%	0.008%
22	3.203	344	347	349	rBV2	132	171	0.03%	0.004%
23	3.605	410	413	414	rBV	214	163	0.03%	0.003%
24	3.721	430	432	433	rBV	192	150	0.03%	0.003%
25	3.916	462	464	467	rBV	101	170	0.03%	0.004%
26	4.215	510	513	515	rBV2	159	217	0.04%	0.004%
27	4.471	546	555	571	rBV2	50372	164346	29.83%	3.404%
28	4.867	618	620	624	rVB2	150	162	0.03%	0.003%
29	4.928	629	630	635	rVB2	137	180	0.03%	0.004%
30	4.965	635	636	639	rBV2	138	157	0.03%	0.003%
31	5.056	639	651	670	rBV	71392	221246	40.15%	4.582%
32	5.379	701	704	705	rBV2	261	275	0.05%	0.006%
33	5.562	728	734	742	rVB2	597	1520	0.28%	0.031%
34	5.830	775	778	781	rBV	107	175	0.03%	0.004%
35	5.964	790	800	820	rBV2	187352	550982	100.00%	11.411%
36	6.214	839	841	845	rVB2	259	291	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042517.D
 Acq On : 24 Jul 2024 15:04
 Operator : JC/MD
 Sample : P3327-25 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	6.330	857	860	861	rBV2	160	193	0.04%	0.004%
38	6.422	873	875	880	rBV2	121	164	0.03%	0.003%
39	6.568	896	899	902	rVB2	168	222	0.04%	0.005%
40	6.763	922	931	949	rBV	173246	417016	75.69%	8.637%
41	7.123	981	990	1006	rBV	176219	386691	70.18%	8.009%
42	7.312	1013	1021	1038	rVB	110787	246489	44.74%	5.105%
43	7.440	1041	1042	1046	rVB	306	265	0.05%	0.005%
44	7.470	1046	1047	1051	rBV2	333	408	0.07%	0.008%
45	7.507	1051	1053	1056	rVB	209	217	0.04%	0.004%
46	7.586	1063	1066	1067	rBV	237	219	0.04%	0.005%
47	7.720	1086	1088	1092	rBV2	162	268	0.05%	0.006%
48	7.958	1123	1127	1129	rBV	217	284	0.05%	0.006%
49	7.982	1129	1131	1133	rBV	155	174	0.03%	0.004%
50	8.324	1181	1187	1205	rBV	63866	110813	20.11%	2.295%
51	8.647	1234	1240	1256	rVV	274607	434869	78.93%	9.007%
52	8.891	1278	1280	1284	rVB2	151	151	0.03%	0.003%
53	8.952	1285	1290	1305	rVV	47646	72127	13.09%	1.494%
54	9.275	1339	1343	1349	rVB4	1544	2209	0.40%	0.046%
55	9.348	1351	1355	1356	rBV	130	172	0.03%	0.004%
56	9.385	1356	1361	1378	rBV	178552	278004	50.46%	5.758%
57	9.616	1397	1399	1403	rVB2	179	236	0.04%	0.005%
58	9.708	1409	1414	1419	rVB2	1534	2210	0.40%	0.046%
59	9.799	1426	1429	1430	rBV2	139	149	0.03%	0.003%
60	9.958	1454	1455	1458	rBV2	144	158	0.03%	0.003%
61	10.055	1465	1471	1489	rBV	351222	477461	86.66%	9.889%
62	10.287	1506	1509	1510	rBV2	121	151	0.03%	0.003%
63	10.317	1510	1514	1520	rVV4	460	875	0.16%	0.018%
64	10.640	1564	1567	1573	rBV3	193	352	0.06%	0.007%
65	11.189	1652	1657	1668	rBV	224318	299933	54.44%	6.212%
66	11.311	1674	1677	1681	rVB2	568	723	0.13%	0.015%
67	11.646	1729	1732	1733	rBV	192	184	0.03%	0.004%
68	12.024	1788	1794	1804	rBV	337109	434374	78.84%	8.996%
69	12.207	1822	1824	1829	rVB2	142	170	0.03%	0.004%
70	12.256	1829	1832	1834	rVB	150	159	0.03%	0.003%
71	12.317	1837	1842	1854	rBV	312431	403732	73.27%	8.362%
72	12.463	1865	1866	1869	rBV	230	179	0.03%	0.004%
73	12.512	1873	1874	1876	rBV2	203	148	0.03%	0.003%
74	12.536	1876	1878	1881	rVB2	163	169	0.03%	0.004%
75	12.628	1890	1893	1894	rBV	150	146	0.03%	0.003%
76	12.768	1909	1916	1919	rBV4	925	1528	0.28%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042517.D
 Acq On : 24 Jul 2024 15:04
 Operator : JC/MD
 Sample : P3327-25 400X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	12.945	1943	1945	1947	rVB	226	168	0.03%	0.003%
78	12.975	1947	1950	1952	rBV	176	216	0.04%	0.004%
79	13.091	1966	1969	1970	rBV2	166	178	0.03%	0.004%
80	13.792	2082	2084	2088	rVV2	232	280	0.05%	0.006%
81	13.865	2094	2096	2101	rBV2	136	173	0.03%	0.004%
82	13.969	2109	2113	2115	rVB	163	174	0.03%	0.004%
83	14.128	2133	2139	2145	rBV4	1184	2006	0.36%	0.042%
84	14.237	2156	2157	2160	rBV2	238	220	0.04%	0.005%
85	14.310	2162	2169	2170	rBV3	222	413	0.07%	0.009%
86	14.725	2235	2237	2240	rVB3	263	161	0.03%	0.003%
87	14.926	2269	2270	2272	rBV2	212	191	0.03%	0.004%
88	15.085	2293	2296	2298	rBV3	253	345	0.06%	0.007%
89	15.115	2298	2301	2302	rBV	176	185	0.03%	0.004%
90	15.243	2320	2322	2325	rVB4	206	247	0.04%	0.005%
91	15.286	2327	2329	2330	rBV	399	284	0.05%	0.006%
92	15.310	2330	2333	2334	rBV	187	204	0.04%	0.004%
93	15.390	2343	2346	2352	rVB	1340	1675	0.30%	0.035%
94	15.530	2366	2369	2371	rBV3	195	230	0.04%	0.005%
95	15.682	2392	2394	2395	rBV2	204	166	0.03%	0.003%
96	15.816	2414	2416	2419	rVB4	260	295	0.05%	0.006%
97	15.883	2426	2427	2429	rBV2	270	160	0.03%	0.003%
98	16.231	2482	2484	2486	rBV2	226	158	0.03%	0.003%
99	16.267	2488	2490	2492	rBV	338	316	0.06%	0.007%
100	16.737	2566	2567	2569	rBV	347	221	0.04%	0.005%




Sum of corrected areas: 4828355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042517.D
Acq On : 24 Jul 2024 15:04
Operator : JC/MD
Sample : P3327-25 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

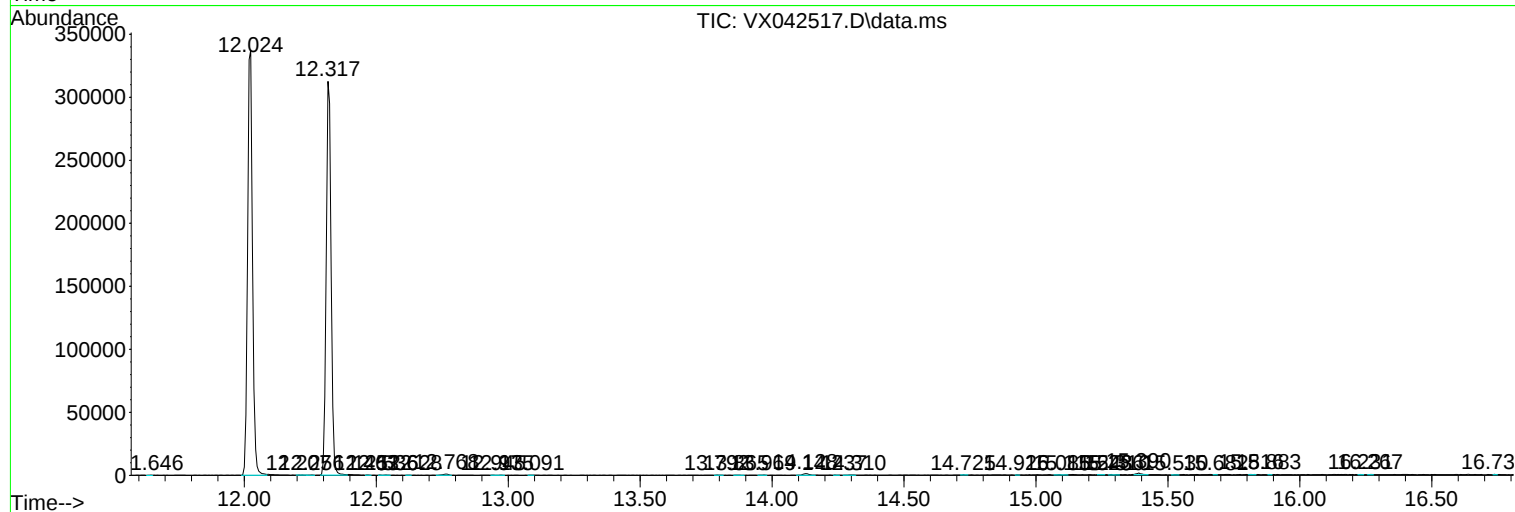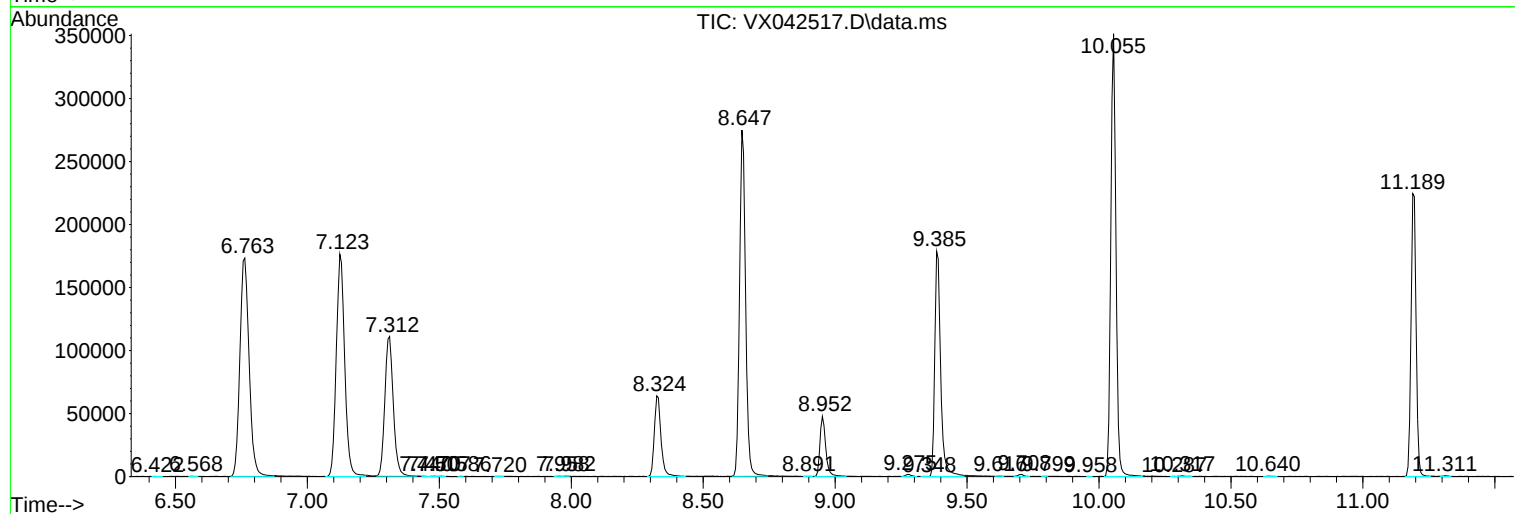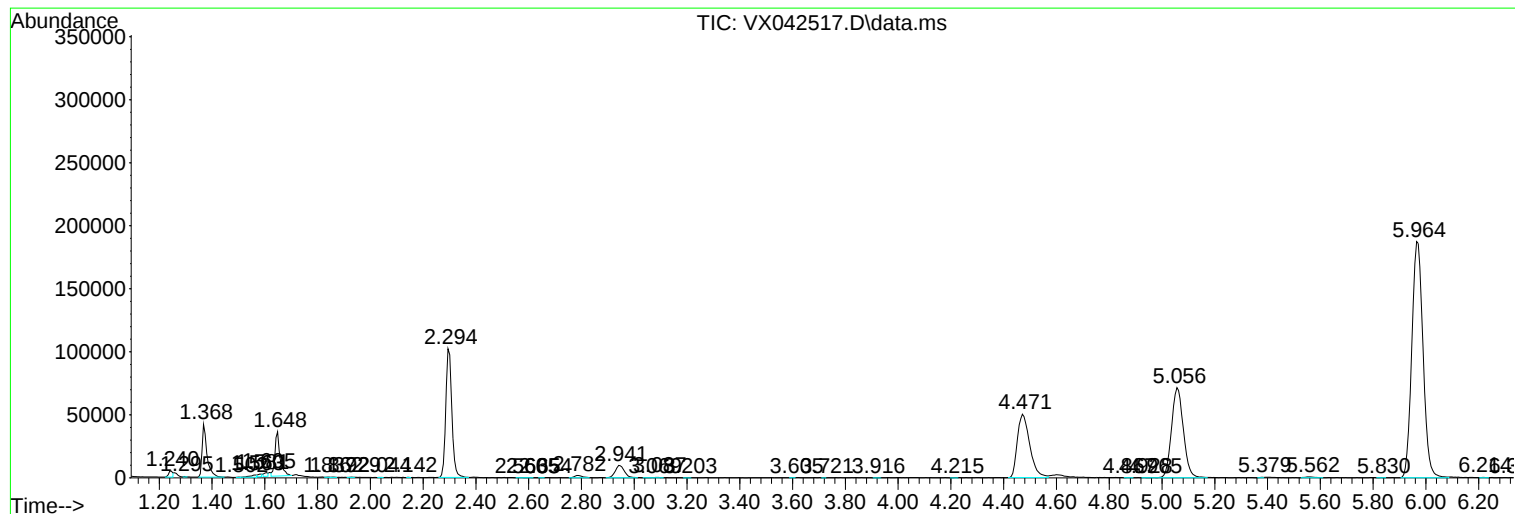

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042517.D
Acq On : 24 Jul 2024 15:04
Operator : JC/MD
Sample : P3327-25 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042517.D
Acq On : 24 Jul 2024 15:04
Operator : JC/MD
Sample : P3327-25 400X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc