

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042518.D
 Acq On : 24 Jul 2024 15:27
 Operator : JC/MD
 Sample : P3327-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	20	rVB	9748	13886	2.49%	0.307%
2	1.240	22	25	27	rBV	5347	6110	1.09%	0.135%
3	1.264	27	29	34	rVB2	6910	7134	1.28%	0.158%
4	1.368	42	46	57	rBV	45067	56935	10.19%	1.259%
5	1.447	57	59	65	rVB3	1295	1639	0.29%	0.036%
6	1.648	88	92	101	rVB	31729	44019	7.88%	0.973%
7	1.721	101	104	114	rVB5	5504	9040	1.62%	0.200%
8	1.941	135	140	143	rVB2	1863	2451	0.44%	0.054%
9	2.294	192	198	209	rBV	102594	159847	28.62%	3.534%
10	2.392	210	214	216	rBV	1568	2377	0.43%	0.053%
11	2.563	239	242	247	rBV2	368	694	0.12%	0.015%
12	2.642	253	255	256	rBV	117	80	0.01%	0.002%
13	2.697	262	264	265	rBV2	116	93	0.02%	0.002%
14	2.794	273	280	281	rBV4	742	1337	0.24%	0.030%
15	2.941	297	304	311	rBV	1268	3008	0.54%	0.066%
16	3.014	314	316	317	rBV2	103	94	0.02%	0.002%
17	3.093	324	329	334	rBV4	733	1480	0.26%	0.033%
18	3.264	355	357	359	rBV	88	81	0.01%	0.002%
19	3.288	359	361	363	rBV	178	149	0.03%	0.003%
20	3.361	372	373	374	rBV	152	82	0.01%	0.002%
21	3.380	374	376	378	rVB2	145	90	0.02%	0.002%
22	3.441	383	386	390	rBV3	469	673	0.12%	0.015%
23	3.648	419	420	423	rVB	159	143	0.03%	0.003%
24	3.684	425	426	429	rVV2	139	121	0.02%	0.003%
25	3.727	431	433	435	rBV2	102	116	0.02%	0.003%
26	3.800	442	445	448	rBV2	134	195	0.03%	0.004%
27	3.837	448	451	452	rVB2	146	133	0.02%	0.003%
28	3.892	458	460	462	rBV2	115	136	0.02%	0.003%
29	3.971	469	473	474	rBV	175	236	0.04%	0.005%
30	4.105	492	495	497	rBV2	136	179	0.03%	0.004%
31	4.136	497	500	503	rVV2	101	161	0.03%	0.004%
32	4.264	518	521	522	rBV	122	138	0.02%	0.003%
33	4.294	524	526	532	rVB3	551	798	0.14%	0.018%
34	4.349	532	535	537	rBV	159	183	0.03%	0.004%
35	4.465	546	554	572	rBV	46298	147872	26.47%	3.269%
36	5.056	639	651	667	rBV	73195	223371	39.99%	4.938%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042518.D
 Acq On : 24 Jul 2024 15:27
 Operator : JC/MD
 Sample : P3327-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.391	701	706	708	rBV3	358	618	0.11%	0.014%
38	5.458	714	717	725	rVB4	504	1082	0.19%	0.024%
39	5.556	728	733	744	rVB3	539	1325	0.24%	0.029%
40	5.678	751	753	755	rBV2	119	138	0.02%	0.003%
41	5.739	761	763	765	rBV2	100	134	0.02%	0.003%
42	5.964	789	800	819	rBV2	187013	558575	100.00%	12.348%
43	6.220	840	842	843	rVB	209	126	0.02%	0.003%
44	6.239	843	845	846	rBV	143	115	0.02%	0.003%
45	6.312	855	857	859	rBV2	96	87	0.02%	0.002%
46	6.361	864	865	867	rVB	330	190	0.03%	0.004%
47	6.763	922	931	946	rBV	171418	418715	74.96%	9.256%
48	7.056	977	979	980	rBV	150	131	0.02%	0.003%
49	7.129	984	991	1003	rBV	29660	68675	12.29%	1.518%
50	7.306	1012	1020	1037	rBV	113031	255239	45.69%	5.642%
51	7.482	1047	1049	1051	rBV2	193	194	0.03%	0.004%
52	7.562	1060	1062	1063	rBV	151	134	0.02%	0.003%
53	7.617	1070	1071	1074	rBV2	108	96	0.02%	0.002%
54	7.720	1085	1088	1090	rBV2	101	119	0.02%	0.003%
55	7.830	1103	1106	1108	rBV	200	216	0.04%	0.005%
56	7.873	1111	1113	1115	rBV2	90	80	0.01%	0.002%
57	7.958	1122	1127	1131	rBV4	387	721	0.13%	0.016%
58	8.324	1182	1187	1203	rBV	64689	112740	20.18%	2.492%
59	8.598	1229	1232	1234	rVB	178	169	0.03%	0.004%
60	8.647	1234	1240	1249	rBV	271518	430568	77.08%	9.518%
61	8.952	1285	1290	1301	rBV	48698	73423	13.14%	1.623%
62	9.061	1306	1308	1311	rVB2	321	337	0.06%	0.007%
63	9.092	1311	1313	1314	rVB	207	120	0.02%	0.003%
64	9.104	1314	1315	1316	rBV	102	73	0.01%	0.002%
65	9.275	1340	1343	1347	rBV4	1663	2410	0.43%	0.053%
66	9.385	1356	1361	1378	rBV	189362	284055	50.85%	6.279%
67	9.830	1432	1434	1435	rBV	107	81	0.01%	0.002%
68	10.055	1465	1471	1490	rBV	352027	476176	85.25%	10.527%
69	10.201	1492	1495	1499	rVB2	853	1083	0.19%	0.024%
70	10.305	1508	1512	1519	rVB	1706	2465	0.44%	0.054%
71	10.390	1524	1526	1527	rBV	157	107	0.02%	0.002%
72	10.506	1543	1545	1547	rBV2	129	135	0.02%	0.003%
73	10.647	1564	1568	1576	rVB3	849	1262	0.23%	0.028%
74	10.781	1587	1590	1595	rBV	261	449	0.08%	0.010%
75	11.189	1652	1657	1665	rBV	234898	306698	54.91%	6.780%
76	11.317	1674	1678	1683	rVB2	492	768	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042518.D
 Acq On : 24 Jul 2024 15:27
 Operator : JC/MD
 Sample : P3327-29
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.378	1687	1688	1690	rBV2	132	113	0.02%	0.002%
78	11.457	1698	1701	1704	rBV2	396	392	0.07%	0.009%
79	11.756	1746	1750	1756	rVB2	707	1162	0.21%	0.026%
80	11.872	1767	1769	1770	rBV	123	85	0.02%	0.002%
81	11.969	1784	1785	1788	rBV2	176	146	0.03%	0.003%
82	12.024	1788	1794	1803	rBV	326463	425004	76.09%	9.395%
83	12.219	1821	1826	1837	rBV	9602	14224	2.55%	0.314%
84	12.317	1837	1842	1858	rVV	297850	393061	70.37%	8.689%
85	12.530	1876	1877	1879	rVB	159	76	0.01%	0.002%
86	12.597	1886	1888	1890	rBV	142	177	0.03%	0.004%
87	12.671	1898	1900	1901	rBV	116	91	0.02%	0.002%
88	12.707	1903	1906	1910	rVV	136	237	0.04%	0.005%
89	12.768	1911	1916	1921	rVV3	862	1351	0.24%	0.030%
90	12.829	1924	1926	1928	rVV2	126	116	0.02%	0.003%
91	12.866	1930	1932	1933	rBV	158	114	0.02%	0.003%
92	13.049	1960	1962	1968	rBV	127	181	0.03%	0.004%
93	13.189	1982	1985	1988	rBV2	173	249	0.04%	0.006%
94	13.713	2069	2071	2074	rBV2	102	96	0.02%	0.002%
95	13.780	2080	2082	2083	rBV	242	124	0.02%	0.003%
96	13.993	2115	2117	2118	rBV	113	86	0.02%	0.002%
97	14.073	2128	2130	2134	rVB2	139	146	0.03%	0.003%
98	14.128	2134	2139	2143	rBV	888	1217	0.22%	0.027%
99	14.292	2165	2166	2167	rBV	177	98	0.02%	0.002%
100	14.530	2203	2205	2206	rBV	185	87	0.02%	0.002%

Sum of corrected areas: 4523543




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042518.D
Acq On : 24 Jul 2024 15:27
Operator : JC/MD
Sample : P3327-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

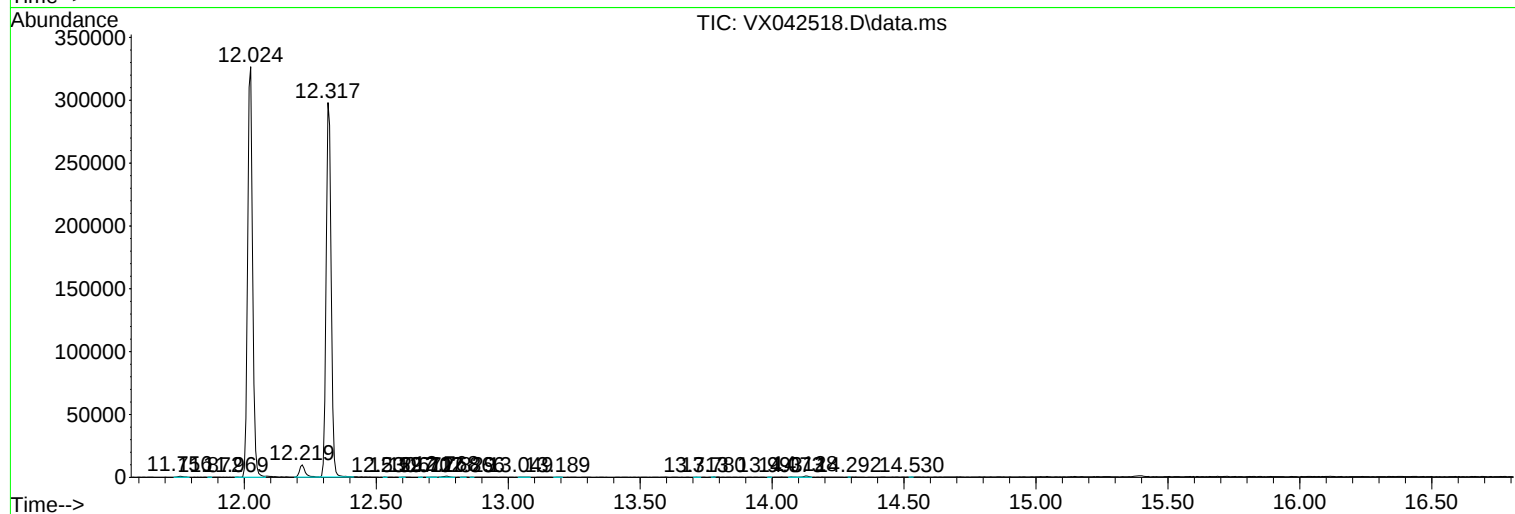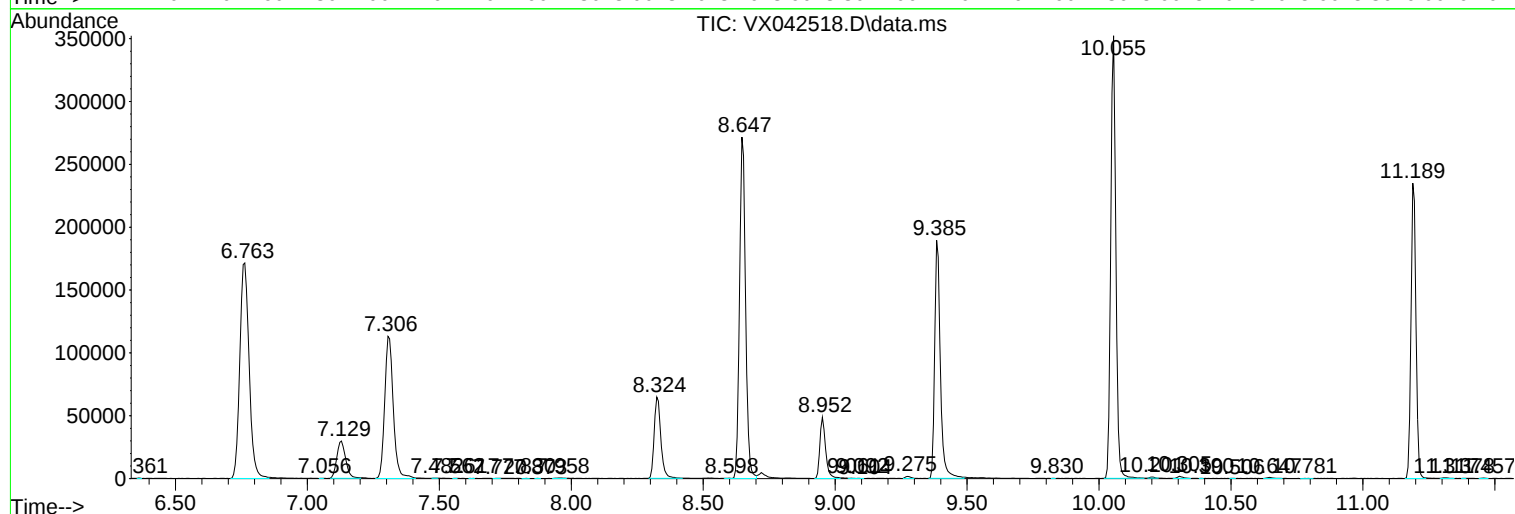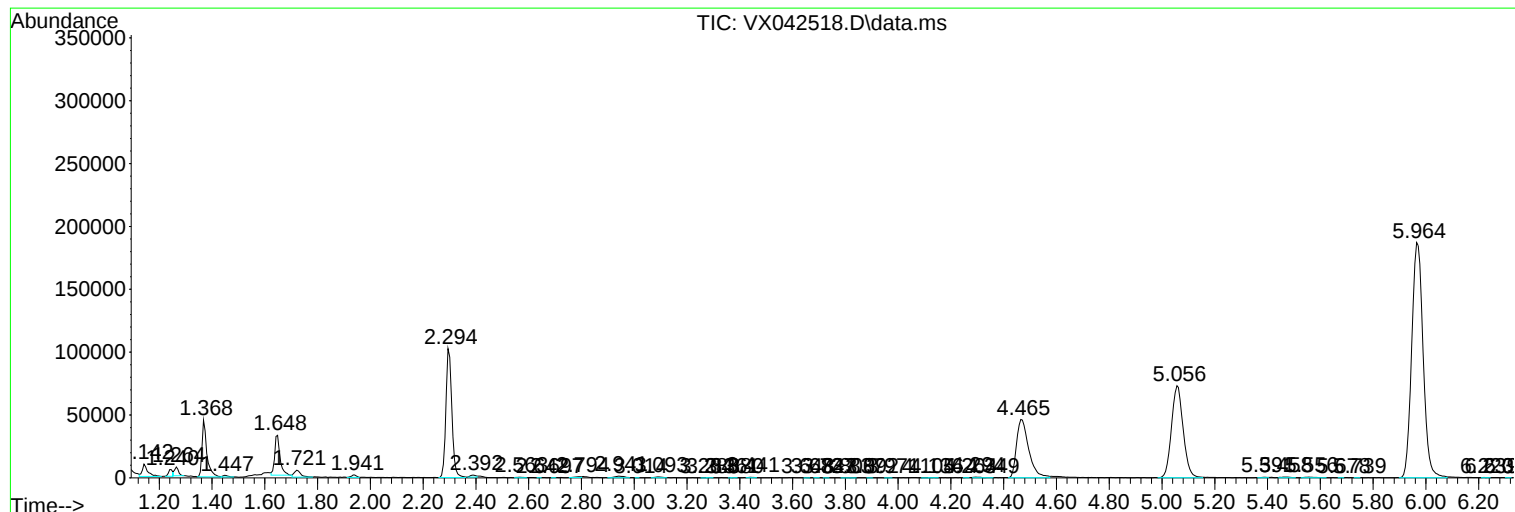

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042518.D
Acq On : 24 Jul 2024 15:27
Operator : JC/MD
Sample : P3327-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042518.D
Acq On : 24 Jul 2024 15:27
Operator : JC/MD
Sample : P3327-29
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc