

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042519.D
 Acq On : 24 Jul 2024 15:51
 Operator : JC/MD
 Sample : P3327-32
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	27	rBV	4913	5074	0.83%	0.103%
2	1.368	42	46	57	rBV	46850	59788	9.76%	1.219%
3	1.453	57	60	66	rVB	1430	1657	0.27%	0.034%
4	1.648	88	92	100	rVB	35973	49995	8.16%	1.020%
5	2.056	157	159	162	rBV2	274	308	0.05%	0.006%
6	2.300	192	199	209	rBV	110889	179054	29.24%	3.652%
7	2.386	209	213	222	rVB	3164	5601	0.91%	0.114%
8	2.508	227	233	235	rBV	294	462	0.08%	0.009%
9	2.562	237	242	251	rVB2	1331	2465	0.40%	0.050%
10	2.672	259	260	263	rBV	160	149	0.02%	0.003%
11	2.715	265	267	270	rVB2	274	300	0.05%	0.006%
12	2.788	274	279	286	rBV2	858	1624	0.27%	0.033%
13	2.873	290	293	295	rVB	102	138	0.02%	0.003%
14	2.934	295	303	312	rBV	2379	5616	0.92%	0.115%
15	3.032	318	319	322	rBV2	182	162	0.03%	0.003%
16	3.093	322	329	331	rBV4	383	639	0.10%	0.013%
17	3.136	335	336	337	rBV	185	84	0.01%	0.002%
18	3.245	353	354	356	rBV	85	83	0.01%	0.002%
19	3.270	356	358	363	rVB	94	130	0.02%	0.003%
20	3.343	364	370	373	rBV2	266	465	0.08%	0.009%
21	3.428	382	384	385	rVB	177	93	0.02%	0.002%
22	3.459	385	389	391	rBV2	143	184	0.03%	0.004%
23	3.477	391	392	396	rVB	167	151	0.02%	0.003%
24	3.526	398	400	402	rBV	77	86	0.01%	0.002%
25	3.581	407	409	412	rBV2	139	170	0.03%	0.003%
26	3.654	416	421	423	rBV	141	204	0.03%	0.004%
27	3.696	425	428	429	rBV	159	157	0.03%	0.003%
28	3.751	436	437	442	rVB	185	182	0.03%	0.004%
29	3.794	442	444	445	rVB	119	76	0.01%	0.002%
30	3.806	445	446	448	rBV	132	133	0.02%	0.003%
31	4.209	509	512	514	rBV	108	161	0.03%	0.003%
32	4.410	543	545	546	rBV	167	125	0.02%	0.003%
33	4.465	546	554	572	rBV	51378	164038	26.79%	3.346%
34	4.830	612	614	616	rBV2	174	131	0.02%	0.003%
35	5.056	639	651	680	rVB	79577	248892	40.65%	5.076%
36	5.251	681	683	685	rVB	146	87	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042519.D
 Acq On : 24 Jul 2024 15:51
 Operator : JC/MD
 Sample : P3327-32
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.318	691	694	695	rBV2	110	114	0.02%	0.002%
38	5.397	701	707	709	rBV3	245	497	0.08%	0.010%
39	5.550	728	732	734	rBV3	292	336	0.05%	0.007%
40	5.769	766	768	769	rBV	117	99	0.02%	0.002%
41	5.970	789	801	820	rBV2	207493	612355	100.00%	12.489%
42	6.312	855	857	858	rBV	208	169	0.03%	0.003%
43	6.458	879	881	883	rBV	117	85	0.01%	0.002%
44	6.690	917	919	921	rVB2	131	97	0.02%	0.002%
45	6.763	921	931	948	rBV	197844	478733	78.18%	9.764%
46	7.129	983	991	1002	rVB3	6860	16917	2.76%	0.345%
47	7.214	1002	1005	1010	rVB3	381	642	0.10%	0.013%
48	7.251	1010	1011	1012	rBV	153	102	0.02%	0.002%
49	7.312	1012	1021	1035	rBV	124249	277851	45.37%	5.667%
50	7.488	1048	1050	1056	rVB	239	330	0.05%	0.007%
51	7.824	1103	1105	1106	rBV	135	91	0.01%	0.002%
52	7.879	1112	1114	1115	rBB	132	64	0.01%	0.001%
53	7.952	1123	1126	1130	rBV2	497	781	0.13%	0.016%
54	8.147	1157	1158	1160	rBV	130	121	0.02%	0.002%
55	8.226	1170	1171	1174	rBV2	151	184	0.03%	0.004%
56	8.324	1181	1187	1201	rBV	71858	121569	19.85%	2.479%
57	8.513	1214	1218	1222	rBV4	515	732	0.12%	0.015%
58	8.647	1234	1240	1257	rBV	294874	473868	77.38%	9.665%
59	8.891	1279	1280	1282	rBV	200	155	0.03%	0.003%
60	8.952	1285	1290	1308	rVV	53667	79996	13.06%	1.632%
61	9.275	1339	1343	1349	rVB4	1944	2853	0.47%	0.058%
62	9.384	1356	1361	1381	rBV	210178	314010	51.28%	6.404%
63	9.701	1409	1413	1418	rBV4	484	664	0.11%	0.014%
64	10.055	1465	1471	1481	rBV	393459	535437	87.44%	10.920%
65	10.201	1493	1495	1498	rVB3	374	311	0.05%	0.006%
66	10.311	1509	1513	1521	rVB3	410	717	0.12%	0.015%
67	10.366	1521	1522	1525	rVB	257	193	0.03%	0.004%
68	10.390	1525	1526	1527	rBV	161	99	0.02%	0.002%
69	10.549	1550	1552	1553	rBV	146	90	0.01%	0.002%
70	10.646	1564	1568	1570	rBV2	354	501	0.08%	0.010%
71	10.695	1574	1576	1577	rBV2	129	116	0.02%	0.002%
72	10.848	1599	1601	1603	rVB	113	82	0.01%	0.002%
73	10.970	1618	1621	1622	rBV2	130	123	0.02%	0.003%
74	11.091	1640	1641	1642	rBV	159	68	0.01%	0.001%
75	11.189	1652	1657	1667	rBV	256611	336636	54.97%	6.866%
76	11.311	1674	1677	1683	rVB3	495	833	0.14%	0.017%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042519.D
 Acq On : 24 Jul 2024 15:51
 Operator : JC/MD
 Sample : P3327-32
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.457	1697	1701	1704	rVB2	224	299	0.05%	0.006%
78	11.506	1704	1709	1712	rBV2	202	370	0.06%	0.008%
79	11.756	1748	1750	1753	rBV	206	177	0.03%	0.004%
80	11.811	1758	1759	1761	rBV	98	99	0.02%	0.002%
81	11.890	1770	1772	1777	rBV	188	320	0.05%	0.007%
82	11.975	1784	1786	1788	rVB	194	173	0.03%	0.004%
83	12.024	1788	1794	1804	rBV	369233	477761	78.02%	9.744%
84	12.219	1823	1826	1834	rVB4	1695	2547	0.42%	0.052%
85	12.280	1834	1836	1837	rBV	158	155	0.03%	0.003%
86	12.317	1837	1842	1855	rBV	337253	429488	70.14%	8.759%
87	12.579	1883	1885	1886	rBV	92	71	0.01%	0.001%
88	12.768	1911	1916	1919	rVB2	880	1241	0.20%	0.025%
89	12.939	1942	1944	1945	rBV	97	68	0.01%	0.001%
90	12.969	1947	1949	1950	rBV	87	61	0.01%	0.001%
91	13.128	1972	1975	1977	rBV2	109	170	0.03%	0.003%
92	13.390	2016	2018	2019	rBV	137	74	0.01%	0.002%
93	13.597	2050	2052	2054	rVB	162	89	0.01%	0.002%
94	13.786	2081	2083	2084	rBV	338	228	0.04%	0.005%
95	13.817	2087	2088	2090	rBV	180	93	0.02%	0.002%
96	14.127	2136	2139	2145	rBV	1412	1741	0.28%	0.036%
97	14.414	2182	2186	2187	rBV2	188	262	0.04%	0.005%
98	14.463	2193	2194	2195	rVB	174	64	0.01%	0.001%
99	14.633	2221	2222	2223	rVB	210	77	0.01%	0.002%
100	14.755	2239	2242	2244	rBV2	277	253	0.04%	0.005%

Sum of corrected areas: 4903166




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042519.D
Acq On : 24 Jul 2024 15:51
Operator : JC/MD
Sample : P3327-32
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

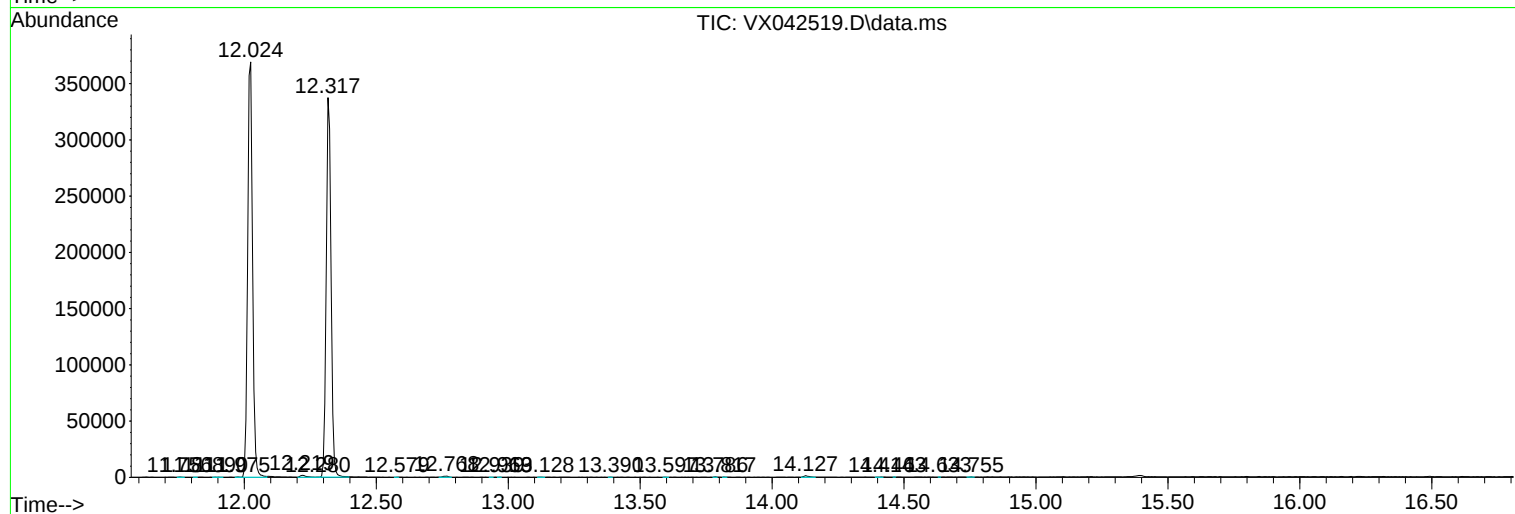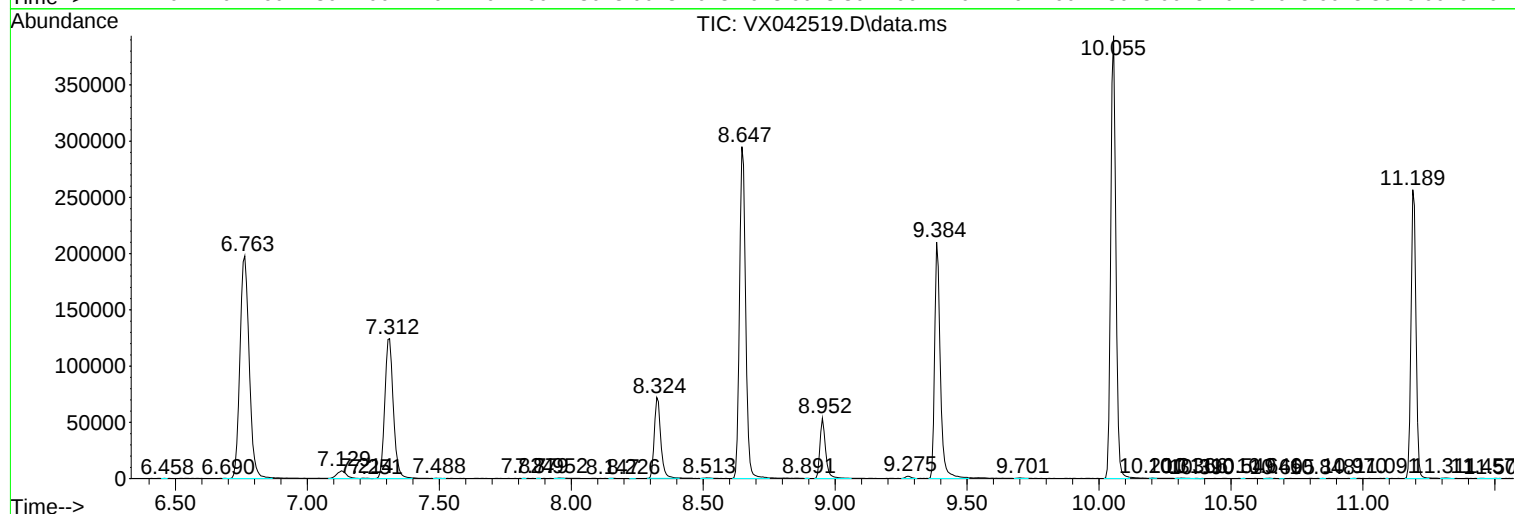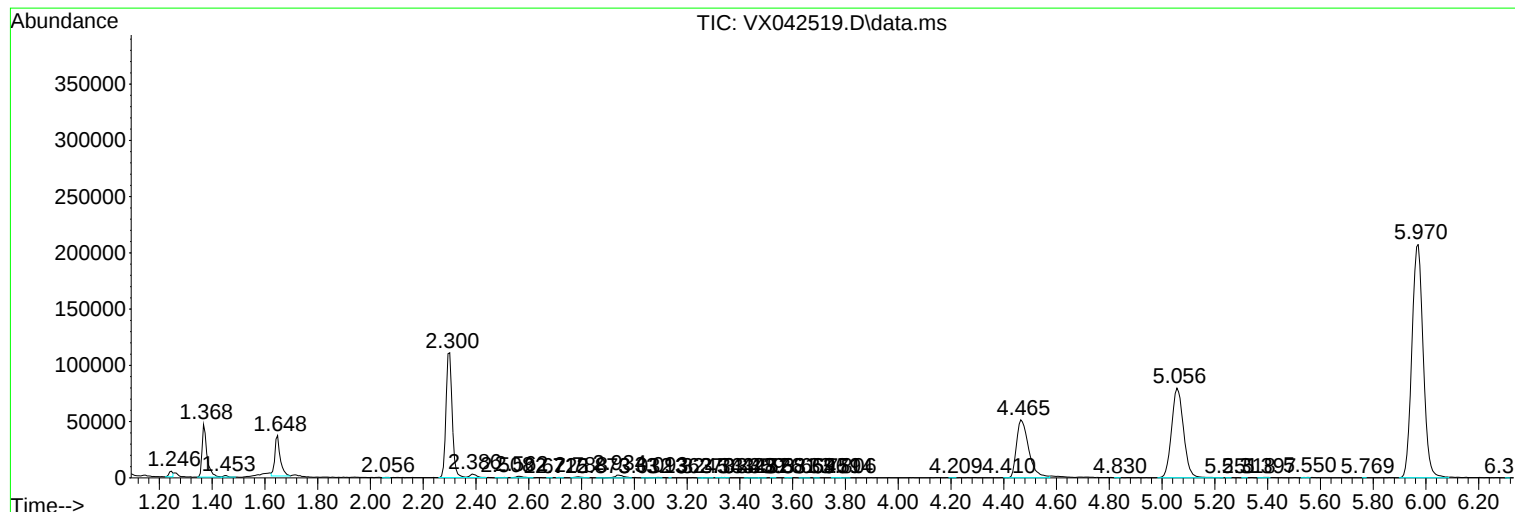

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042519.D
Acq On : 24 Jul 2024 15:51
Operator : JC/MD
Sample : P3327-32
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042519.D
Acq On : 24 Jul 2024 15:51
Operator : JC/MD
Sample : P3327-32
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc