

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042521.D
 Acq On : 24 Jul 2024 16:37
 Operator : JC/MD
 Sample : P3327-30
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	20	rVB	6558	9661	1.73%	0.217%
2	1.240	22	25	27	rBV2	5343	5794	1.04%	0.130%
3	1.368	43	46	57	rVV	44262	53453	9.60%	1.203%
4	1.453	57	60	64	rVB	1322	1403	0.25%	0.032%
5	1.648	88	92	100	rVB	34578	45467	8.16%	1.023%
6	2.294	192	198	209	rBV	97919	156871	28.17%	3.529%
7	2.392	210	214	216	rBV	1862	2839	0.51%	0.064%
8	2.477	226	228	230	rBV	79	57	0.01%	0.001%
9	2.502	230	232	235	rBV2	190	219	0.04%	0.005%
10	2.569	240	243	248	rVB	528	704	0.13%	0.016%
11	2.709	264	266	269	rBV2	145	124	0.02%	0.003%
12	2.782	275	278	286	rBV4	663	1284	0.23%	0.029%
13	2.941	298	304	311	rBV	2455	5515	0.99%	0.124%
14	3.087	326	328	331	rBV	207	213	0.04%	0.005%
15	3.209	344	348	350	rBV	127	181	0.03%	0.004%
16	3.306	363	364	365	rBV	109	53	0.01%	0.001%
17	3.343	365	370	376	rVV2	374	619	0.11%	0.014%
18	3.392	376	378	380	rVB	195	125	0.02%	0.003%
19	3.428	380	384	386	rBV	170	256	0.05%	0.006%
20	3.501	393	396	398	rVB2	147	155	0.03%	0.003%
21	3.538	398	402	403	rBV2	118	151	0.03%	0.003%
22	3.562	404	406	407	rVB	169	108	0.02%	0.002%
23	3.575	407	408	409	rBV	140	90	0.02%	0.002%
24	3.593	409	411	413	rBV2	250	219	0.04%	0.005%
25	3.660	420	422	424	rVB	93	78	0.01%	0.002%
26	3.678	424	425	427	rBV2	128	105	0.02%	0.002%
27	3.751	434	437	438	rBV2	115	105	0.02%	0.002%
28	3.818	445	448	449	rBV2	97	101	0.02%	0.002%
29	3.831	449	450	451	rVB	140	53	0.01%	0.001%
30	3.989	473	476	477	rBV2	153	147	0.03%	0.003%
31	4.032	481	483	485	rVB	142	98	0.02%	0.002%
32	4.099	492	494	496	rBV	135	89	0.02%	0.002%
33	4.172	505	506	508	rVB	139	70	0.01%	0.002%
34	4.221	512	514	518	rVV2	104	129	0.02%	0.003%
35	4.337	531	533	536	rBV2	115	115	0.02%	0.003%
36	4.465	546	554	572	rBV	46064	144307	25.91%	3.247%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042521.D
 Acq On : 24 Jul 2024 16:37
 Operator : JC/MD
 Sample : P3327-30
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	4.824	611	613	614	rBV	109	71	0.01%	0.002%
38	4.879	620	622	623	rVB	147	78	0.01%	0.002%
39	5.056	639	651	673	rBV	71895	223995	40.22%	5.040%
40	5.233	678	680	681	rBV	173	140	0.03%	0.003%
41	5.288	686	689	690	rBV	104	85	0.02%	0.002%
42	5.471	714	719	723	rBV2	233	421	0.08%	0.009%
43	5.727	757	761	762	rBV	133	184	0.03%	0.004%
44	5.818	774	776	777	rBV	94	55	0.01%	0.001%
45	5.836	777	779	780	rVB	188	109	0.02%	0.002%
46	5.855	780	782	786	rBV2	130	221	0.04%	0.005%
47	5.964	789	800	822	rBV2	186959	556969	100.00%	12.531%
48	6.422	874	875	878	rBV	107	78	0.01%	0.002%
49	6.574	898	900	902	rBV	72	63	0.01%	0.001%
50	6.763	921	931	948	rBV	178956	437047	78.47%	9.833%
51	6.989	966	968	969	rBV	185	194	0.03%	0.004%
52	7.129	984	991	1000	rBV4	9803	24074	4.32%	0.542%
53	7.312	1012	1021	1037	rVB	112832	252753	45.38%	5.687%
54	7.617	1069	1071	1073	rVB	158	106	0.02%	0.002%
55	7.958	1122	1127	1129	rBV2	318	501	0.09%	0.011%
56	8.123	1153	1154	1155	rBV	153	87	0.02%	0.002%
57	8.141	1155	1157	1158	rVV	154	98	0.02%	0.002%
58	8.165	1158	1161	1162	rVV2	121	132	0.02%	0.003%
59	8.324	1181	1187	1196	rBV	63789	109279	19.62%	2.459%
60	8.580	1228	1229	1234	rBV	200	176	0.03%	0.004%
61	8.647	1234	1240	1250	rBV	265722	422478	75.85%	9.505%
62	8.952	1285	1290	1300	rBV2	47351	70133	12.59%	1.578%
63	9.196	1327	1330	1331	rBV2	86	73	0.01%	0.002%
64	9.275	1339	1343	1349	rVB4	1948	2990	0.54%	0.067%
65	9.385	1356	1361	1374	rBV	185540	280655	50.39%	6.314%
66	10.055	1465	1471	1484	rBV	362996	491163	88.18%	11.050%
67	10.208	1492	1496	1500	rVB3	582	990	0.18%	0.022%
68	10.250	1500	1503	1505	rBV3	146	223	0.04%	0.005%
69	10.305	1508	1512	1520	rVB2	691	1301	0.23%	0.029%
70	10.384	1523	1525	1527	rVB2	147	82	0.01%	0.002%
71	10.647	1565	1568	1573	rVB2	432	605	0.11%	0.014%
72	10.768	1583	1588	1589	rBV	135	194	0.03%	0.004%
73	10.787	1589	1591	1593	rVV2	163	140	0.03%	0.003%
74	10.829	1596	1598	1599	rVB	135	80	0.01%	0.002%
75	10.884	1605	1607	1608	rBV	109	71	0.01%	0.002%
76	10.903	1608	1610	1614	rVB2	160	207	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042521.D
 Acq On : 24 Jul 2024 16:37
 Operator : JC/MD
 Sample : P3327-30
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.000	1624	1626	1629	rBV2	112	123	0.02%	0.003%
78	11.189	1652	1657	1668	rBV	231575	305255	54.81%	6.868%
79	11.305	1674	1676	1682	rBV4	413	714	0.13%	0.016%
80	11.457	1698	1701	1704	rBV3	210	299	0.05%	0.007%
81	11.494	1706	1707	1710	rVB	131	63	0.01%	0.001%
82	11.518	1710	1711	1715	rBV	113	84	0.02%	0.002%
83	11.707	1740	1742	1744	rBV2	131	122	0.02%	0.003%
84	11.762	1747	1751	1755	rBB3	326	503	0.09%	0.011%
85	11.793	1755	1756	1758	rBV2	93	82	0.01%	0.002%
86	11.982	1783	1787	1788	rBV2	175	196	0.04%	0.004%
87	12.024	1788	1794	1808	rBV	330703	430554	77.30%	9.687%
88	12.219	1822	1826	1837	rBV	7352	10366	1.86%	0.233%
89	12.317	1837	1842	1852	rBV	292642	382981	68.76%	8.616%
90	12.762	1912	1915	1919	rBV3	866	1000	0.18%	0.022%
91	12.866	1930	1932	1934	rVB	119	69	0.01%	0.002%
92	13.597	2050	2052	2054	rBV	194	250	0.04%	0.006%
93	13.780	2081	2082	2084	rBV	194	152	0.03%	0.003%
94	13.847	2091	2093	2097	rVB2	178	151	0.03%	0.003%
95	13.914	2100	2104	2107	rVB2	180	258	0.05%	0.006%
96	14.006	2117	2119	2120	rBV	245	133	0.02%	0.003%
97	14.024	2120	2122	2128	rVB3	192	363	0.07%	0.008%
98	14.073	2128	2130	2133	rBV2	179	222	0.04%	0.005%
99	14.128	2135	2139	2144	rVB2	1053	1380	0.25%	0.031%
100	14.292	2164	2166	2168	rBV	313	203	0.04%	0.005%

Sum of corrected areas: 4444782




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042521.D
Acq On : 24 Jul 2024 16:37
Operator : JC/MD
Sample : P3327-30
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

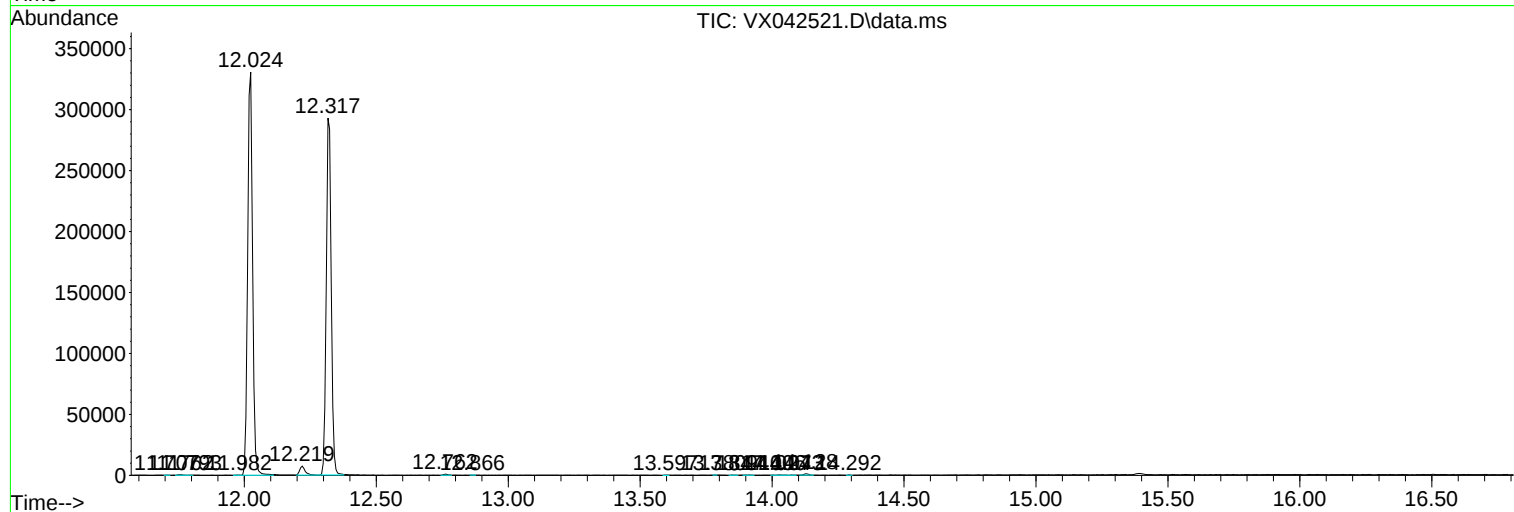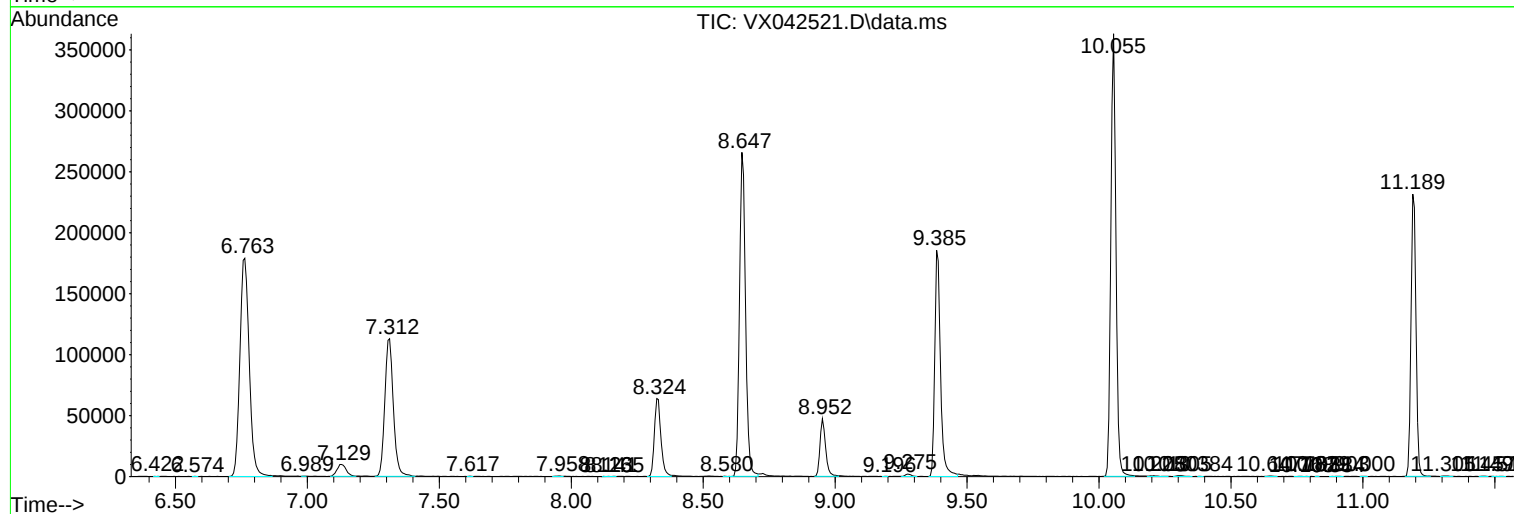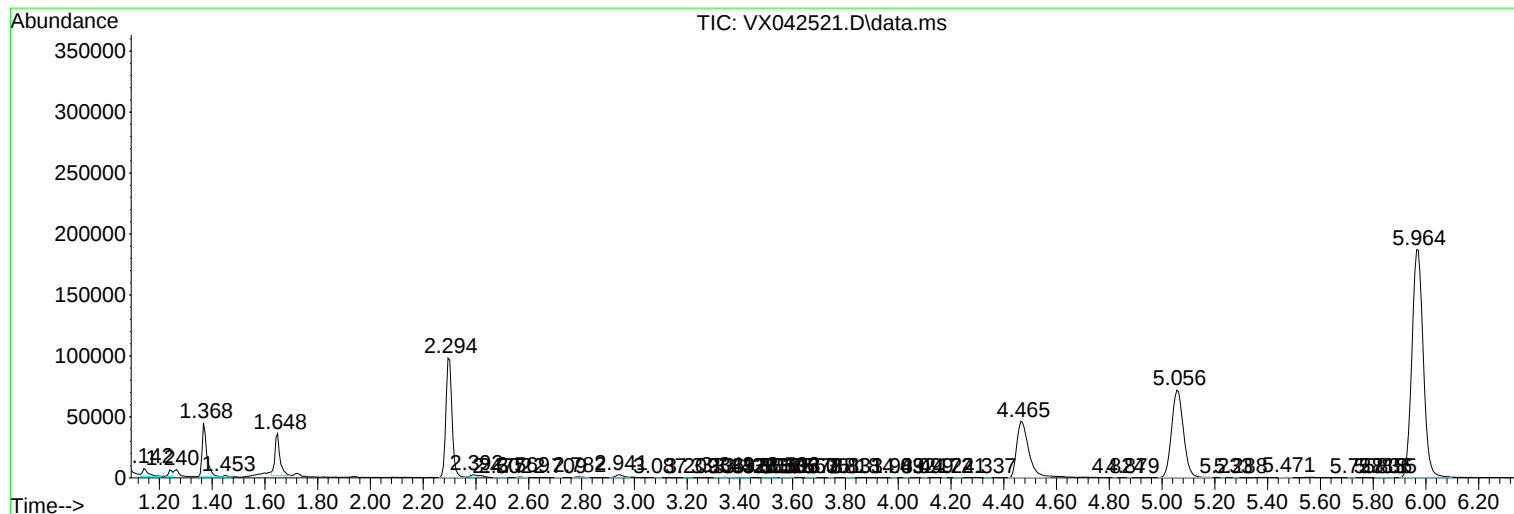

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042521.D
Acq On : 24 Jul 2024 16:37
Operator : JC/MD
Sample : P3327-30
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042521.D
Acq On : 24 Jul 2024 16:37
Operator : JC/MD
Sample : P3327-30
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------