

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042522.D
 Acq On : 24 Jul 2024 17:00
 Operator : JC/MD
 Sample : P3334-01 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	27	rBV	4890	5491	1.03%	0.127%
2	1.368	43	46	58	rVB	39819	51271	9.62%	1.188%
3	1.617	70	87	88	rBV5	4314	13920	2.61%	0.323%
4	1.648	88	92	102	rVB	34192	45188	8.48%	1.047%
5	2.105	165	167	170	rBV	257	184	0.03%	0.004%
6	2.294	192	198	211	rBV	96198	153561	28.80%	3.559%
7	2.465	224	226	229	rBV	125	108	0.02%	0.003%
8	2.501	230	232	235	rVB2	274	286	0.05%	0.007%
9	2.538	235	238	239	rBV	181	206	0.04%	0.005%
10	2.629	252	253	255	rBV	147	127	0.02%	0.003%
11	2.788	274	279	288	rVB2	2031	4351	0.82%	0.101%
12	2.861	290	291	293	rBV	160	90	0.02%	0.002%
13	2.879	293	294	297	rBV	130	124	0.02%	0.003%
14	2.940	297	304	315	rVB	8289	18483	3.47%	0.428%
15	3.050	321	322	325	rVB	87	82	0.02%	0.002%
16	3.075	325	326	327	rBV	110	76	0.01%	0.002%
17	3.209	345	348	350	rVB	138	131	0.02%	0.003%
18	3.239	352	353	354	rBV	119	74	0.01%	0.002%
19	3.294	360	362	366	rVB2	149	164	0.03%	0.004%
20	3.324	366	367	368	rBV	114	76	0.01%	0.002%
21	3.428	383	384	387	rBV2	126	130	0.02%	0.003%
22	3.513	396	398	403	rBV	193	276	0.05%	0.006%
23	3.556	403	405	407	rVB	148	124	0.02%	0.003%
24	3.666	421	423	426	rBV	178	209	0.04%	0.005%
25	3.751	436	437	440	rVB	134	117	0.02%	0.003%
26	3.788	440	443	444	rBV2	117	135	0.03%	0.003%
27	3.879	454	458	459	rBV	127	148	0.03%	0.003%
28	3.898	459	461	464	rBV2	84	136	0.03%	0.003%
29	4.111	495	496	499	rBV2	101	78	0.01%	0.002%
30	4.135	499	500	503	rVB	111	74	0.01%	0.002%
31	4.361	536	537	538	rBV	115	82	0.02%	0.002%
32	4.471	546	555	568	rBV	42170	124475	23.35%	2.885%
33	4.775	604	605	606	rBV	173	72	0.01%	0.002%
34	4.910	626	627	628	rVB	179	66	0.01%	0.002%
35	5.056	639	651	667	rBV	68878	213563	40.05%	4.949%
36	5.239	680	681	683	rVB	171	104	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042522.D
 Acq On : 24 Jul 2024 17:00
 Operator : JC/MD
 Sample : P3334-01 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.452	715	716	719	rBV2	111	101	0.02%	0.002%
38	5.562	729	734	735	rBV2	355	631	0.12%	0.015%
39	5.659	749	750	753	rVB	167	148	0.03%	0.003%
40	5.690	753	755	757	rBV2	158	199	0.04%	0.005%
41	5.763	766	767	769	rBV	139	98	0.02%	0.002%
42	5.964	790	800	822	rBV2	179550	533191	100.00%	12.356%
43	6.190	836	837	840	rVB2	194	180	0.03%	0.004%
44	6.671	914	916	918	rBV	114	126	0.02%	0.003%
45	6.763	922	931	952	rBV	174649	416215	78.06%	9.645%
46	7.129	984	991	1001	rVB7	4267	10647	2.00%	0.247%
47	7.202	1001	1003	1004	rBV	211	144	0.03%	0.003%
48	7.312	1013	1021	1034	rBV	108295	240209	45.05%	5.567%
49	7.470	1046	1047	1048	rBV	113	66	0.01%	0.002%
50	7.677	1079	1081	1084	rVB	112	114	0.02%	0.003%
51	7.793	1098	1100	1101	rBV	104	77	0.01%	0.002%
52	8.135	1154	1156	1159	rBV	130	123	0.02%	0.003%
53	8.202	1165	1167	1169	rVB2	160	95	0.02%	0.002%
54	8.257	1173	1176	1177	rBV	149	146	0.03%	0.003%
55	8.275	1177	1179	1181	rBV2	101	88	0.02%	0.002%
56	8.324	1181	1187	1202	rBV	59945	105497	19.79%	2.445%
57	8.519	1217	1219	1224	rVB2	270	295	0.06%	0.007%
58	8.580	1227	1229	1230	rBV	128	98	0.02%	0.002%
59	8.647	1234	1240	1257	rBV	256388	413134	77.48%	9.574%
60	8.952	1285	1290	1302	rBV	44387	67582	12.68%	1.566%
61	9.195	1327	1330	1331	rBV	125	139	0.03%	0.003%
62	9.275	1340	1343	1348	rVB2	1609	2295	0.43%	0.053%
63	9.384	1356	1361	1381	rBV	180323	280970	52.70%	6.511%
64	9.701	1409	1413	1418	rVB3	1283	2177	0.41%	0.050%
65	9.994	1459	1461	1463	rVB	121	81	0.02%	0.002%
66	10.055	1465	1471	1485	rBV	345264	477849	89.62%	11.074%
67	10.305	1509	1512	1518	rBV3	359	624	0.12%	0.014%
68	10.366	1521	1522	1525	rVV	163	147	0.03%	0.003%
69	10.415	1528	1530	1531	rVB	159	90	0.02%	0.002%
70	10.531	1547	1549	1552	rBV2	107	102	0.02%	0.002%
71	10.652	1566	1569	1573	rVB2	223	279	0.05%	0.006%
72	10.768	1585	1588	1590	rBV2	170	224	0.04%	0.005%
73	10.829	1594	1598	1599	rBV2	166	229	0.04%	0.005%
74	11.134	1646	1648	1652	rBV	140	99	0.02%	0.002%
75	11.189	1652	1657	1667	rVV	222147	299525	56.18%	6.941%
76	11.311	1675	1677	1682	rVB	543	567	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042522.D
 Acq On : 24 Jul 2024 17:00
 Operator : JC/MD
 Sample : P3334-01 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.366	1684	1686	1687	rVB	151	87	0.02%	0.002%
78	11.402	1687	1692	1694	rBV2	186	335	0.06%	0.008%
79	11.579	1719	1721	1723	rVB	113	122	0.02%	0.003%
80	11.597	1723	1724	1726	rBV	136	121	0.02%	0.003%
81	11.689	1736	1739	1741	rBV2	106	108	0.02%	0.003%
82	11.817	1758	1760	1762	rBV2	113	133	0.02%	0.003%
83	12.024	1788	1794	1806	rBV	327186	432087	81.04%	10.013%
84	12.250	1829	1831	1833	rBV	180	136	0.03%	0.003%
85	12.317	1837	1842	1852	rBV	297218	385971	72.39%	8.945%
86	12.518	1874	1875	1882	rVB2	248	226	0.04%	0.005%
87	12.768	1911	1916	1919	rVB2	943	1389	0.26%	0.032%
88	12.798	1919	1921	1924	rBV	123	140	0.03%	0.003%
89	12.829	1924	1926	1928	rVV	155	88	0.02%	0.002%
90	13.286	1998	2001	2003	rBV	114	153	0.03%	0.004%
91	13.371	2014	2015	2016	rBV	171	72	0.01%	0.002%
92	13.695	2064	2068	2070	rBV2	147	213	0.04%	0.005%
93	13.847	2091	2093	2096	rVB2	220	179	0.03%	0.004%
94	13.871	2096	2097	2100	rBV2	120	105	0.02%	0.002%
95	14.005	2117	2119	2121	rBV	99	69	0.01%	0.002%
96	14.134	2136	2140	2146	rVB2	1215	2049	0.38%	0.047%
97	14.213	2151	2153	2158	rBV	134	222	0.04%	0.005%
98	14.274	2161	2163	2165	rVB	258	175	0.03%	0.004%
99	14.749	2239	2241	2243	rBV2	273	171	0.03%	0.004%
100	15.389	2342	2346	2354	rVB3	1292	2425	0.45%	0.056%




Sum of corrected areas: 4315159

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042522.D
Acq On : 24 Jul 2024 17:00
Operator : JC/MD
Sample : P3334-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

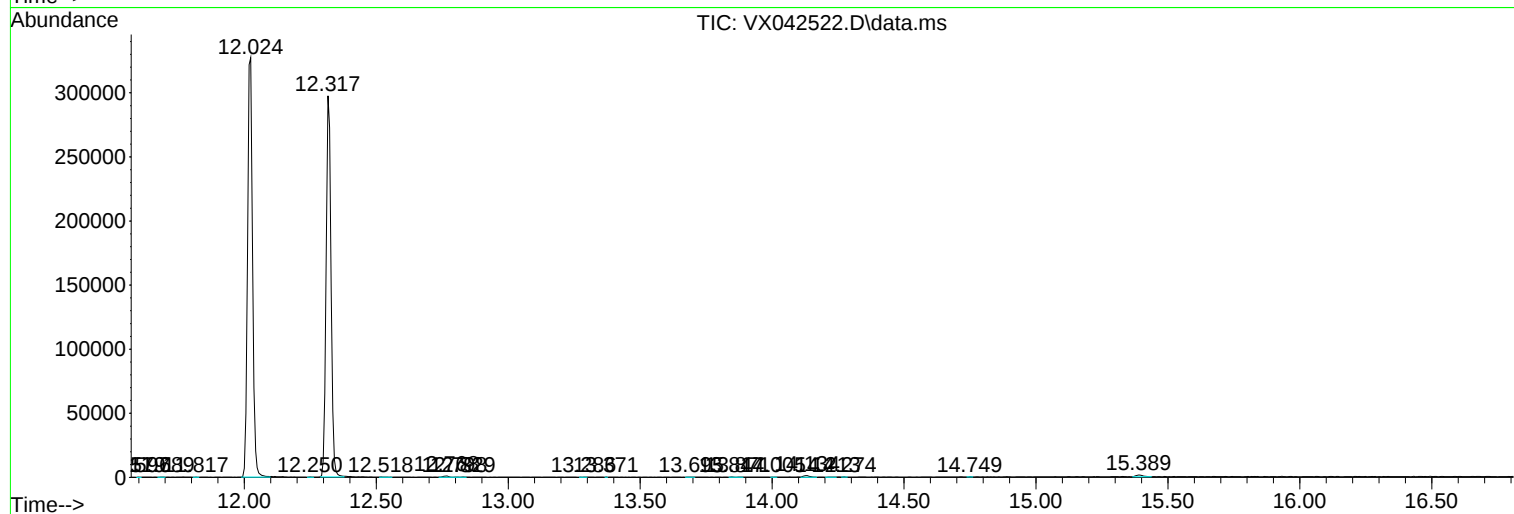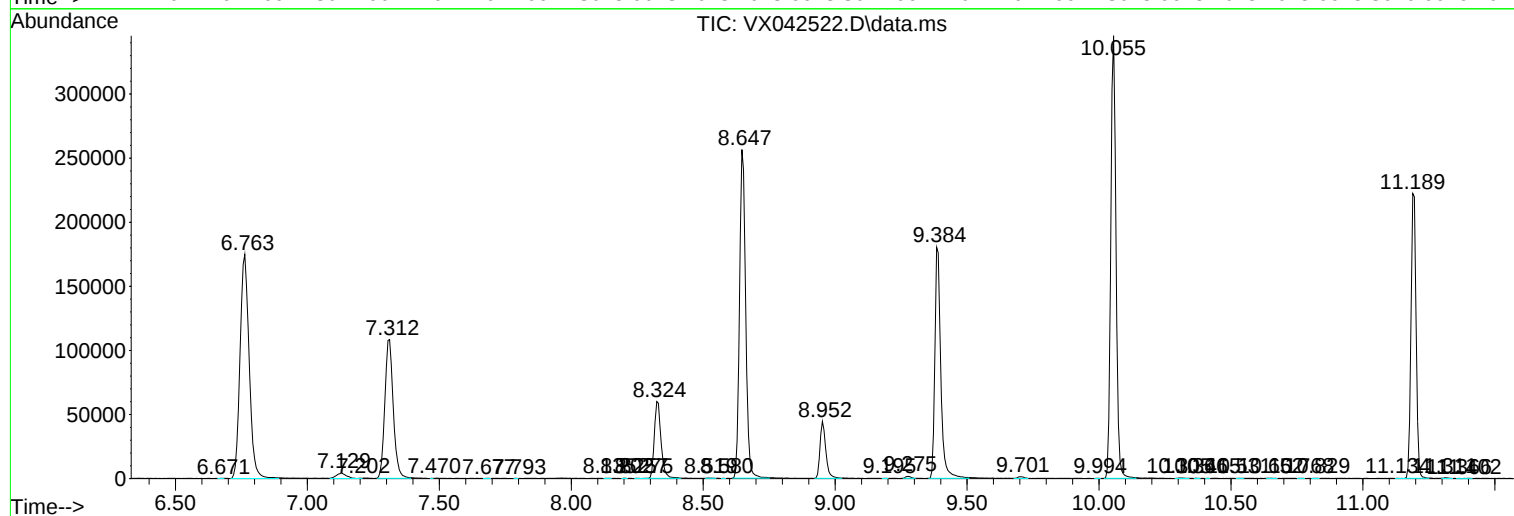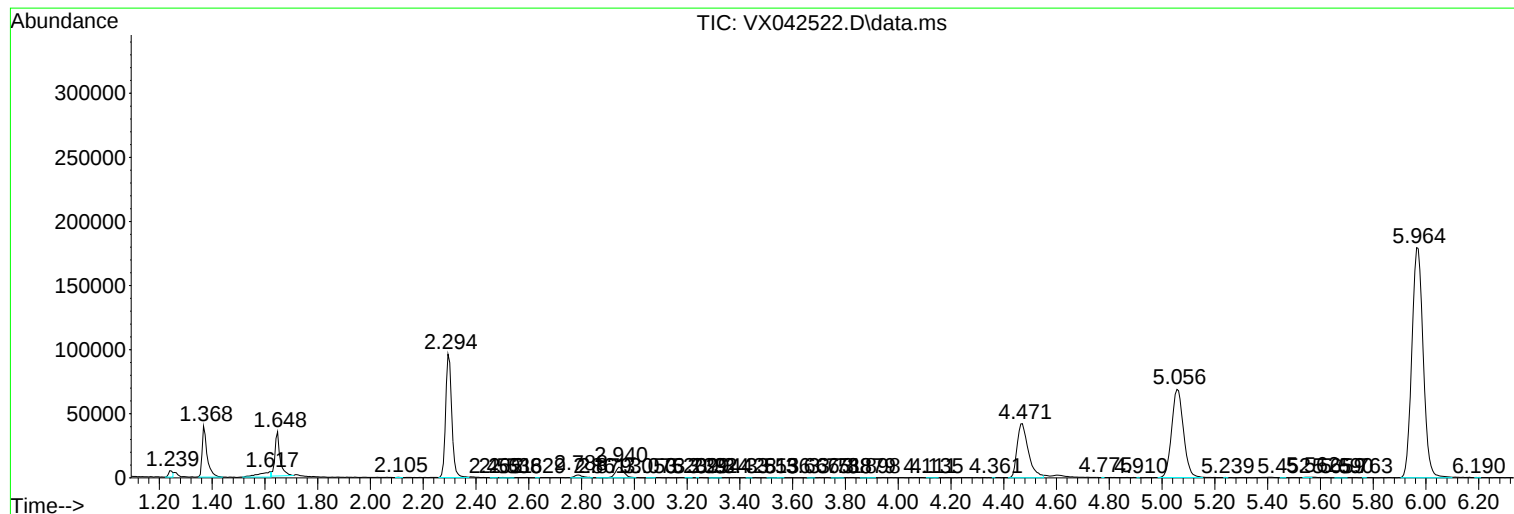

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042522.D
Acq On : 24 Jul 2024 17:00
Operator : JC/MD
Sample : P3334-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042522.D
Acq On : 24 Jul 2024 17:00
Operator : JC/MD
Sample : P3334-01 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc