

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042523.D
 Acq On : 24 Jul 2024 17:23
 Operator : JC/MD
 Sample : P3334-02 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	27	rBV	4880	5430	0.99%	0.122%
2	1.368	43	46	61	rVB	40051	53354	9.74%	1.199%
3	1.538	72	74	75	rBV	871	712	0.13%	0.016%
4	1.648	88	92	101	rVB	31616	44371	8.10%	0.997%
5	1.831	120	122	125	rBV2	324	260	0.05%	0.006%
6	2.294	192	198	210	rBV	100380	157599	28.77%	3.541%
7	2.562	240	242	244	rBV	114	132	0.02%	0.003%
8	2.605	247	249	250	rBV	99	55	0.01%	0.001%
9	2.703	262	265	266	rBV	291	238	0.04%	0.005%
10	2.782	274	278	284	rBV3	2026	4068	0.74%	0.091%
11	2.861	289	291	292	rVB2	96	62	0.01%	0.001%
12	2.879	292	294	295	rBV	137	86	0.02%	0.002%
13	2.940	295	304	313	rBV	8321	18836	3.44%	0.423%
14	3.062	321	324	327	rBV2	151	253	0.05%	0.006%
15	3.117	332	333	337	rVB	176	172	0.03%	0.004%
16	3.154	337	339	342	rBV2	132	206	0.04%	0.005%
17	3.270	356	358	360	rVB	158	145	0.03%	0.003%
18	3.288	360	361	363	rBV	136	117	0.02%	0.003%
19	3.318	365	366	368	rBV2	126	108	0.02%	0.002%
20	3.373	374	375	377	rBV	152	132	0.02%	0.003%
21	3.446	386	387	388	rBV	89	40	0.01%	0.001%
22	3.526	396	400	402	rBV2	109	118	0.02%	0.003%
23	3.672	420	424	427	rBV2	132	240	0.04%	0.005%
24	3.715	429	431	432	rBV	121	117	0.02%	0.003%
25	3.745	435	436	437	rBV	88	58	0.01%	0.001%
26	3.812	444	447	449	rBV2	130	161	0.03%	0.004%
27	3.885	456	459	462	rVB2	142	196	0.04%	0.004%
28	3.916	462	464	468	rBV2	174	271	0.05%	0.006%
29	4.141	500	501	504	rVB2	136	106	0.02%	0.002%
30	4.300	525	527	528	rVB	115	67	0.01%	0.002%
31	4.336	531	533	535	rBV	64	64	0.01%	0.001%
32	4.471	546	555	570	rBV	45536	139100	25.39%	3.125%
33	5.056	639	651	670	rBV	71897	221892	40.50%	4.985%
34	5.208	675	676	677	rBV	101	46	0.01%	0.001%
35	5.385	702	705	707	rBV3	230	336	0.06%	0.008%
36	5.702	754	757	758	rBV	118	161	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042523.D
Acq On : 24 Jul 2024 17:23
Operator : JC/MD
Sample : P3334-02 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Title : VOC Analysis

37	5.800	772	773	775	rBV2	111	53	0.01%	0.001%
38	5.854	780	782	784	rVB	114	80	0.01%	0.002%
39	5.897	788	789	790	rBV	88	61	0.01%	0.001%
40	5.964	790	800	817	rBV2	186835	547869	100.00%	12.308%
41	6.464	879	882	883	rBV2	122	139	0.03%	0.003%
42	6.519	890	891	894	rBV	85	50	0.01%	0.001%
43	6.641	909	911	912	rBV	165	146	0.03%	0.003%
44	6.763	922	931	946	rBV	177606	430073	78.50%	9.662%
45	7.129	983	991	1001	rBV3	16303	39246	7.16%	0.882%
46	7.305	1013	1020	1045	rBV	113683	252953	46.17%	5.683%
47	7.501	1049	1052	1053	rBV2	277	219	0.04%	0.005%
48	7.653	1076	1077	1078	rBV	176	97	0.02%	0.002%
49	7.836	1105	1107	1111	rBV2	139	196	0.04%	0.004%
50	7.952	1123	1126	1129	rBV2	405	525	0.10%	0.012%
51	8.244	1173	1174	1176	rBV2	104	82	0.01%	0.002%
52	8.324	1182	1187	1203	rBV	63272	108771	19.85%	2.444%
53	8.519	1215	1219	1220	rBV2	397	474	0.09%	0.011%
54	8.647	1234	1240	1256	rBV	271141	425088	77.59%	9.550%
55	8.952	1285	1290	1305	rBV	45944	70730	12.91%	1.589%
56	9.165	1324	1325	1327	rVV	98	41	0.01%	0.001%
57	9.195	1327	1330	1331	rVB2	134	112	0.02%	0.003%
58	9.275	1339	1343	1347	rBV3	1600	2124	0.39%	0.048%
59	9.336	1351	1353	1356	rBV	107	174	0.03%	0.004%
60	9.384	1356	1361	1384	rBV	181627	289283	52.80%	6.499%
61	9.701	1410	1413	1419	rBV2	1327	1912	0.35%	0.043%
62	9.915	1446	1448	1450	rBV2	88	59	0.01%	0.001%
63	9.988	1458	1460	1463	rBV2	96	68	0.01%	0.002%
64	10.012	1463	1464	1465	rBV	86	47	0.01%	0.001%
65	10.055	1465	1471	1482	rBV	353151	488709	89.20%	10.979%
66	10.317	1509	1514	1518	rBV3	316	454	0.08%	0.010%
67	10.646	1566	1568	1570	rBV	266	228	0.04%	0.005%
68	10.793	1591	1592	1593	rBV	90	64	0.01%	0.001%
69	10.823	1596	1597	1601	rVV2	165	144	0.03%	0.003%
70	10.866	1601	1604	1606	rVV2	154	134	0.02%	0.003%
71	10.884	1606	1607	1609	rBV	61	42	0.01%	0.001%
72	10.915	1609	1612	1614	rBV2	110	104	0.02%	0.002%
73	10.994	1623	1625	1628	rBV2	87	87	0.02%	0.002%
74	11.079	1638	1639	1642	rVB	175	123	0.02%	0.003%
75	11.104	1642	1643	1645	rBV	116	110	0.02%	0.002%
76	11.195	1652	1658	1666	rBV	228076	306585	55.96%	6.888%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042523.D
 Acq On : 24 Jul 2024 17:23
 Operator : JC/MD
 Sample : P3334-02 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.317	1675	1678	1680	rBV2	456	413	0.08%	0.009%
78	11.421	1694	1695	1696	rBV	118	62	0.01%	0.001%
79	11.610	1724	1726	1727	rBV2	107	69	0.01%	0.002%
80	11.884	1769	1771	1773	rBV	70	73	0.01%	0.002%
81	12.024	1788	1794	1808	rBV	347268	438022	79.95%	9.841%
82	12.231	1826	1828	1831	rBV3	200	138	0.03%	0.003%
83	12.317	1837	1842	1855	rBV	292152	391193	71.40%	8.788%
84	12.463	1864	1866	1871	rBV2	168	253	0.05%	0.006%
85	12.579	1884	1885	1888	rBV	110	81	0.01%	0.002%
86	12.695	1902	1904	1906	rBV	99	56	0.01%	0.001%
87	12.762	1911	1915	1920	rVB2	693	1032	0.19%	0.023%
88	13.201	1985	1987	1989	rBV	127	114	0.02%	0.003%
89	13.579	2047	2049	2052	rVB2	150	124	0.02%	0.003%
90	13.634	2057	2058	2061	rBV	193	192	0.04%	0.004%
91	13.786	2081	2083	2086	rBV2	200	217	0.04%	0.005%
92	13.902	2100	2102	2103	rBV	128	107	0.02%	0.002%
93	13.987	2114	2116	2119	rVB2	221	143	0.03%	0.003%
94	14.012	2119	2120	2123	rBV	130	145	0.03%	0.003%
95	14.109	2134	2136	2137	rBV	245	165	0.03%	0.004%
96	14.127	2137	2139	2143	rVV2	618	801	0.15%	0.018%
97	14.231	2154	2156	2157	rBV	131	58	0.01%	0.001%
98	14.298	2166	2167	2169	rBV2	213	173	0.03%	0.004%
99	14.993	2280	2281	2283	rBV2	248	205	0.04%	0.005%
100	16.389	2506	2510	2514	rBV2	353	597	0.11%	0.013%




Sum of corrected areas: 4451198

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042523.D
Acq On : 24 Jul 2024 17:23
Operator : JC/MD
Sample : P3334-02 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

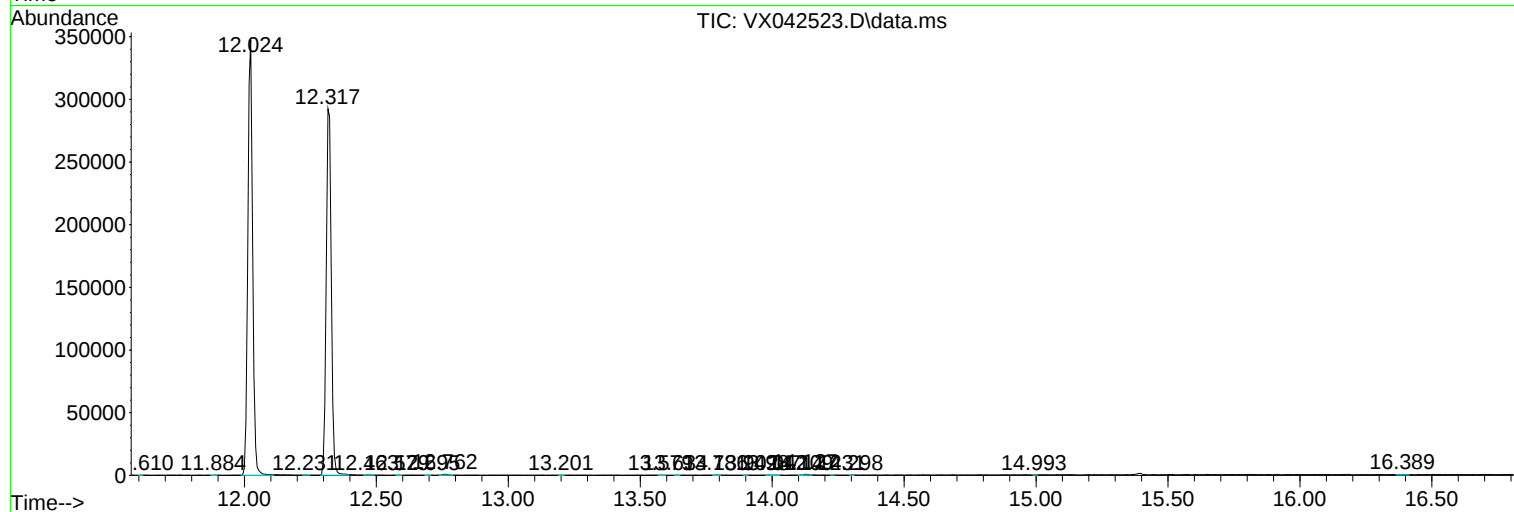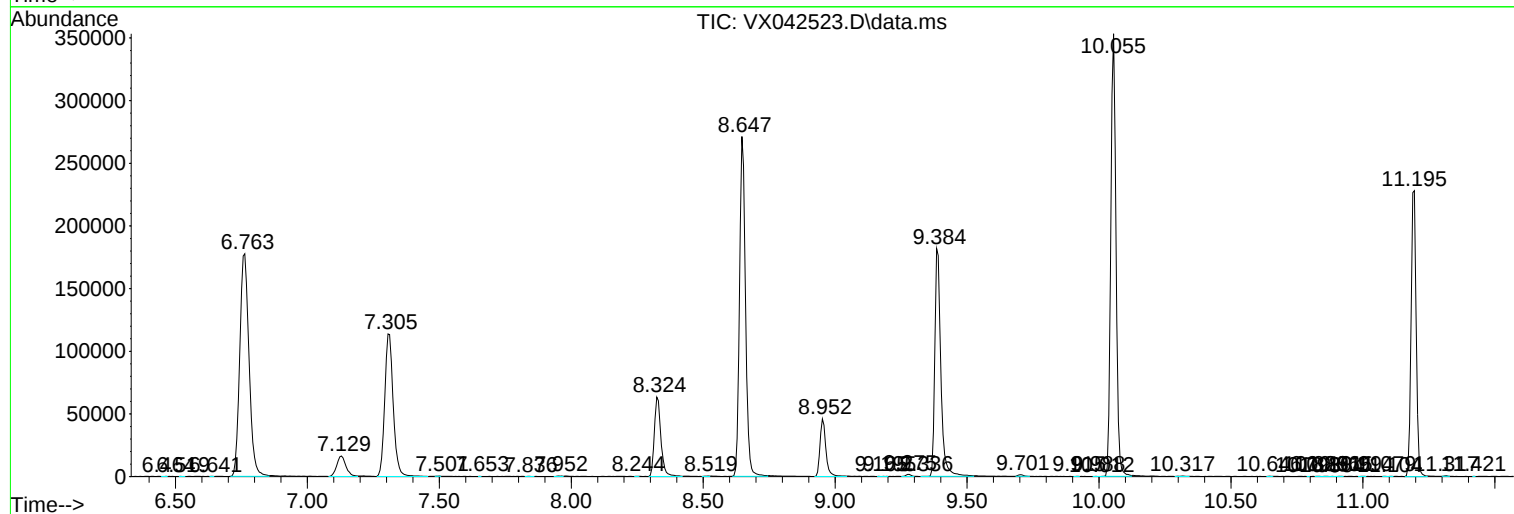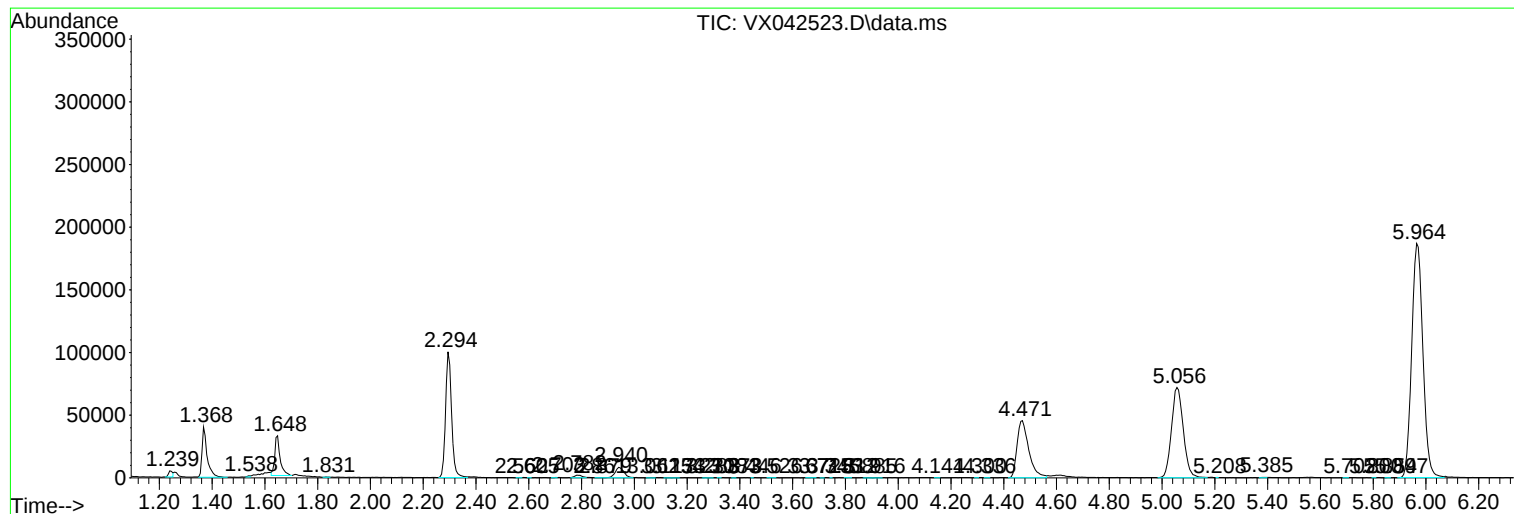

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042523.D
Acq On : 24 Jul 2024 17:23
Operator : JC/MD
Sample : P3334-02 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042523.D
Acq On : 24 Jul 2024 17:23
Operator : JC/MD
Sample : P3334-02 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc