

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042524.D
 Acq On : 24 Jul 2024 17:47
 Operator : JC/MD
 Sample : P3334-03 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	38	rBV2	4511	9133	1.62%	0.204%
2	1.368	42	46	60	rVB	41086	54423	9.67%	1.216%
3	1.648	88	92	101	rVB	33838	45781	8.13%	1.023%
4	2.026	153	154	156	rBV2	192	140	0.02%	0.003%
5	2.051	156	158	159	rBV	128	76	0.01%	0.002%
6	2.294	192	198	212	rBV	104327	163660	29.07%	3.658%
7	2.581	244	245	250	rBV2	199	236	0.04%	0.005%
8	2.654	255	257	260	rVB2	128	165	0.03%	0.004%
9	2.685	260	262	264	rBV2	90	105	0.02%	0.002%
10	2.703	264	265	266	rBV	234	117	0.02%	0.003%
11	2.746	270	272	273	rVB	106	63	0.01%	0.001%
12	2.788	273	279	284	rBV2	2024	3754	0.67%	0.084%
13	2.947	295	305	316	rBV	8733	21353	3.79%	0.477%
14	3.026	316	318	319	rBV	137	86	0.02%	0.002%
15	3.081	325	327	330	rBV2	86	86	0.02%	0.002%
16	3.111	330	332	333	rVB	141	90	0.02%	0.002%
17	3.142	335	337	339	rBV	163	118	0.02%	0.003%
18	3.319	363	366	367	rBV	118	101	0.02%	0.002%
19	3.355	369	372	373	rVV	117	83	0.01%	0.002%
20	3.544	401	403	406	rVB2	167	186	0.03%	0.004%
21	3.575	406	408	410	rBV2	121	129	0.02%	0.003%
22	3.678	423	425	427	rVB	161	141	0.03%	0.003%
23	3.715	427	431	432	rBV	153	176	0.03%	0.004%
24	3.751	435	437	439	rVV	67	69	0.01%	0.002%
25	3.782	441	442	444	rVB	128	75	0.01%	0.002%
26	3.812	444	447	449	rBV2	93	108	0.02%	0.002%
27	3.892	459	460	462	rVB	132	81	0.01%	0.002%
28	3.922	462	465	466	rBV	159	151	0.03%	0.003%
29	3.947	466	469	470	rBV	150	139	0.02%	0.003%
30	4.026	479	482	483	rVB	125	101	0.02%	0.002%
31	4.160	503	504	507	rBV2	117	117	0.02%	0.003%
32	4.312	527	529	532	rVB2	122	118	0.02%	0.003%
33	4.471	547	555	571	rBV	43807	132376	23.51%	2.959%
34	4.776	603	605	606	rBV	171	151	0.03%	0.003%
35	4.892	622	624	627	rBV2	96	68	0.01%	0.002%
36	4.922	627	629	630	rVB	163	93	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042524.D
 Acq On : 24 Jul 2024 17:47
 Operator : JC/MD
 Sample : P3334-03 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.056	640	651	669	rBV	73490	227932	40.48%	5.095%
38	5.398	702	707	708	rBV3	284	507	0.09%	0.011%
39	5.544	727	731	732	rBV3	300	328	0.06%	0.007%
40	5.696	754	756	757	rBV	142	122	0.02%	0.003%
41	5.794	768	772	773	rBV2	142	183	0.03%	0.004%
42	5.964	790	800	816	rBV2	193374	563064	100.00%	12.586%
43	6.300	853	855	856	rVB2	194	117	0.02%	0.003%
44	6.312	856	857	860	rBV2	127	153	0.03%	0.003%
45	6.342	860	862	864	rVV	103	82	0.01%	0.002%
46	6.379	864	868	869	rVV2	183	217	0.04%	0.005%
47	6.428	874	876	879	rVB	117	80	0.01%	0.002%
48	6.519	887	891	892	rBV	65	71	0.01%	0.002%
49	6.544	894	895	898	rVB2	208	128	0.02%	0.003%
50	6.635	909	910	913	rBV	100	60	0.01%	0.001%
51	6.696	916	920	921	rBV2	121	107	0.02%	0.002%
52	6.763	921	931	949	rBV	177170	430889	76.53%	9.631%
53	7.123	983	990	991	rBV3	3517	5540	0.98%	0.124%
54	7.214	1000	1005	1006	rBV3	451	565	0.10%	0.013%
55	7.306	1012	1020	1037	rBV	112172	255893	45.45%	5.720%
56	7.537	1056	1058	1061	rVB	162	189	0.03%	0.004%
57	7.568	1061	1063	1064	rBV	125	111	0.02%	0.002%
58	7.611	1069	1070	1071	rBV	138	60	0.01%	0.001%
59	7.861	1107	1111	1112	rBV	110	95	0.02%	0.002%
60	7.879	1112	1114	1115	rBV	119	70	0.01%	0.002%
61	7.940	1122	1124	1125	rBV2	209	150	0.03%	0.003%
62	7.958	1125	1127	1129	rVV	229	237	0.04%	0.005%
63	8.092	1146	1149	1152	rBV2	126	161	0.03%	0.004%
64	8.232	1170	1172	1174	rVB	103	62	0.01%	0.001%
65	8.287	1179	1181	1182	rBV2	120	93	0.02%	0.002%
66	8.324	1182	1187	1204	rBV	64183	111669	19.83%	2.496%
67	8.519	1214	1219	1221	rBV3	363	557	0.10%	0.012%
68	8.647	1234	1240	1256	rBV	272847	437355	77.67%	9.776%
69	8.952	1285	1290	1299	rBV	48068	71967	12.78%	1.609%
70	9.250	1337	1339	1340	rBV	96	61	0.01%	0.001%
71	9.275	1340	1343	1347	rVB5	1377	2243	0.40%	0.050%
72	9.348	1353	1355	1356	rBV2	109	76	0.01%	0.002%
73	9.385	1356	1361	1380	rBV	183261	287927	51.14%	6.436%
74	9.702	1409	1413	1419	rVB	1454	2168	0.39%	0.048%
75	9.775	1423	1425	1426	rBV	107	55	0.01%	0.001%
76	9.909	1446	1447	1450	rVB	131	105	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042524.D
 Acq On : 24 Jul 2024 17:47
 Operator : JC/MD
 Sample : P3334-03 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	10.055	1465	1471	1488	rBV	354105	487160	86.52%	10.889%
78	10.281	1507	1508	1509	rBV	127	61	0.01%	0.001%
79	10.537	1546	1550	1551	rBV2	170	222	0.04%	0.005%
80	10.653	1567	1569	1572	rVB2	209	208	0.04%	0.005%
81	10.781	1589	1590	1593	rBV	152	123	0.02%	0.003%
82	11.134	1645	1648	1649	rBV	207	217	0.04%	0.005%
83	11.189	1652	1657	1670	rVV	231832	306208	54.38%	6.844%
84	11.549	1714	1716	1717	rBV2	85	84	0.01%	0.002%
85	11.762	1749	1751	1753	rVB	227	144	0.03%	0.003%
86	12.024	1788	1794	1803	rBV	332785	437337	77.67%	9.775%
87	12.317	1837	1842	1853	rBV	315300	402583	71.50%	8.999%
88	12.476	1867	1868	1870	rBB	238	131	0.02%	0.003%
89	12.689	1902	1903	1905	rBV2	112	88	0.02%	0.002%
90	12.762	1911	1915	1919	rBV3	898	1400	0.25%	0.031%
91	12.860	1929	1931	1935	rVB2	150	140	0.02%	0.003%
92	12.939	1942	1944	1946	rBV	118	64	0.01%	0.001%
93	13.073	1965	1966	1968	rBV	105	66	0.01%	0.001%
94	13.189	1984	1985	1986	rVB	287	105	0.02%	0.002%
95	13.201	1986	1987	1988	rBV	175	109	0.02%	0.002%
96	13.317	2004	2006	2007	rBV	107	58	0.01%	0.001%
97	13.353	2011	2012	2013	rVB	162	59	0.01%	0.001%
98	13.719	2071	2072	2074	rVB2	167	84	0.01%	0.002%
99	14.061	2127	2128	2130	rBV2	98	68	0.01%	0.002%
100	14.128	2136	2139	2149	rVB	1192	1833	0.33%	0.041%

Sum of corrected areas: 4473850




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042524.D
Acq On : 24 Jul 2024 17:47
Operator : JC/MD
Sample : P3334-03 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

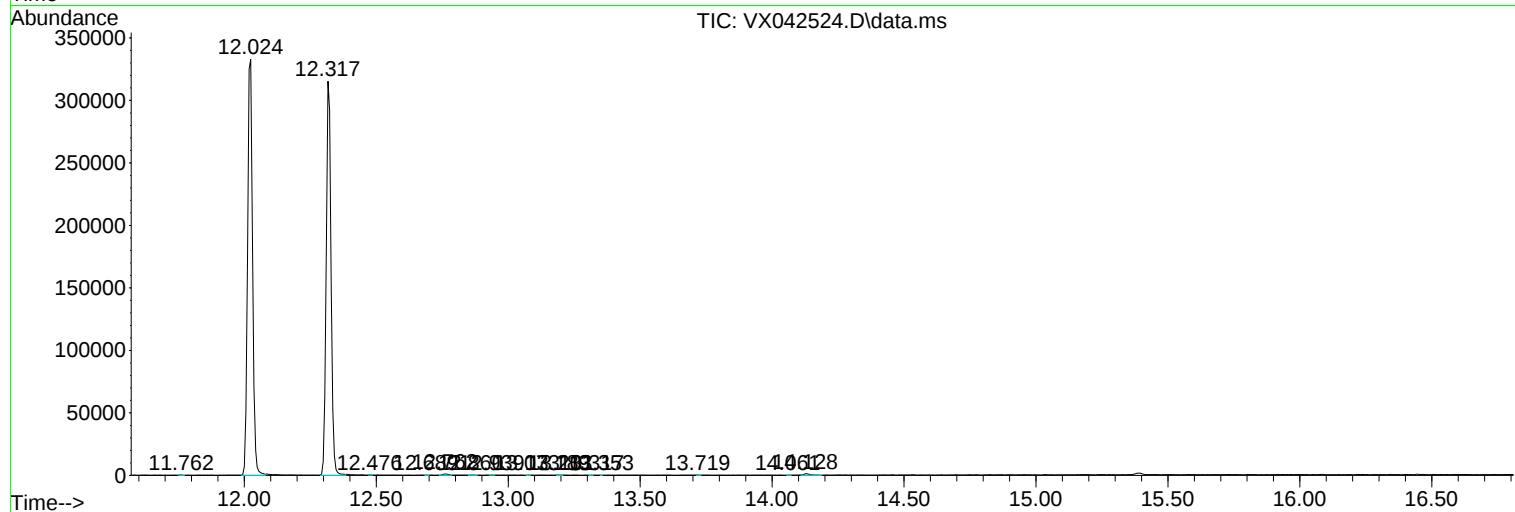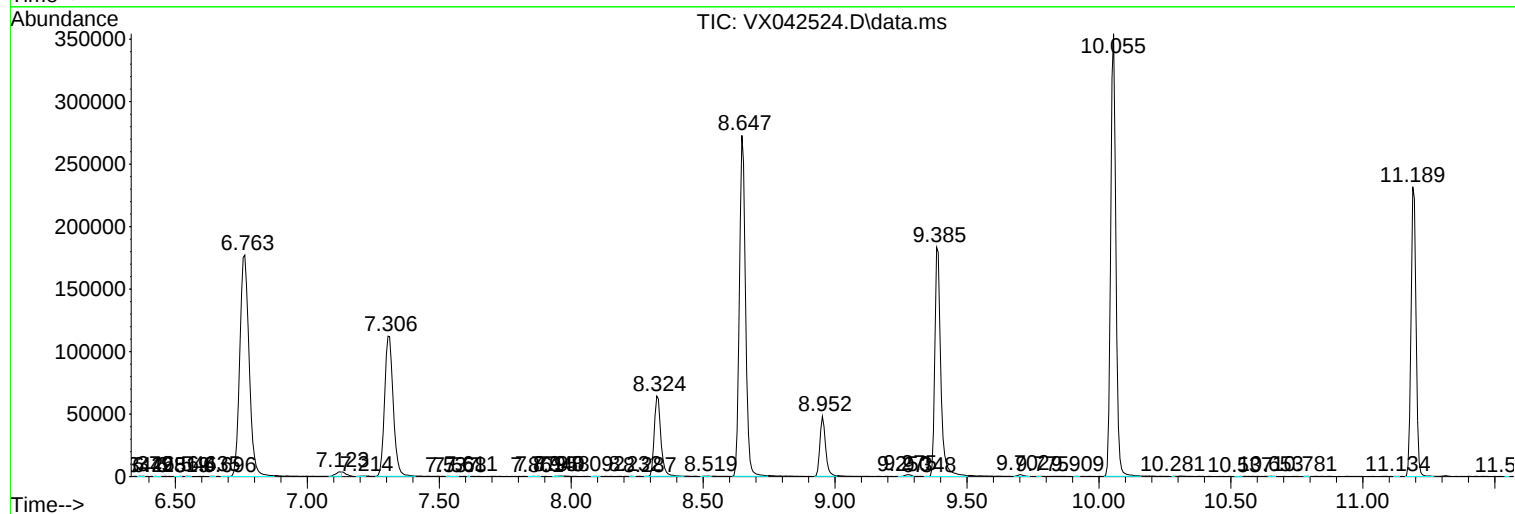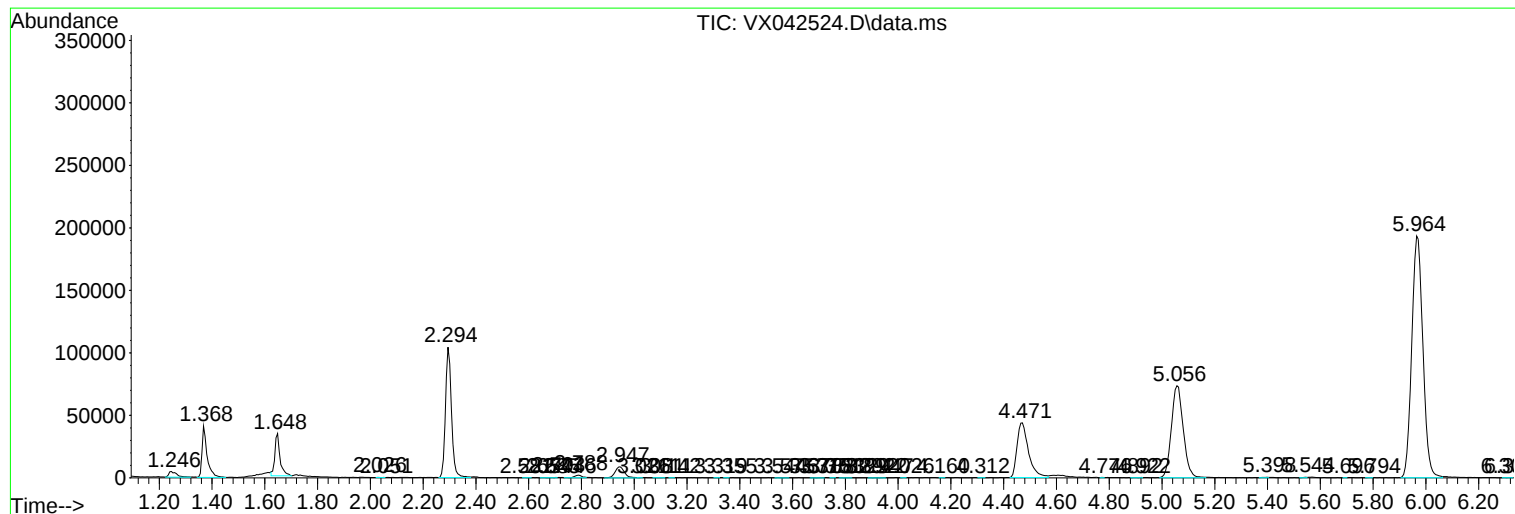

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042524.D
Acq On : 24 Jul 2024 17:47
Operator : JC/MD
Sample : P3334-03 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042524.D
Acq On : 24 Jul 2024 17:47
Operator : JC/MD
Sample : P3334-03 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc