

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042525.D
 Acq On : 24 Jul 2024 18:10
 Operator : JC/MD
 Sample : P3334-04 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	27	rBV	4367	4616	0.88%	0.098%
2	1.368	43	46	57	rVB	37506	48629	9.32%	1.032%
3	1.502	65	68	69	rBV2	293	363	0.07%	0.008%
4	1.648	89	92	101	rVB	32280	40585	7.78%	0.862%
5	2.057	158	159	161	rBV	217	163	0.03%	0.003%
6	2.118	167	169	170	rBV	186	143	0.03%	0.003%
7	2.160	174	176	178	rVB	249	165	0.03%	0.004%
8	2.203	182	183	185	rBV	123	110	0.02%	0.002%
9	2.294	191	198	210	rBV	90755	143691	27.55%	3.051%
10	2.502	229	232	233	rBV	113	127	0.02%	0.003%
11	2.544	238	239	240	rVV	131	80	0.02%	0.002%
12	2.569	240	243	245	rVB	260	263	0.05%	0.006%
13	2.654	255	257	259	rBV2	81	94	0.02%	0.002%
14	2.709	263	266	272	rVV2	144	252	0.05%	0.005%
15	2.788	273	279	286	rVV2	1944	3895	0.75%	0.083%
16	2.947	292	305	318	rBV	10630	24660	4.73%	0.524%
17	3.081	324	327	328	rBV	175	202	0.04%	0.004%
18	3.123	332	334	335	rBV	100	94	0.02%	0.002%
19	3.160	338	340	341	rBV2	80	73	0.01%	0.002%
20	3.227	349	351	354	rVB2	151	181	0.03%	0.004%
21	3.538	399	402	404	rBV2	160	210	0.04%	0.004%
22	3.587	408	410	411	rVB	160	87	0.02%	0.002%
23	3.599	411	412	416	rBV	129	175	0.03%	0.004%
24	3.660	421	422	424	rBV	161	116	0.02%	0.002%
25	3.696	426	428	431	rVV	152	154	0.03%	0.003%
26	3.751	435	437	439	rBV2	144	161	0.03%	0.003%
27	3.825	447	449	452	rBV2	65	82	0.02%	0.002%
28	3.867	454	456	459	rVB2	87	102	0.02%	0.002%
29	3.892	459	460	462	rBV	99	90	0.02%	0.002%
30	3.959	468	471	472	rBV	131	112	0.02%	0.002%
31	4.093	491	493	495	rBV2	123	139	0.03%	0.003%
32	4.209	509	512	513	rBV	121	140	0.03%	0.003%
33	4.263	519	521	522	rVB	170	99	0.02%	0.002%
34	4.294	522	526	527	rBV2	117	166	0.03%	0.004%
35	4.465	547	554	568	rBV	44121	132563	25.41%	2.814%
36	4.916	626	628	631	rVB2	170	168	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042525.D
 Acq On : 24 Jul 2024 18:10
 Operator : JC/MD
 Sample : P3334-04 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	4.946	631	633	636	rBV2	115	165	0.03%	0.004%
38	5.056	638	651	668	rBV	68798	213351	40.90%	4.530%
39	5.397	703	707	712	rBV3	222	313	0.06%	0.007%
40	5.483	716	721	722	rBV	145	161	0.03%	0.003%
41	5.751	763	765	766	rBV	125	78	0.01%	0.002%
42	5.806	772	774	778	rBV2	101	141	0.03%	0.003%
43	5.964	789	800	820	rBV3	175956	521599	100.00%	11.074%
44	6.391	868	870	871	rVB2	162	95	0.02%	0.002%
45	6.672	914	916	919	rVB2	151	148	0.03%	0.003%
46	6.763	922	931	948	rVV	175902	421034	80.72%	8.939%
47	7.123	981	990	1004	rBV	204266	460071	88.20%	9.768%
48	7.312	1013	1021	1036	rBV	106036	238786	45.78%	5.070%
49	7.440	1041	1042	1043	rVB	210	77	0.01%	0.002%
50	7.690	1080	1083	1085	rBV2	208	210	0.04%	0.004%
51	7.738	1089	1091	1094	rVV2	161	174	0.03%	0.004%
52	7.793	1098	1100	1103	rBV	103	108	0.02%	0.002%
53	7.921	1117	1121	1123	rBV2	119	149	0.03%	0.003%
54	7.958	1123	1127	1130	rBV3	422	648	0.12%	0.014%
55	8.257	1174	1176	1178	rBV	148	110	0.02%	0.002%
56	8.324	1181	1187	1206	rBV	60177	105854	20.29%	2.247%
57	8.501	1214	1216	1218	rBV3	169	120	0.02%	0.003%
58	8.525	1218	1220	1225	rVB3	302	454	0.09%	0.010%
59	8.647	1234	1240	1252	rBV	251841	399248	76.54%	8.476%
60	8.952	1285	1290	1304	rBV	44081	67963	13.03%	1.443%
61	9.208	1331	1332	1333	rBV	124	88	0.02%	0.002%
62	9.275	1340	1343	1352	rVB2	1503	2306	0.44%	0.049%
63	9.391	1356	1362	1375	rBV	174874	274645	52.65%	5.831%
64	9.702	1409	1413	1422	rVB	2142	2934	0.56%	0.062%
65	10.055	1465	1471	1486	rBV	349147	483041	92.61%	10.255%
66	10.183	1490	1492	1493	rVB	234	127	0.02%	0.003%
67	10.305	1510	1512	1515	rBV3	324	408	0.08%	0.009%
68	10.378	1522	1524	1526	rVB2	106	81	0.02%	0.002%
69	10.494	1541	1543	1547	rVB2	113	114	0.02%	0.002%
70	10.537	1547	1550	1553	rBV2	96	162	0.03%	0.003%
71	10.592	1556	1559	1561	rVB2	96	114	0.02%	0.002%
72	10.610	1561	1562	1566	rBV	156	149	0.03%	0.003%
73	10.653	1566	1569	1570	rBV2	180	172	0.03%	0.004%
74	10.744	1582	1584	1585	rBV	133	99	0.02%	0.002%
75	10.854	1600	1602	1604	rVB	165	88	0.02%	0.002%
76	10.878	1604	1606	1609	rVB2	107	90	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042525.D
 Acq On : 24 Jul 2024 18:10
 Operator : JC/MD
 Sample : P3334-04 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	10.915	1611	1612	1615	rBV2	140	125	0.02%	0.003%
78	11.061	1634	1636	1639	rBV2	92	74	0.01%	0.002%
79	11.189	1652	1657	1665	rBV	222576	298744	57.27%	6.342%
80	11.311	1675	1677	1684	rVB3	489	607	0.12%	0.013%
81	11.500	1706	1708	1711	rVB	119	91	0.02%	0.002%
82	11.622	1726	1728	1730	rBV	149	132	0.03%	0.003%
83	11.762	1748	1751	1753	rBV2	147	158	0.03%	0.003%
84	12.024	1788	1794	1810	rBV	346573	431012	82.63%	9.151%
85	12.317	1837	1842	1851	rBV	289043	374047	71.71%	7.941%
86	12.518	1874	1875	1877	rBV	139	81	0.02%	0.002%
87	12.762	1911	1915	1919	rVB2	928	1320	0.25%	0.028%
88	12.945	1944	1945	1947	rBV	140	86	0.02%	0.002%
89	13.036	1958	1960	1964	rVB	125	152	0.03%	0.003%
90	13.091	1967	1969	1971	rBV	124	104	0.02%	0.002%
91	13.225	1989	1991	1994	rVB	144	116	0.02%	0.002%
92	13.500	2035	2036	2038	rBV	161	93	0.02%	0.002%
93	13.573	2047	2048	2050	rBV2	116	112	0.02%	0.002%
94	13.731	2072	2074	2077	rBV2	117	86	0.02%	0.002%
95	13.774	2080	2081	2083	rBV	125	104	0.02%	0.002%
96	13.829	2088	2090	2093	rBV2	104	86	0.02%	0.002%
97	14.054	2125	2127	2128	rBV	174	87	0.02%	0.002%
98	14.128	2135	2139	2144	rBV	1227	1811	0.35%	0.038%
99	14.189	2147	2149	2150	rBV2	141	101	0.02%	0.002%
100	15.396	2343	2347	2351	rVB3	1541	2243	0.43%	0.048%

Sum of corrected areas: 4710197


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042525.D
Acq On : 24 Jul 2024 18:10
Operator : JC/MD
Sample : P3334-04 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

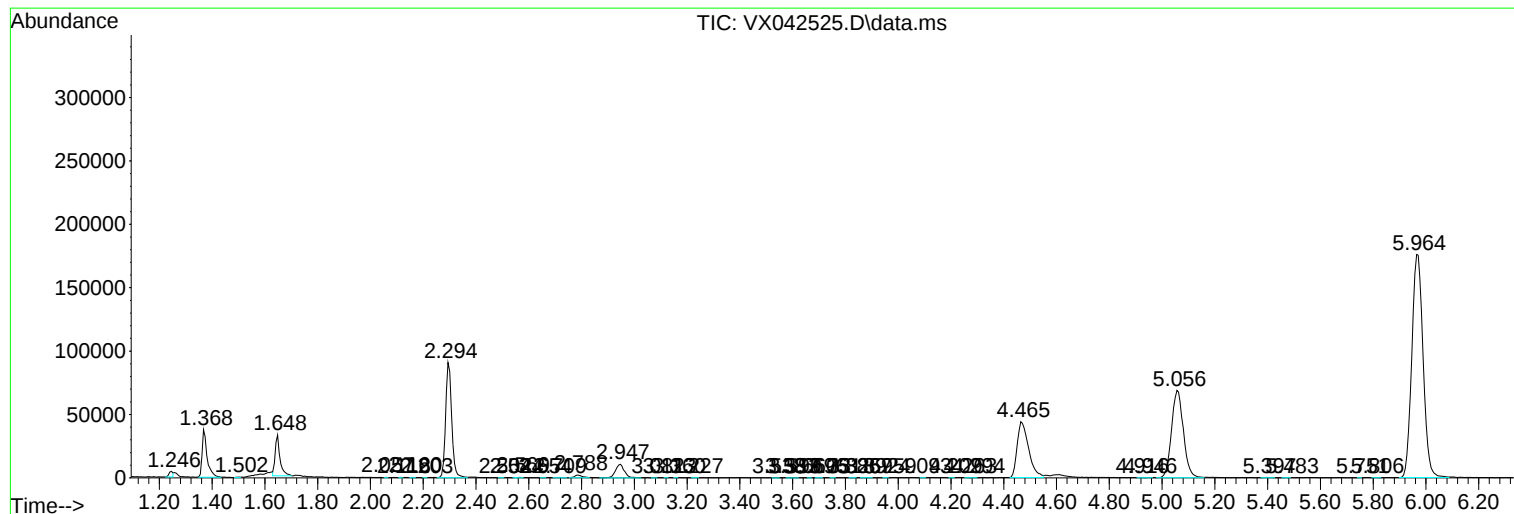

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042525.D
Acq On : 24 Jul 2024 18:10
Operator : JC/MD
Sample : P3334-04 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042525.D
Acq On : 24 Jul 2024 18:10
Operator : JC/MD
Sample : P3334-04 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc