

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042526.D
 Acq On : 24 Jul 2024 18:33
 Operator : JC/MD
 Sample : P3334-05 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	34	rBV2	4268	8026	1.52%	0.188%
2	1.368	43	46	59	rVB	37317	48228	9.13%	1.128%
3	1.648	88	92	101	rVB	32441	42535	8.05%	0.995%
4	2.227	185	187	188	rBV	160	135	0.03%	0.003%
5	2.294	192	198	211	rVV	90687	143521	27.17%	3.358%
6	2.508	231	233	235	rBV	107	78	0.01%	0.002%
7	2.538	235	238	240	rBV2	177	171	0.03%	0.004%
8	2.605	248	249	253	rBV2	146	164	0.03%	0.004%
9	2.782	274	278	283	rBV3	1775	3495	0.66%	0.082%
10	2.874	292	293	295	rBV	171	153	0.03%	0.004%
11	2.947	297	305	316	rVV2	8505	19600	3.71%	0.459%
12	3.056	321	323	324	rVB	156	102	0.02%	0.002%
13	3.069	324	325	326	rBV	111	78	0.01%	0.002%
14	3.123	331	334	335	rBV2	144	143	0.03%	0.003%
15	3.227	349	351	352	rBV	150	124	0.02%	0.003%
16	3.245	352	354	358	rVV2	142	248	0.05%	0.006%
17	3.276	358	359	364	rVB	183	220	0.04%	0.005%
18	3.319	364	366	367	rBV2	104	96	0.02%	0.002%
19	3.349	369	371	374	rVB	112	93	0.02%	0.002%
20	3.386	374	377	382	rBV	120	233	0.04%	0.005%
21	3.428	382	384	387	rVB	203	162	0.03%	0.004%
22	3.465	387	390	392	rBV	195	194	0.04%	0.005%
23	3.514	397	398	400	rVB	195	109	0.02%	0.003%
24	3.556	400	405	407	rBV	187	235	0.04%	0.005%
25	3.581	407	409	411	rVB	182	144	0.03%	0.003%
26	3.611	411	414	416	rVB2	138	175	0.03%	0.004%
27	3.636	416	418	420	rBV	123	114	0.02%	0.003%
28	3.660	420	422	424	rVB	91	66	0.01%	0.002%
29	3.690	426	427	429	rBV2	133	113	0.02%	0.003%
30	3.770	438	440	441	rBV	85	67	0.01%	0.002%
31	3.818	445	448	449	rBV	148	126	0.02%	0.003%
32	3.831	449	450	452	rBV2	85	72	0.01%	0.002%
33	3.922	462	465	467	rBV	116	142	0.03%	0.003%
34	3.947	467	469	470	rBV	92	69	0.01%	0.002%
35	3.977	470	474	475	rBV2	139	168	0.03%	0.004%
36	4.056	485	487	488	rBV	116	74	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042526.D
 Acq On : 24 Jul 2024 18:33
 Operator : JC/MD
 Sample : P3334-05 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	4.123	496	498	501	rVB	274	260	0.05%	0.006%
38	4.154	501	503	505	rBV	137	185	0.04%	0.004%
39	4.282	522	524	525	rBV	136	69	0.01%	0.002%
40	4.465	546	554	570	rBV	42239	128674	24.36%	3.010%
41	4.873	619	621	622	rBV	163	113	0.02%	0.003%
42	5.056	640	651	667	rBV2	67794	211519	40.05%	4.948%
43	5.385	703	705	708	rVB	181	146	0.03%	0.003%
44	5.416	708	710	712	rVB	211	164	0.03%	0.004%
45	5.434	712	713	714	rBV	188	127	0.02%	0.003%
46	5.568	731	735	738	rBV2	175	241	0.05%	0.006%
47	5.775	767	769	772	rVV2	133	142	0.03%	0.003%
48	5.806	772	774	777	rVB	127	119	0.02%	0.003%
49	5.964	789	800	819	rBV3	178732	528141	100.00%	12.355%
50	6.562	896	898	899	rVB	120	63	0.01%	0.001%
51	6.763	922	931	949	rBV	171255	419578	79.44%	9.816%
52	7.123	984	990	1000	rBV4	4046	10437	1.98%	0.244%
53	7.208	1002	1004	1005	rBV	189	128	0.02%	0.003%
54	7.306	1012	1020	1038	rBV	107811	240589	45.55%	5.628%
55	7.470	1046	1047	1048	rBV	175	100	0.02%	0.002%
56	7.489	1048	1050	1051	rVV	259	209	0.04%	0.005%
57	7.519	1053	1055	1058	rBV2	92	115	0.02%	0.003%
58	7.958	1124	1127	1128	rBV2	325	314	0.06%	0.007%
59	8.031	1137	1139	1144	rVB2	157	161	0.03%	0.004%
60	8.226	1169	1171	1173	rVB	151	91	0.02%	0.002%
61	8.324	1182	1187	1201	rBV	59507	103675	19.63%	2.425%
62	8.513	1216	1218	1221	rBV2	276	353	0.07%	0.008%
63	8.647	1234	1240	1256	rBV	253884	403794	76.46%	9.446%
64	8.872	1275	1277	1282	rVB3	209	246	0.05%	0.006%
65	8.952	1285	1290	1300	rBV	42776	65802	12.46%	1.539%
66	9.281	1338	1344	1348	rBV4	1403	2108	0.40%	0.049%
67	9.385	1356	1361	1380	rBV	177811	284230	53.82%	6.649%
68	9.702	1408	1413	1419	rVB2	2177	3217	0.61%	0.075%
69	9.781	1424	1426	1431	rBV3	130	188	0.04%	0.004%
70	9.903	1445	1446	1450	rBB	164	81	0.02%	0.002%
71	10.055	1465	1471	1489	rBV	354463	485192	91.87%	11.351%
72	10.311	1510	1513	1514	rBV	227	203	0.04%	0.005%
73	10.549	1550	1552	1556	rBV2	141	252	0.05%	0.006%
74	10.695	1574	1576	1578	rBV	95	76	0.01%	0.002%
75	10.817	1593	1596	1597	rBV	165	154	0.03%	0.004%
76	11.055	1634	1635	1637	rBV	68	73	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042526.D
 Acq On : 24 Jul 2024 18:33
 Operator : JC/MD
 Sample : P3334-05 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.189	1652	1657	1671	rBV	223858	302194	57.22%	7.070%
78	11.317	1674	1678	1683	rVB4	427	750	0.14%	0.018%
79	11.463	1700	1702	1707	rBV2	97	128	0.02%	0.003%
80	11.628	1727	1729	1732	rVB2	183	173	0.03%	0.004%
81	11.817	1758	1760	1761	rBV2	108	81	0.02%	0.002%
82	12.018	1788	1793	1806	rBV	325594	430229	81.46%	10.065%
83	12.128	1809	1811	1812	rBV	297	178	0.03%	0.004%
84	12.219	1824	1826	1832	rBV2	133	200	0.04%	0.005%
85	12.317	1837	1842	1853	rBV	285304	375687	71.13%	8.789%
86	12.512	1872	1874	1877	rVB2	221	206	0.04%	0.005%
87	12.543	1877	1879	1880	rBV	211	158	0.03%	0.004%
88	12.591	1885	1887	1888	rBV	169	119	0.02%	0.003%
89	12.732	1909	1910	1911	rBV	120	67	0.01%	0.002%
90	12.762	1912	1915	1918	rVB2	868	1052	0.20%	0.025%
91	12.823	1923	1925	1926	rBV2	113	62	0.01%	0.001%
92	12.921	1940	1941	1944	rVB	116	83	0.02%	0.002%
93	13.036	1958	1960	1965	rVB2	218	244	0.05%	0.006%
94	13.079	1965	1967	1968	rBV	131	68	0.01%	0.002%
95	13.402	2019	2020	2022	rBV	172	106	0.02%	0.002%
96	13.792	2083	2084	2087	rVB	166	90	0.02%	0.002%
97	13.987	2115	2116	2117	rBV	181	74	0.01%	0.002%
98	14.128	2135	2139	2143	rBV	920	1238	0.23%	0.029%
99	14.158	2143	2144	2147	rVB2	256	166	0.03%	0.004%
100	14.341	2171	2174	2180	rBV2	216	399	0.08%	0.009%




Sum of corrected areas: 4274554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042526.D
Acq On : 24 Jul 2024 18:33
Operator : JC/MD
Sample : P3334-05 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

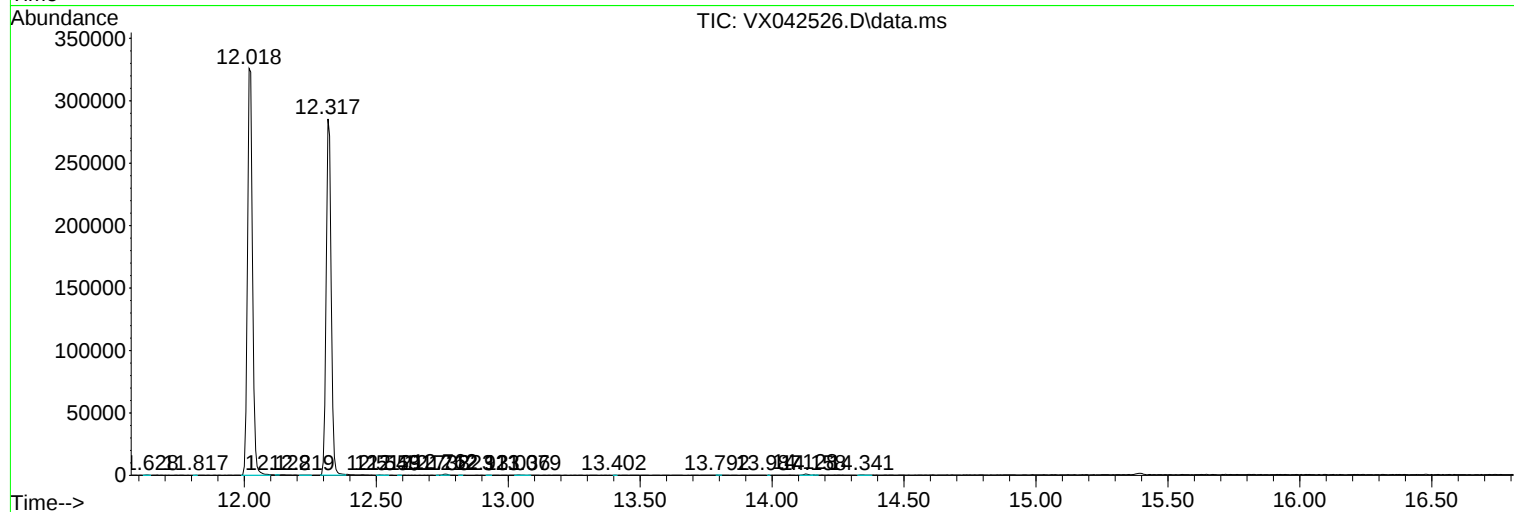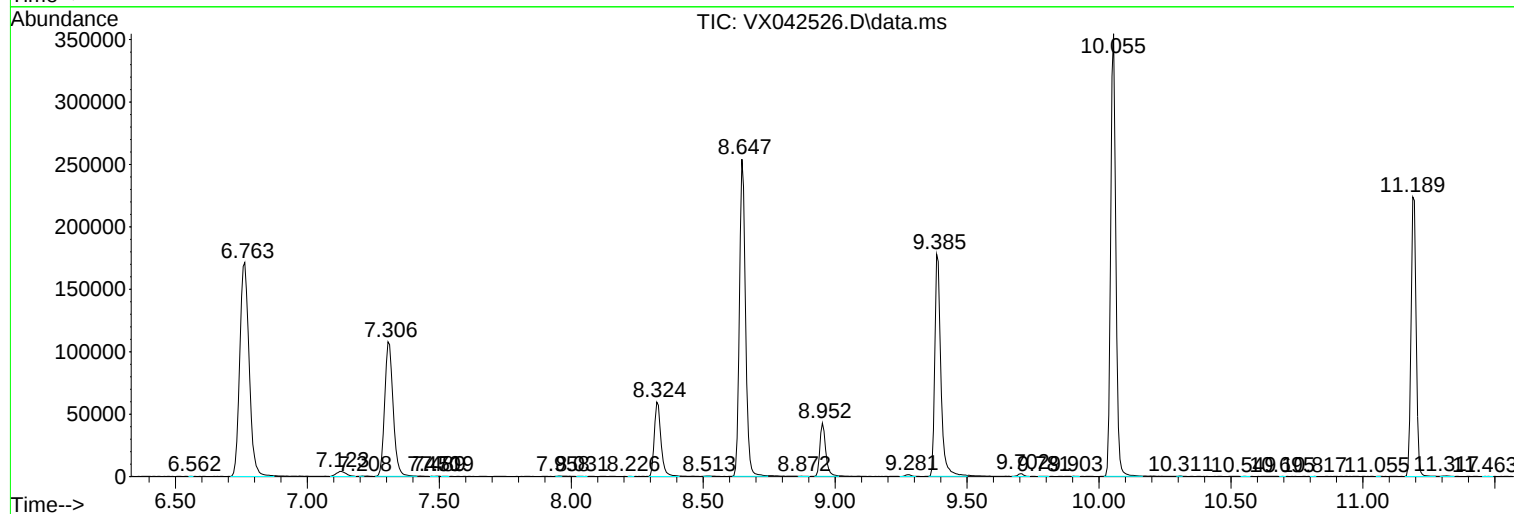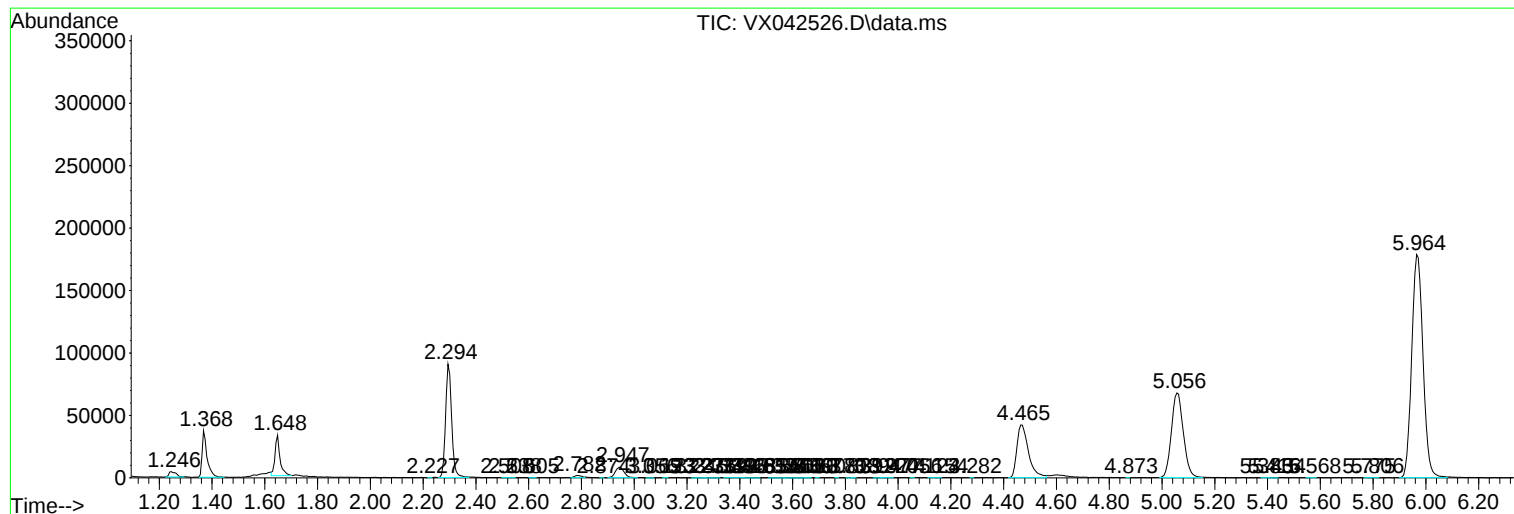

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042526.D
Acq On : 24 Jul 2024 18:33
Operator : JC/MD
Sample : P3334-05 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042526.D
Acq On : 24 Jul 2024 18:33
Operator : JC/MD
Sample : P3334-05 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc