

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042527.D
 Acq On : 24 Jul 2024 18:57
 Operator : JC/MD
 Sample : P3327-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	7	9	19	rVB	8904	11914	0.95%	0.203%
2	1.246	22	26	27	rVV	4031	4600	0.37%	0.078%
3	1.264	27	29	38	rVB2	7396	8573	0.69%	0.146%
4	1.374	43	47	66	rVB2	74510	103459	8.28%	1.765%
5	1.544	69	75	76	rBV4	1149	1667	0.13%	0.028%
6	1.593	76	83	84	rVV2	2660	5326	0.43%	0.091%
7	1.648	88	92	100	rVV	31320	44831	3.59%	0.765%
8	1.721	100	104	111	rVB2	5648	8985	0.72%	0.153%
9	1.934	135	139	144	rVB2	2843	3775	0.30%	0.064%
10	2.014	150	152	155	rVB	181	174	0.01%	0.003%
11	2.197	180	182	187	rVB2	226	254	0.02%	0.004%
12	2.252	187	191	192	rBV	224	294	0.02%	0.005%
13	2.300	192	199	211	rVV3	111206	203061	16.25%	3.465%
14	2.392	211	214	222	rVB3	1966	4395	0.35%	0.075%
15	2.508	230	233	236	rVB3	177	245	0.02%	0.004%
16	2.575	239	244	249	rVB2	755	1419	0.11%	0.024%
17	2.611	249	250	254	rVB	130	153	0.01%	0.003%
18	2.697	261	264	265	rBV	220	207	0.02%	0.004%
19	2.715	265	267	270	rVB2	214	236	0.02%	0.004%
20	2.794	270	280	281	rBV5	985	2001	0.16%	0.034%
21	2.947	297	305	313	rBV	2318	5411	0.43%	0.092%
22	3.087	321	328	340	rBV	9950	19927	1.60%	0.340%
23	3.343	367	370	371	rBV2	147	161	0.01%	0.003%
24	3.440	381	386	391	rVV3	849	1473	0.12%	0.025%
25	3.605	403	413	428	rBV	42114	100485	8.04%	1.715%
26	3.776	435	441	443	rBV2	182	356	0.03%	0.006%
27	3.824	445	449	450	rBV2	127	177	0.01%	0.003%
28	3.928	463	466	468	rBV	116	164	0.01%	0.003%
29	4.282	520	524	529	rBV2	691	1393	0.11%	0.024%
30	4.483	544	557	589	rBV2	437839	1249241	100.00%	21.317%
31	5.056	639	651	669	rBV	71245	216810	17.36%	3.700%
32	5.178	669	671	676	rVB3	328	461	0.04%	0.008%
33	5.385	692	705	716	rBV	58715	179956	14.41%	3.071%
34	5.586	736	738	742	rVB	281	235	0.02%	0.004%
35	5.964	789	800	819	rBV2	182073	544324	43.57%	9.289%
36	6.245	844	846	848	rBV	208	155	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042527.D
 Acq On : 24 Jul 2024 18:57
 Operator : JC/MD
 Sample : P3327-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	6.367	861	866	869	rBV3	439	795	0.06%	0.014%
38	6.610	903	906	907	rBV2	192	191	0.02%	0.003%
39	6.763	922	931	946	rBV	167744	407093	32.59%	6.947%
40	7.129	984	991	1002	rBV3	13306	31527	2.52%	0.538%
41	7.214	1002	1005	1008	rBV3	311	380	0.03%	0.006%
42	7.305	1012	1020	1038	rBV	110518	251471	20.13%	4.291%
43	7.488	1047	1050	1053	rBV3	222	280	0.02%	0.005%
44	7.860	1105	1111	1112	rBV	114	249	0.02%	0.004%
45	7.958	1123	1127	1132	rBV2	580	885	0.07%	0.015%
46	8.031	1137	1139	1143	rBV2	123	160	0.01%	0.003%
47	8.324	1182	1187	1202	rBV	61885	108143	8.66%	1.845%
48	8.433	1204	1205	1207	rVV2	336	223	0.02%	0.004%
49	8.458	1207	1209	1212	rVB3	236	164	0.01%	0.003%
50	8.525	1214	1220	1224	rBV4	349	797	0.06%	0.014%
51	8.598	1228	1232	1234	rBV2	355	488	0.04%	0.008%
52	8.647	1234	1240	1249	rVV	253581	405918	32.49%	6.927%
53	8.720	1249	1252	1264	rVB	6880	12668	1.01%	0.216%
54	8.952	1285	1290	1303	rBV	45261	70264	5.62%	1.199%
55	9.159	1320	1324	1330	rVB2	1726	2639	0.21%	0.045%
56	9.281	1339	1344	1348	rBV3	1319	1938	0.16%	0.033%
57	9.390	1356	1362	1380	rBV	173466	274162	21.95%	4.678%
58	9.598	1395	1396	1399	rBV2	242	200	0.02%	0.003%
59	9.665	1405	1407	1411	rVB2	197	177	0.01%	0.003%
60	10.055	1465	1471	1490	rBV	339371	463120	37.07%	7.903%
61	10.201	1490	1495	1499	rVV2	1931	3244	0.26%	0.055%
62	10.238	1499	1501	1507	rVB3	308	565	0.05%	0.010%
63	10.305	1507	1512	1522	rBV2	3360	5006	0.40%	0.085%
64	10.646	1562	1568	1573	rBV4	984	1744	0.14%	0.030%
65	10.969	1616	1621	1625	rBV2	270	523	0.04%	0.009%
66	11.195	1652	1658	1670	rBV	224862	300553	24.06%	5.129%
67	11.311	1675	1677	1681	rVB4	544	621	0.05%	0.011%
68	11.396	1686	1691	1694	rVV2	458	818	0.07%	0.014%
69	11.457	1698	1701	1708	rVB3	453	741	0.06%	0.013%
70	11.616	1723	1727	1732	rBV2	279	335	0.03%	0.006%
71	11.756	1746	1750	1755	rVB2	1247	1790	0.14%	0.031%
72	12.024	1788	1794	1803	rBV	311754	399616	31.99%	6.819%
73	12.219	1823	1826	1837	rVB2	3477	4753	0.38%	0.081%
74	12.317	1837	1842	1855	rBV	293148	371518	29.74%	6.340%
75	12.762	1912	1915	1918	rBV3	642	882	0.07%	0.015%
76	13.786	2080	2083	2087	rBV3	354	509	0.04%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042527.D
 Acq On : 24 Jul 2024 18:57
 Operator : JC/MD
 Sample : P3327-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	13.957	2109	2111	2114	rVB2	187	188	0.02%	0.003%
78	14.005	2117	2119	2122	rVB2	192	154	0.01%	0.003%
79	14.042	2123	2125	2128	rVB2	157	167	0.01%	0.003%
80	14.066	2128	2129	2133	rBV3	163	188	0.02%	0.003%
81	14.134	2135	2140	2143	rBV2	593	907	0.07%	0.015%
82	14.194	2147	2150	2151	rBV	192	197	0.02%	0.003%
83	14.243	2154	2158	2160	rBV2	136	243	0.02%	0.004%
84	14.463	2192	2194	2196	rBV2	146	151	0.01%	0.003%
85	14.512	2200	2202	2205	rBV2	140	196	0.02%	0.003%
86	14.646	2222	2224	2225	rBV	256	186	0.01%	0.003%
87	14.682	2227	2230	2231	rVV3	196	199	0.02%	0.003%
88	14.725	2234	2237	2240	rBV2	195	323	0.03%	0.006%
89	14.810	2249	2251	2254	rBV3	179	154	0.01%	0.003%
90	14.853	2256	2258	2259	rBV	249	153	0.01%	0.003%
91	14.981	2277	2279	2284	rVB3	272	336	0.03%	0.006%
92	15.018	2284	2285	2286	rBV	357	165	0.01%	0.003%
93	15.353	2338	2340	2341	rBV	248	175	0.01%	0.003%
94	15.395	2341	2347	2349	rVV5	906	1340	0.11%	0.023%
95	15.530	2367	2369	2371	rBV2	244	192	0.02%	0.003%
96	16.267	2489	2490	2492	rVB2	351	182	0.01%	0.003%
97	16.389	2508	2510	2512	rVB2	233	169	0.01%	0.003%
98	16.450	2518	2520	2521	rBV	220	187	0.01%	0.003%
99	16.639	2549	2551	2555	rVB3	350	381	0.03%	0.007%
100	16.676	2555	2557	2558	rBV	200	190	0.02%	0.003%

Sum of corrected areas: 5860171




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042527.D
Acq On : 24 Jul 2024 18:57
Operator : JC/MD
Sample : P3327-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

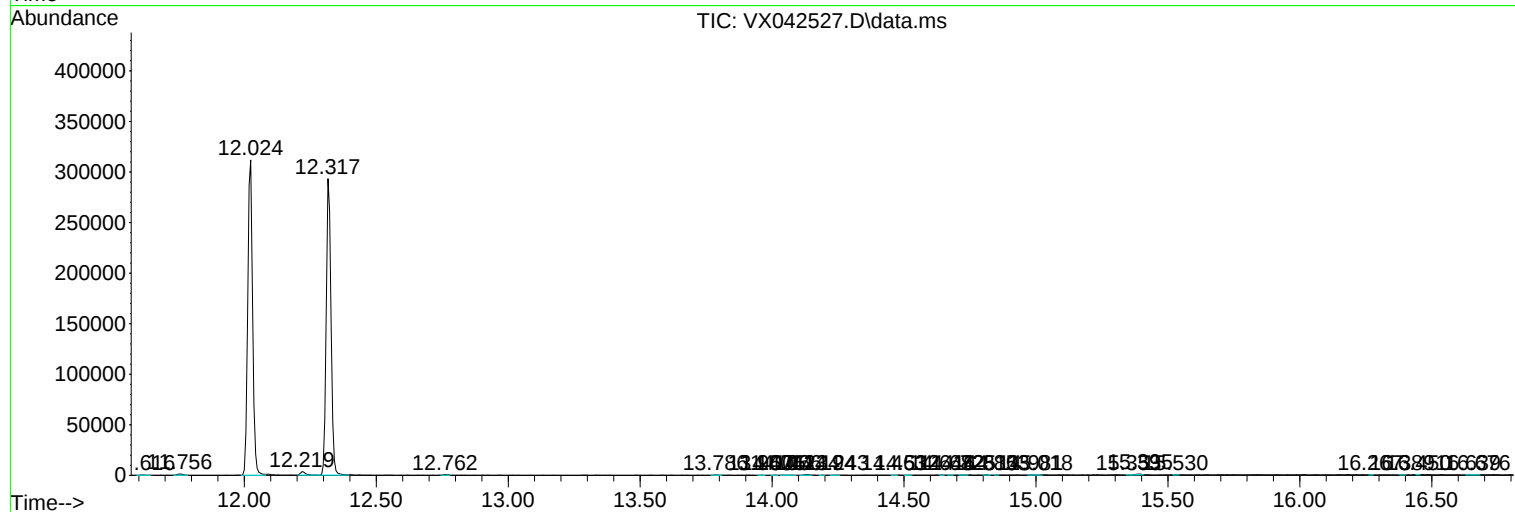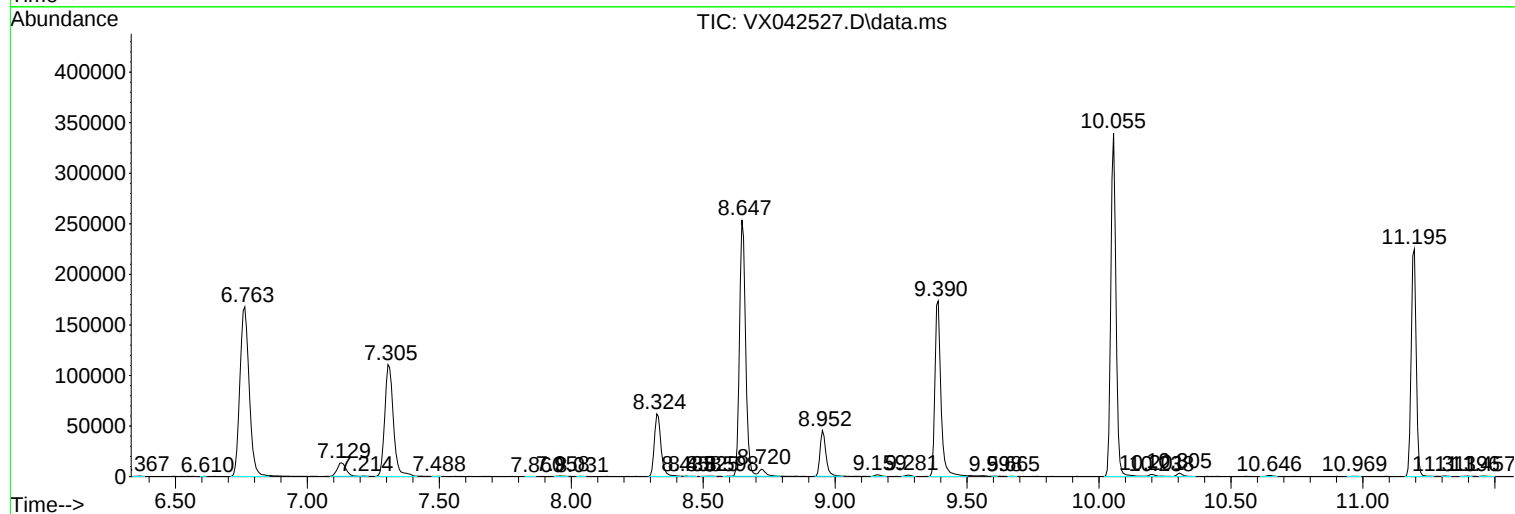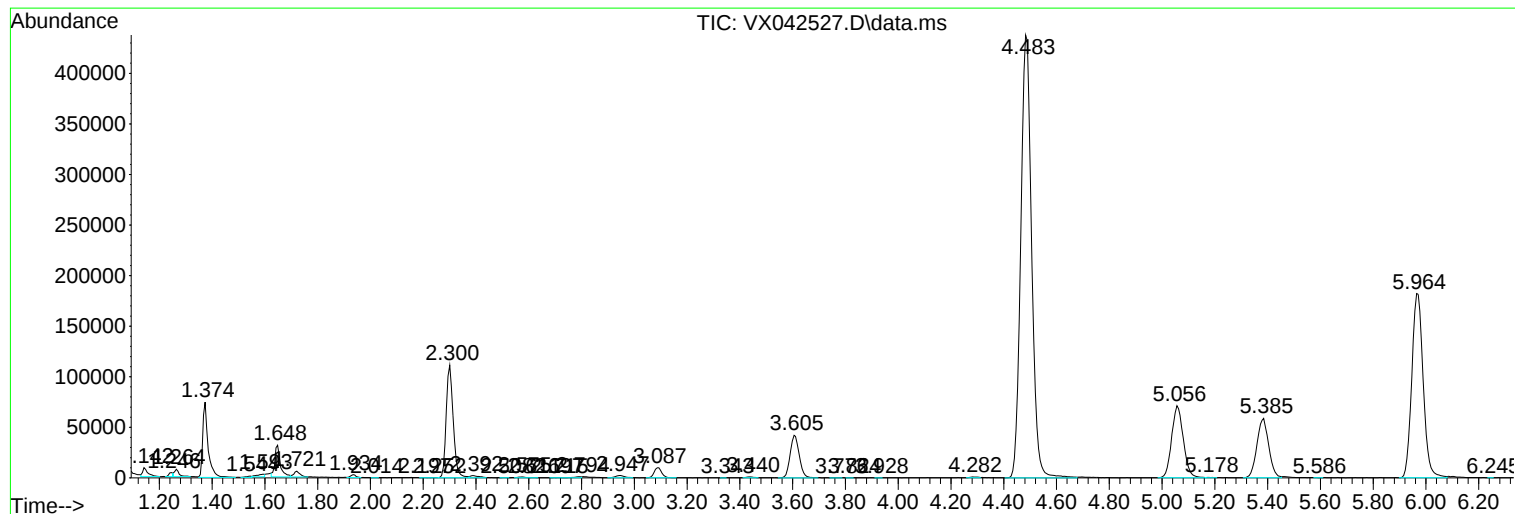

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042527.D
Acq On : 24 Jul 2024 18:57
Operator : JC/MD
Sample : P3327-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042527.D
Acq On : 24 Jul 2024 18:57
Operator : JC/MD
Sample : P3327-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc