

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042530.D
 Acq On : 24 Jul 2024 20:29
 Operator : JC/MD
 Sample : VX0725WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK696

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.245	22	26	27	rBV	3924	4079	0.72%	0.094%
2	1.367	43	46	60	rVB	43207	56245	9.95%	1.291%
3	1.617	71	87	88	rBV5	4159	13797	2.44%	0.317%
4	1.648	88	92	101	rVB	37244	48169	8.52%	1.106%
5	1.910	133	135	138	rBV2	216	207	0.04%	0.005%
6	2.081	161	163	166	rVB3	245	181	0.03%	0.004%
7	2.227	185	187	190	rBV2	279	294	0.05%	0.007%
8	2.300	192	199	211	rVV	106717	172848	30.58%	3.968%
9	2.428	218	220	221	rBV	146	106	0.02%	0.002%
10	2.544	238	239	241	rBV	144	106	0.02%	0.002%
11	2.562	241	242	245	rVV2	169	188	0.03%	0.004%
12	2.599	246	248	251	rVV2	208	228	0.04%	0.005%
13	2.660	254	258	259	rBV2	127	144	0.03%	0.003%
14	2.702	262	265	266	rBV2	169	140	0.02%	0.003%
15	2.788	275	279	285	rVB3	955	1745	0.31%	0.040%
16	2.940	297	304	311	rBV	3072	7223	1.28%	0.166%
17	3.038	316	320	322	rVV	140	161	0.03%	0.004%
18	3.123	331	334	339	rVB2	216	275	0.05%	0.006%
19	3.166	339	341	344	rBV	134	166	0.03%	0.004%
20	3.318	363	366	369	rBV	231	282	0.05%	0.006%
21	3.477	391	392	395	rBV	109	122	0.02%	0.003%
22	3.538	401	402	405	rVB2	133	110	0.02%	0.003%
23	3.617	412	415	416	rVV	135	114	0.02%	0.003%
24	3.629	416	417	420	rVV	91	86	0.02%	0.002%
25	3.653	420	421	424	rVV	84	90	0.02%	0.002%
26	3.708	428	430	433	rVB2	124	99	0.02%	0.002%
27	3.733	433	434	436	rBV	111	94	0.02%	0.002%
28	3.836	447	451	452	rBV	88	100	0.02%	0.002%
29	3.879	456	458	460	rBV	81	76	0.01%	0.002%
30	3.903	460	462	463	rVB	174	101	0.02%	0.002%
31	3.964	468	472	476	rBV2	125	276	0.05%	0.006%
32	4.056	486	487	490	rVB2	100	85	0.02%	0.002%
33	4.464	545	554	573	rBV	42749	127885	22.62%	2.936%
34	5.056	640	651	668	rVV	71912	221644	39.21%	5.088%
35	5.245	681	682	684	rBV2	122	83	0.01%	0.002%
36	5.970	789	801	818	rBV2	191990	565262	100.00%	12.976%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042530.D
 Acq On : 24 Jul 2024 20:29
 Operator : JC/MD
 Sample : VX0725WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK696

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	6.385	868	869	870	rBV	153	95	0.02%	0.002%
38	6.403	870	872	873	rVV	137	83	0.01%	0.002%
39	6.629	907	909	910	rBV	142	122	0.02%	0.003%
40	6.763	922	931	944	rBV	159961	384932	68.10%	8.836%
41	6.970	963	965	966	rBV	134	105	0.02%	0.002%
42	7.037	974	976	978	rBV	143	95	0.02%	0.002%
43	7.122	983	990	999	rBV6	2599	6975	1.23%	0.160%
44	7.226	1001	1007	1009	rBV3	339	721	0.13%	0.017%
45	7.311	1012	1021	1037	rBV	111682	252531	44.68%	5.797%
46	7.445	1041	1043	1044	rVB	169	84	0.01%	0.002%
47	7.488	1048	1050	1052	rBV3	191	149	0.03%	0.003%
48	7.549	1058	1060	1062	rBV	151	150	0.03%	0.003%
49	7.793	1097	1100	1102	rBV2	177	242	0.04%	0.006%
50	7.951	1123	1126	1127	rBV2	232	226	0.04%	0.005%
51	8.128	1153	1155	1156	rBV	144	90	0.02%	0.002%
52	8.244	1172	1174	1175	rBV	194	120	0.02%	0.003%
53	8.323	1181	1187	1203	rBV	65209	112544	19.91%	2.583%
54	8.518	1215	1219	1221	rBV3	228	242	0.04%	0.006%
55	8.592	1229	1231	1234	rBV2	140	147	0.03%	0.003%
56	8.646	1234	1240	1253	rBV	280350	448368	79.32%	10.292%
57	8.951	1285	1290	1305	rBV	47462	72609	12.85%	1.667%
58	9.146	1320	1322	1326	rVB2	92	94	0.02%	0.002%
59	9.213	1331	1333	1335	rBV	117	102	0.02%	0.002%
60	9.281	1340	1344	1349	rVB3	1399	1914	0.34%	0.044%
61	9.384	1356	1361	1379	rBV	178854	280412	49.61%	6.437%
62	9.652	1404	1405	1408	rVB	204	115	0.02%	0.003%
63	9.701	1411	1413	1418	rVV3	673	607	0.11%	0.014%
64	9.756	1421	1422	1426	rBV2	162	253	0.04%	0.006%
65	9.829	1433	1434	1435	rBV	153	93	0.02%	0.002%
66	10.055	1465	1471	1486	rBV	335414	449109	79.45%	10.309%
67	10.311	1509	1513	1517	rVB4	414	661	0.12%	0.015%
68	10.573	1554	1556	1560	rBV	146	157	0.03%	0.004%
69	10.969	1618	1621	1625	rBV3	246	412	0.07%	0.009%
70	11.195	1652	1658	1666	rBV	231612	303033	53.61%	6.956%
71	11.311	1675	1677	1679	rBV2	290	274	0.05%	0.006%
72	11.561	1717	1718	1721	rBV2	182	215	0.04%	0.005%
73	11.695	1737	1740	1741	rBV2	178	232	0.04%	0.005%
74	11.756	1748	1750	1751	rBV	226	226	0.04%	0.005%
75	11.847	1763	1765	1768	rVV	150	112	0.02%	0.003%
76	11.951	1778	1782	1784	rBV2	111	150	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042530.D
 Acq On : 24 Jul 2024 20:29
 Operator : JC/MD
 Sample : VX0725WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK696

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.975	1784	1786	1789	rBV	338	417	0.07%	0.010%
78	12.024	1789	1794	1807	rVV	314594	402173	71.15%	9.232%
79	12.317	1837	1842	1859	rBV	307520	406496	71.91%	9.331%
80	12.530	1876	1877	1879	rBV	152	142	0.03%	0.003%
81	12.567	1882	1883	1884	rBV	178	88	0.02%	0.002%
82	12.615	1890	1891	1894	rBV2	75	87	0.02%	0.002%
83	12.768	1911	1916	1919	rVB3	584	995	0.18%	0.023%
84	12.823	1921	1925	1927	rBV2	190	233	0.04%	0.005%
85	12.938	1940	1944	1945	rBV2	165	254	0.04%	0.006%
86	13.115	1972	1973	1976	rBV2	349	332	0.06%	0.008%
87	13.329	2006	2008	2010	rBV	123	132	0.02%	0.003%
88	13.603	2050	2053	2056	rBV2	262	235	0.04%	0.005%
89	13.646	2058	2060	2061	rBV2	107	80	0.01%	0.002%
90	13.780	2080	2082	2084	rBV2	275	266	0.05%	0.006%
91	13.835	2090	2091	2093	rVB2	172	96	0.02%	0.002%
92	14.017	2118	2121	2122	rBV	101	99	0.02%	0.002%
93	14.066	2128	2129	2132	rBV2	150	174	0.03%	0.004%
94	14.091	2132	2133	2135	rVV2	260	181	0.03%	0.004%
95	14.133	2136	2140	2145	rVB2	793	1264	0.22%	0.029%
96	14.170	2145	2146	2150	rBV2	165	217	0.04%	0.005%
97	14.200	2150	2151	2154	rVV2	176	177	0.03%	0.004%
98	14.255	2158	2160	2162	rBV	284	217	0.04%	0.005%
99	14.658	2225	2226	2228	rVB2	297	172	0.03%	0.004%
100	16.255	2486	2488	2489	rBV	308	178	0.03%	0.004%

Sum of corrected areas: 4356317




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042530.D
Acq On : 24 Jul 2024 20:29
Operator : JC/MD
Sample : VX0725WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK696

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

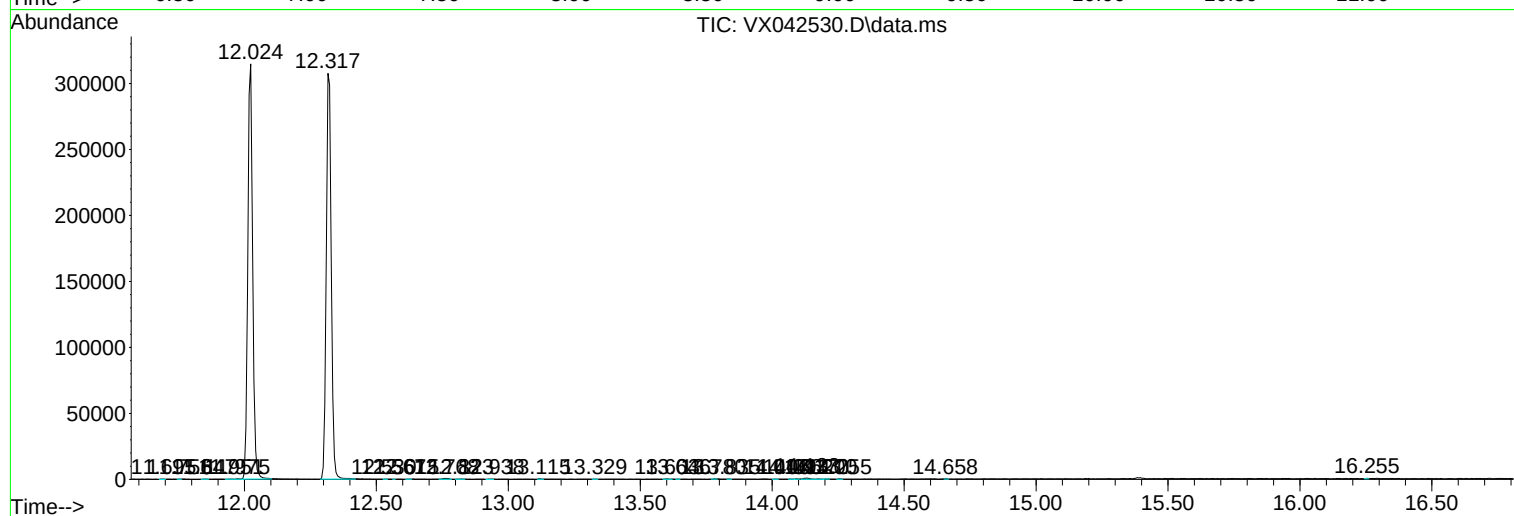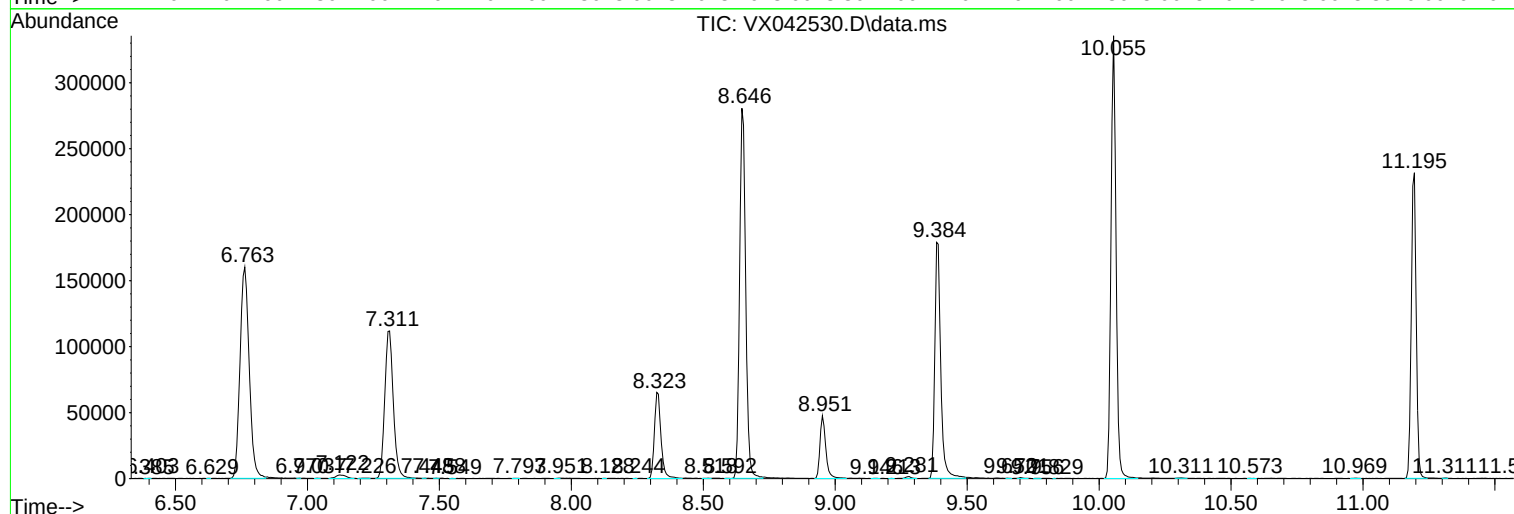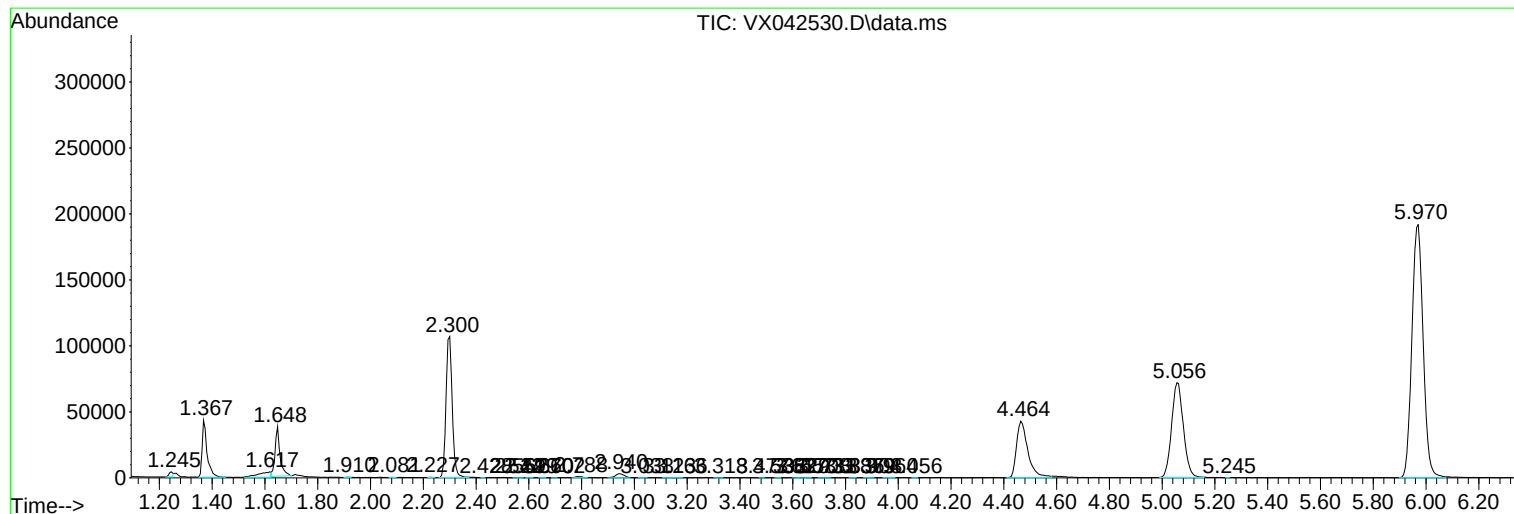

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042530.D
Acq On : 24 Jul 2024 20:29
Operator : JC/MD
Sample : VX0725WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK696

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042530.D
Acq On : 24 Jul 2024 20:29
Operator : JC/MD
Sample : VX0725WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK696

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
