

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042531.D
 Acq On : 24 Jul 2024 20:52
 Operator : JC/MD
 Sample : P3334-06 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	27	rBV	3825	3906	0.77%	0.098%
2	1.367	43	46	57	rBV	34654	42891	8.50%	1.076%
3	1.599	71	84	85	rBV2	3459	8667	1.72%	0.217%
4	1.648	89	92	100	rVB	26896	36341	7.20%	0.912%
5	2.087	162	164	165	rBV	184	123	0.02%	0.003%
6	2.300	192	199	209	rBV	80944	129921	25.74%	3.260%
7	2.459	220	225	226	rVB	146	200	0.04%	0.005%
8	2.568	242	243	247	rBV2	153	138	0.03%	0.003%
9	2.660	256	258	262	rVB	131	149	0.03%	0.004%
10	2.715	265	267	270	rBV	241	251	0.05%	0.006%
11	2.739	270	271	273	rVV	140	84	0.02%	0.002%
12	2.782	274	278	286	rVV2	1616	3461	0.69%	0.087%
13	2.873	290	293	294	rBV	122	121	0.02%	0.003%
14	2.946	297	305	319	rVB	9301	22199	4.40%	0.557%
15	3.056	319	323	325	rBV	157	205	0.04%	0.005%
16	3.117	330	333	334	rBV2	115	112	0.02%	0.003%
17	3.306	363	364	366	rBV2	104	86	0.02%	0.002%
18	3.331	366	368	371	rVV	111	111	0.02%	0.003%
19	3.379	375	376	379	rBV	183	128	0.03%	0.003%
20	3.410	379	381	385	rBV	110	128	0.03%	0.003%
21	3.440	385	386	389	rBV2	154	137	0.03%	0.003%
22	3.513	394	398	399	rBV	153	113	0.02%	0.003%
23	3.587	407	410	412	rBV2	136	158	0.03%	0.004%
24	3.672	420	424	426	rVB	132	126	0.02%	0.003%
25	3.702	426	429	430	rVB	130	123	0.02%	0.003%
26	3.733	430	434	435	rBV	138	186	0.04%	0.005%
27	3.873	452	457	459	rBV2	94	165	0.03%	0.004%
28	3.940	466	468	469	rBV	162	108	0.02%	0.003%
29	3.995	475	477	480	rBV2	100	136	0.03%	0.003%
30	4.117	496	497	502	rBV2	175	187	0.04%	0.005%
31	4.464	546	554	571	rBV	37867	112238	22.23%	2.816%
32	4.769	602	604	606	rBV2	133	127	0.03%	0.003%
33	4.903	625	626	631	rBV2	161	245	0.05%	0.006%
34	4.970	634	637	639	rBV2	133	154	0.03%	0.004%
35	5.062	639	652	666	rBV2	60663	187385	37.12%	4.702%
36	5.318	693	694	697	rVB2	113	90	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042531.D
 Acq On : 24 Jul 2024 20:52
 Operator : JC/MD
 Sample : P3334-06 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.391	705	706	707	rBV	252	135	0.03%	0.003%
38	5.452	714	716	717	rBV	106	101	0.02%	0.003%
39	5.635	742	746	748	rBV2	185	297	0.06%	0.007%
40	5.665	748	751	753	rVV	129	134	0.03%	0.003%
41	5.818	774	776	778	rBV	123	116	0.02%	0.003%
42	5.970	789	801	820	rBV2	153746	458729	90.87%	11.510%
43	6.763	922	931	948	rBV	182704	436319	86.43%	10.948%
44	7.129	984	991	1000	rBV6	2604	6912	1.37%	0.173%
45	7.312	1012	1021	1035	rBV	94114	210866	41.77%	5.291%
46	7.433	1039	1041	1044	rVB3	367	335	0.07%	0.008%
47	7.464	1044	1046	1047	rBV	140	132	0.03%	0.003%
48	7.708	1085	1086	1089	rVB2	141	117	0.02%	0.003%
49	7.732	1089	1090	1093	rBV	148	172	0.03%	0.004%
50	7.793	1098	1100	1102	rVV	119	119	0.02%	0.003%
51	7.848	1106	1109	1112	rBV	219	259	0.05%	0.006%
52	7.915	1119	1120	1122	rVB2	168	102	0.02%	0.003%
53	7.970	1122	1129	1132	rBV3	377	771	0.15%	0.019%
54	8.147	1156	1158	1160	rVB	173	145	0.03%	0.004%
55	8.165	1160	1161	1162	rBV	174	90	0.02%	0.002%
56	8.269	1176	1178	1179	rVB	162	98	0.02%	0.002%
57	8.324	1181	1187	1202	rVV	52390	91355	18.10%	2.292%
58	8.513	1215	1218	1220	rBV2	280	378	0.07%	0.009%
59	8.647	1234	1240	1255	rBV	218408	350713	69.47%	8.800%
60	8.951	1285	1290	1303	rBV	38822	58376	11.56%	1.465%
61	9.238	1335	1337	1339	rBV	160	131	0.03%	0.003%
62	9.275	1339	1343	1347	rVB4	1600	2184	0.43%	0.055%
63	9.384	1356	1361	1381	rBV	156955	245090	48.55%	6.150%
64	9.701	1409	1413	1422	rBV	1652	2215	0.44%	0.056%
65	9.842	1434	1436	1437	rVB	145	90	0.02%	0.002%
66	9.866	1437	1440	1441	rBV	162	188	0.04%	0.005%
67	9.994	1457	1461	1462	rBV	155	197	0.04%	0.005%
68	10.055	1465	1471	1484	rBV	371539	504822	100.00%	12.667%
69	10.305	1510	1512	1515	rBV2	283	308	0.06%	0.008%
70	10.604	1560	1561	1564	rVB	163	120	0.02%	0.003%
71	10.658	1564	1570	1572	rBV2	214	370	0.07%	0.009%
72	11.085	1635	1640	1641	rBV2	81	120	0.02%	0.003%
73	11.195	1652	1658	1670	rBV	199028	263196	52.14%	6.604%
74	11.317	1675	1678	1681	rVV3	416	446	0.09%	0.011%
75	11.378	1684	1688	1691	rBV2	86	104	0.02%	0.003%
76	11.457	1699	1701	1703	rBV	257	179	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042531.D
 Acq On : 24 Jul 2024 20:52
 Operator : JC/MD
 Sample : P3334-06 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.500	1706	1708	1712	rBV	162	154	0.03%	0.004%
78	11.603	1723	1725	1726	rBV2	83	89	0.02%	0.002%
79	11.664	1734	1735	1737	rBV2	162	103	0.02%	0.003%
80	11.756	1748	1750	1756	rVB3	239	389	0.08%	0.010%
81	11.811	1756	1759	1761	rBV2	156	175	0.03%	0.004%
82	11.908	1774	1775	1776	rBV	182	89	0.02%	0.002%
83	11.981	1784	1787	1788	rBV2	315	328	0.06%	0.008%
84	12.024	1788	1794	1803	rBV	346077	455122	90.15%	11.420%
85	12.317	1837	1842	1858	rBV	261186	336259	66.61%	8.437%
86	12.579	1883	1885	1886	rBV	141	94	0.02%	0.002%
87	12.762	1911	1915	1919	rVB2	1009	1423	0.28%	0.036%
88	12.951	1943	1946	1947	rBV	178	187	0.04%	0.005%
89	13.042	1959	1961	1964	rBV	149	156	0.03%	0.004%
90	13.121	1971	1974	1976	rBV	154	197	0.04%	0.005%
91	13.292	2000	2002	2004	rBV2	97	90	0.02%	0.002%
92	13.317	2004	2006	2010	rVB2	157	172	0.03%	0.004%
93	13.353	2010	2012	2015	rBV	127	125	0.02%	0.003%
94	13.457	2028	2029	2031	rVB2	156	102	0.02%	0.003%
95	13.603	2051	2053	2058	rVB2	234	186	0.04%	0.005%
96	13.792	2081	2084	2085	rBV	239	219	0.04%	0.005%
97	14.054	2124	2127	2129	rBV2	180	252	0.05%	0.006%
98	14.127	2134	2139	2142	rBV2	1150	1685	0.33%	0.042%
99	14.670	2225	2228	2230	rBV2	217	271	0.05%	0.007%
100	14.914	2267	2268	2269	rBV	220	107	0.02%	0.003%




Sum of corrected areas: 3985405

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042531.D
Acq On : 24 Jul 2024 20:52
Operator : JC/MD
Sample : P3334-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

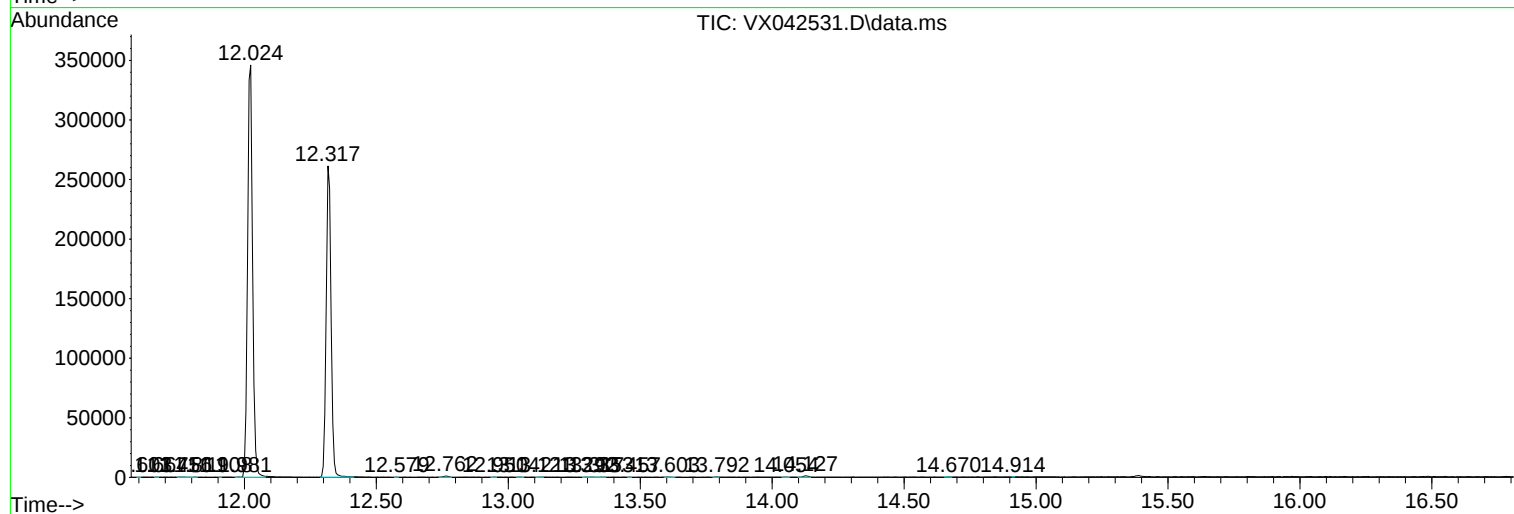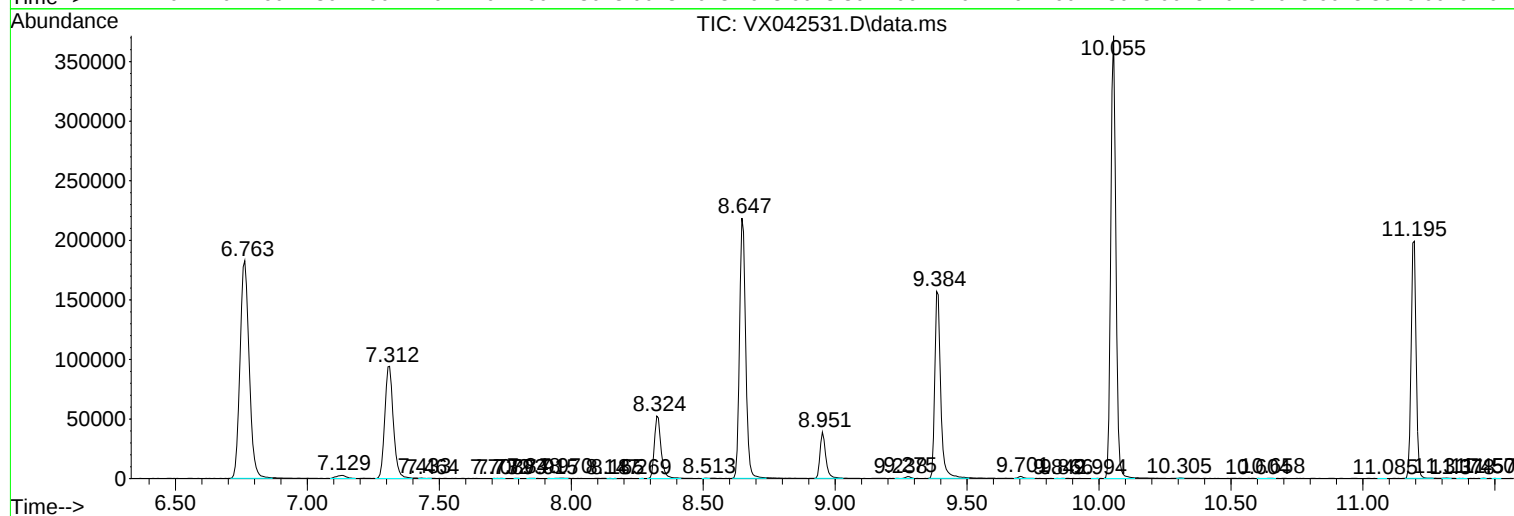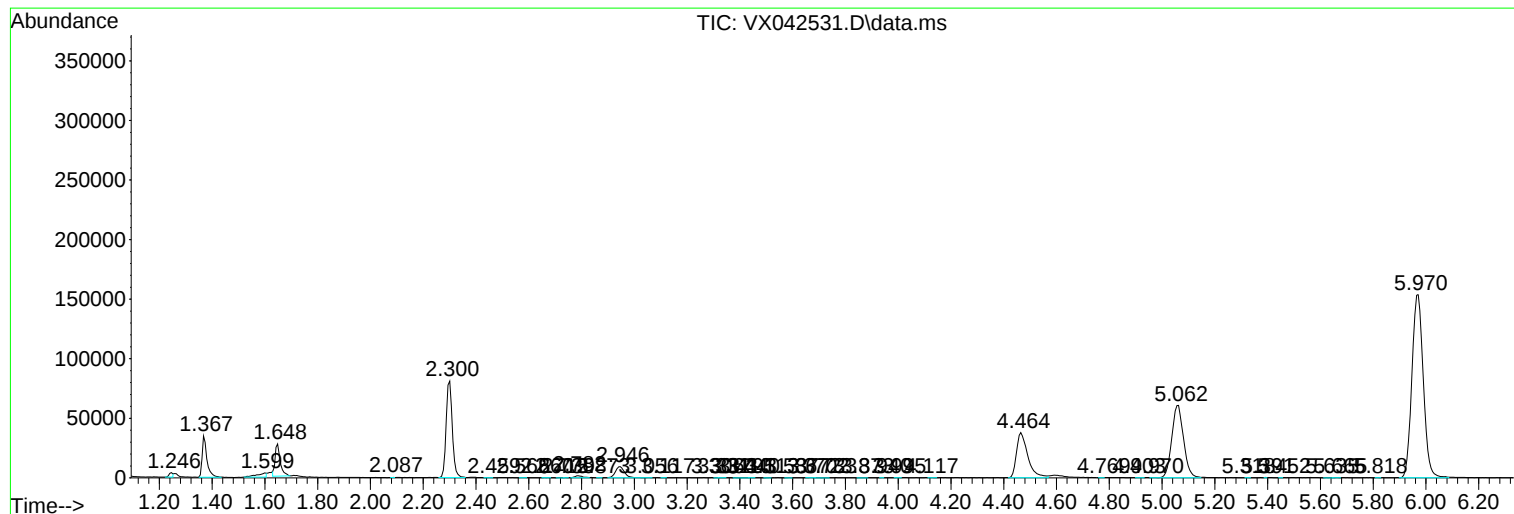

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042531.D
Acq On : 24 Jul 2024 20:52
Operator : JC/MD
Sample : P3334-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042531.D
Acq On : 24 Jul 2024 20:52
Operator : JC/MD
Sample : P3334-06 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc