

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042538.D
 Acq On : 24 Jul 2024 23:34
 Operator : JC/MD
 Sample : P3334-11 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.215	19	21	23	rBV	248	156	0.01%	0.003%
2	1.246	23	26	27	rBV	3444	3553	0.23%	0.066%
3	1.368	43	46	59	rVB	31802	42078	2.72%	0.783%
4	1.477	62	64	68	rBV	188	275	0.02%	0.005%
5	1.508	68	69	71	rBV	198	199	0.01%	0.004%
6	1.550	71	76	77	rBV	1461	2091	0.14%	0.039%
7	1.599	77	84	85	rVV2	2651	5489	0.35%	0.102%
8	1.648	88	92	100	rVB	25692	37418	2.42%	0.697%
9	1.849	123	125	130	rVB2	171	218	0.01%	0.004%
10	1.995	148	149	154	rVB2	280	299	0.02%	0.006%
11	2.075	159	162	163	rBV2	223	235	0.02%	0.004%
12	2.233	186	188	190	rVV2	163	173	0.01%	0.003%
13	2.300	193	199	211	rVB	78082	122473	7.92%	2.280%
14	2.392	211	214	218	rBV2	351	447	0.03%	0.008%
15	2.501	230	232	236	rVB3	150	142	0.01%	0.003%
16	2.569	238	243	244	rVB2	246	331	0.02%	0.006%
17	2.587	244	246	248	rBV	134	143	0.01%	0.003%
18	2.788	273	279	288	rVV	2377	5030	0.33%	0.094%
19	2.855	288	290	292	rVB	156	137	0.01%	0.003%
20	2.886	292	295	297	rBV	120	154	0.01%	0.003%
21	2.947	297	305	318	rVB	8628	20082	1.30%	0.374%
22	3.044	318	321	323	rBV2	146	178	0.01%	0.003%
23	3.087	326	328	331	rBV	224	214	0.01%	0.004%
24	3.379	373	376	378	rVB	207	248	0.02%	0.005%
25	3.404	378	380	383	rBV	197	229	0.01%	0.004%
26	3.611	408	414	420	rVB	989	2119	0.14%	0.039%
27	3.690	424	427	429	rVB2	156	146	0.01%	0.003%
28	3.812	445	447	450	rBV	157	222	0.01%	0.004%
29	3.843	450	452	456	rBV	92	122	0.01%	0.002%
30	3.934	464	467	469	rBV	138	172	0.01%	0.003%
31	3.977	472	474	478	rVB2	182	247	0.02%	0.005%
32	4.032	478	483	484	rBV2	154	240	0.02%	0.004%
33	4.251	517	519	524	rVB2	131	194	0.01%	0.004%
34	4.300	524	527	532	rBV2	127	142	0.01%	0.003%
35	4.471	546	555	568	rBV2	46326	154345	9.98%	2.873%
36	5.056	639	651	669	rBV2	59180	186608	12.07%	3.474%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042538.D
 Acq On : 24 Jul 2024 23:34
 Operator : JC/MD
 Sample : P3334-11 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.397	704	707	710	rVB2	114	140	0.01%	0.003%
38	5.550	730	732	733	rBV2	142	136	0.01%	0.003%
39	5.800	770	773	776	rBV2	169	293	0.02%	0.005%
40	5.964	789	800	821	rBV2	152223	453743	29.35%	8.447%
41	6.251	843	847	852	rVB2	137	226	0.01%	0.004%
42	6.495	885	887	890	rVB	199	195	0.01%	0.004%
43	6.562	896	898	902	rVB2	163	239	0.02%	0.004%
44	6.604	902	905	908	rBV2	143	207	0.01%	0.004%
45	6.671	913	916	918	rBV2	126	125	0.01%	0.002%
46	6.763	922	931	955	rBV	160979	388421	25.12%	7.231%
47	7.062	976	980	981	rBV2	157	162	0.01%	0.003%
48	7.123	981	990	1011	rVV	716114	1546228	100.00%	28.786%
49	7.305	1012	1020	1040	rVV	95448	216381	13.99%	4.028%
50	7.452	1042	1044	1047	rVV2	223	180	0.01%	0.003%
51	7.854	1109	1110	1113	rVB	174	136	0.01%	0.003%
52	7.958	1124	1127	1128	rBV	334	333	0.02%	0.006%
53	7.976	1128	1130	1133	rVB2	111	129	0.01%	0.002%
54	8.324	1181	1187	1203	rBV	50849	88984	5.75%	1.657%
55	8.470	1208	1211	1213	rBV	98	141	0.01%	0.003%
56	8.507	1216	1217	1219	rBV	192	158	0.01%	0.003%
57	8.555	1223	1225	1228	rVB	141	136	0.01%	0.003%
58	8.647	1233	1240	1250	rBV	207970	332951	21.53%	6.198%
59	8.952	1285	1290	1306	rBV2	36771	57255	3.70%	1.066%
60	9.189	1328	1329	1331	rBV	204	167	0.01%	0.003%
61	9.275	1339	1343	1349	rVB3	1691	2480	0.16%	0.046%
62	9.336	1349	1353	1356	rBV2	199	272	0.02%	0.005%
63	9.384	1356	1361	1377	rBV	167672	254350	16.45%	4.735%
64	9.647	1402	1404	1409	rVB2	172	172	0.01%	0.003%
65	9.701	1409	1413	1419	rVB2	1778	2741	0.18%	0.051%
66	10.055	1465	1471	1488	rVV	321879	445380	28.80%	8.291%
67	10.207	1494	1496	1498	rVB2	195	162	0.01%	0.003%
68	10.317	1510	1514	1518	rBV2	341	468	0.03%	0.009%
69	10.457	1535	1537	1541	rVB	171	136	0.01%	0.003%
70	10.488	1541	1542	1544	rVB	205	129	0.01%	0.002%
71	10.518	1544	1547	1548	rBV2	194	213	0.01%	0.004%
72	10.969	1618	1621	1626	rVV3	204	310	0.02%	0.006%
73	11.018	1626	1629	1631	rVV2	91	135	0.01%	0.003%
74	11.189	1652	1657	1668	rVV	205060	268726	17.38%	5.003%
75	11.311	1675	1677	1682	rVB3	366	438	0.03%	0.008%
76	11.555	1716	1717	1721	rBV	153	194	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042538.D
 Acq On : 24 Jul 2024 23:34
 Operator : JC/MD
 Sample : P3334-11 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	12.024	1788	1794	1807	rBV	293998	393398	25.44%	7.324%
78	12.256	1829	1832	1833	rVB2	178	147	0.01%	0.003%
79	12.280	1833	1836	1837	rBV	146	136	0.01%	0.003%
80	12.317	1837	1842	1851	rBV	252606	318889	20.62%	5.937%
81	12.762	1911	1915	1919	rVV3	801	1184	0.08%	0.022%
82	13.347	2008	2011	2013	rVB	178	192	0.01%	0.004%
83	13.378	2013	2016	2019	rBV2	177	243	0.02%	0.005%
84	13.676	2062	2065	2068	rBV2	148	161	0.01%	0.003%
85	13.780	2080	2082	2086	rVV2	156	239	0.02%	0.004%
86	13.829	2089	2090	2093	rVB2	160	123	0.01%	0.002%
87	14.042	2124	2125	2129	rVB2	183	170	0.01%	0.003%
88	14.127	2135	2139	2144	rVB	1410	1859	0.12%	0.035%
89	14.201	2149	2151	2154	rVB2	145	153	0.01%	0.003%
90	14.438	2189	2190	2195	rVB2	238	164	0.01%	0.003%
91	14.512	2199	2202	2204	rBV2	143	132	0.01%	0.002%
92	14.603	2215	2217	2219	rVB2	216	161	0.01%	0.003%
93	14.694	2231	2232	2235	rBV2	202	246	0.02%	0.005%
94	15.243	2320	2322	2323	rBV3	199	173	0.01%	0.003%
95	15.389	2341	2346	2350	rVB3	1810	2740	0.18%	0.051%
96	15.487	2361	2362	2364	rBV	317	267	0.02%	0.005%
97	15.664	2389	2391	2393	rBV2	217	177	0.01%	0.003%
98	16.499	2526	2528	2531	rBV2	162	153	0.01%	0.003%
99	16.670	2552	2556	2558	rVB3	244	293	0.02%	0.005%
100	16.749	2567	2569	2570	rBV	361	229	0.01%	0.004%




Sum of corrected areas: 5371550

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042538.D
Acq On : 24 Jul 2024 23:34
Operator : JC/MD
Sample : P3334-11 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

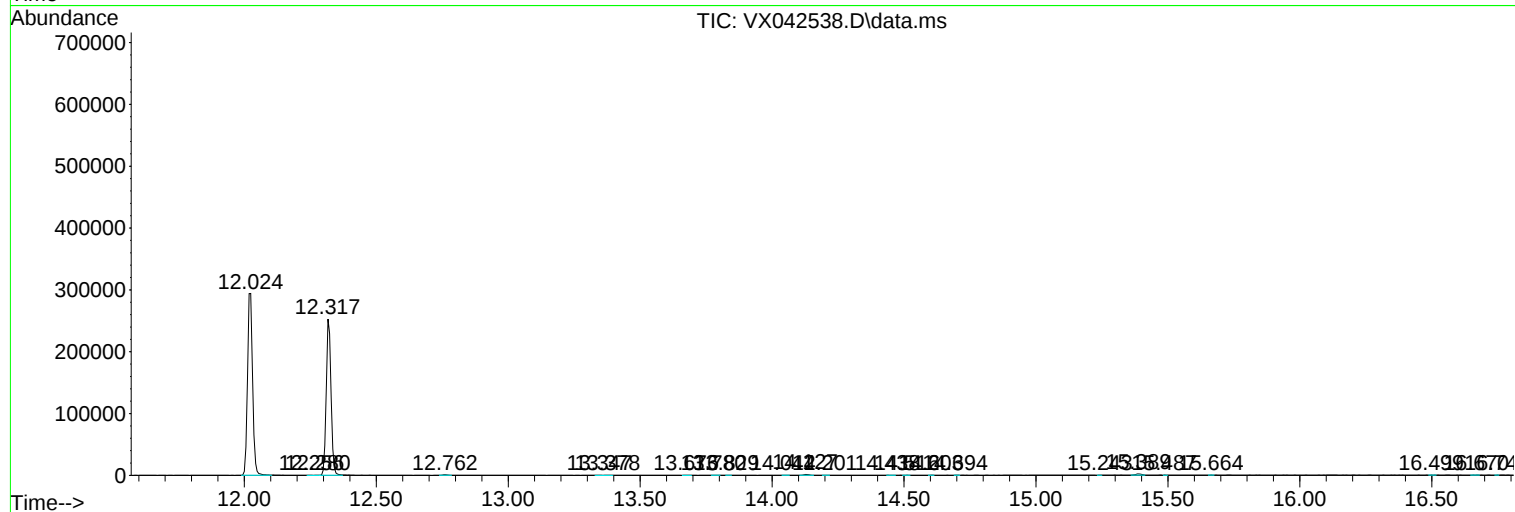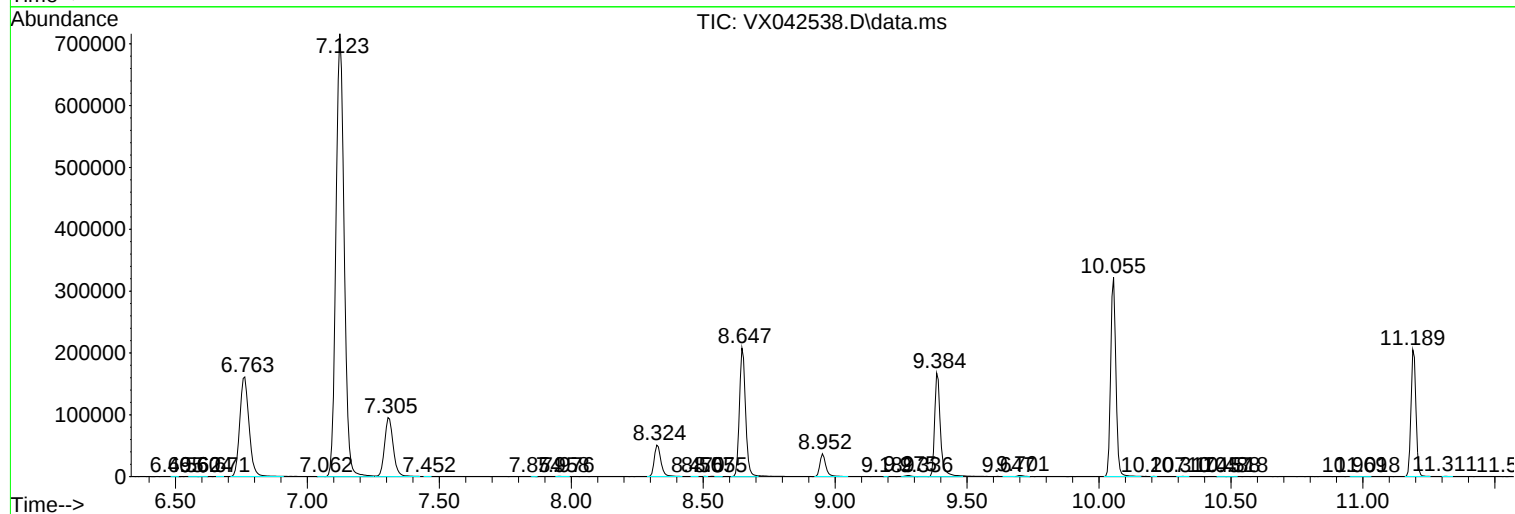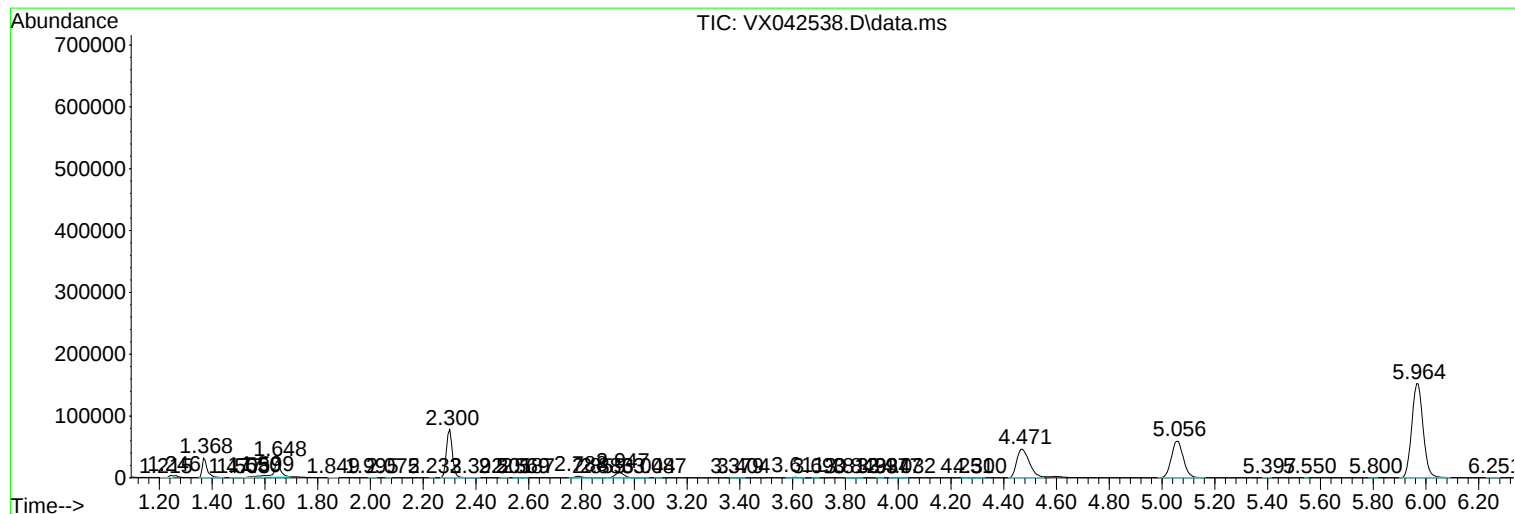

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042538.D
Acq On : 24 Jul 2024 23:34
Operator : JC/MD
Sample : P3334-11 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042538.D
Acq On : 24 Jul 2024 23:34
Operator : JC/MD
Sample : P3334-11 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc