

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042539.D
 Acq On : 24 Jul 2024 23:57
 Operator : JC/MD
 Sample : P3334-09 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042539.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.160	10	12	14	rBV	230	192	0.04%	0.005%
2	1.246	23	26	27	rBV	3052	3151	0.65%	0.079%
3	1.368	43	46	61	rVB	33734	43280	8.98%	1.084%
4	1.575	78	80	81	rBV	1103	944	0.20%	0.024%
5	1.648	88	92	101	rVB	30228	40272	8.36%	1.009%
6	1.807	117	118	121	rVB	354	256	0.05%	0.006%
7	1.880	128	130	132	rVB	326	239	0.05%	0.006%
8	1.916	134	136	137	rVV2	224	181	0.04%	0.005%
9	1.947	139	141	143	rBV	256	172	0.04%	0.004%
10	1.989	145	148	150	rBV2	216	267	0.06%	0.007%
11	2.063	158	160	161	rBV	167	143	0.03%	0.004%
12	2.081	161	163	166	rVV	223	247	0.05%	0.006%
13	2.148	171	174	176	rVV	253	297	0.06%	0.007%
14	2.184	178	180	182	rVB	214	201	0.04%	0.005%
15	2.233	186	188	191	rVV	178	188	0.04%	0.005%
16	2.300	192	199	211	rVB	82105	133284	27.66%	3.339%
17	2.392	211	214	218	rBV3	315	552	0.11%	0.014%
18	2.703	263	265	267	rVV2	144	151	0.03%	0.004%
19	2.788	274	279	287	rVB4	1643	3446	0.72%	0.086%
20	2.947	297	305	318	rVB	7253	18041	3.74%	0.452%
21	3.062	318	324	325	rBV2	184	333	0.07%	0.008%
22	3.209	346	348	353	rVB2	185	309	0.06%	0.008%
23	3.282	355	360	361	rVV2	92	161	0.03%	0.004%
24	3.459	388	389	391	rBV2	193	171	0.04%	0.004%
25	3.489	391	394	397	rBV2	171	229	0.05%	0.006%
26	3.550	403	404	406	rBV2	197	150	0.03%	0.004%
27	3.587	409	410	413	rVV	125	144	0.03%	0.004%
28	3.617	413	415	419	rVV2	118	155	0.03%	0.004%
29	3.733	432	434	438	rVB	177	179	0.04%	0.004%
30	3.782	438	442	445	rVB	93	153	0.03%	0.004%
31	3.965	469	472	476	rBV	149	214	0.04%	0.005%
32	4.215	512	513	518	rVV	163	184	0.04%	0.005%
33	4.465	546	554	568	rBV	40179	118329	24.56%	2.964%
34	4.757	599	602	603	rVB2	153	152	0.03%	0.004%
35	5.056	638	651	672	rVV2	63319	197144	40.91%	4.938%
36	5.239	678	681	684	rBV2	259	313	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042539.D
 Acq On : 24 Jul 2024 23:57
 Operator : JC/MD
 Sample : P3334-09 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.361	700	701	703	rBV	190	178	0.04%	0.004%
38	5.544	728	731	732	rVB	212	156	0.03%	0.004%
39	5.568	732	735	736	rBV2	174	202	0.04%	0.005%
40	5.861	780	783	786	rVV	171	215	0.04%	0.005%
41	5.964	790	800	826	rVV2	161938	481875	100.00%	12.070%
42	6.550	893	896	899	rVB2	125	146	0.03%	0.004%
43	6.763	922	931	948	rBV	172901	416469	86.43%	10.432%
44	7.062	978	980	983	rVB	233	154	0.03%	0.004%
45	7.129	983	991	1001	rBV5	4977	12823	2.66%	0.321%
46	7.306	1012	1020	1039	rVV	101096	221383	45.94%	5.545%
47	7.714	1086	1087	1091	rVB	163	166	0.03%	0.004%
48	7.812	1101	1103	1104	rVB	196	141	0.03%	0.004%
49	7.842	1104	1108	1109	rBV	164	204	0.04%	0.005%
50	8.324	1182	1187	1200	rVV	53339	90444	18.77%	2.265%
51	8.409	1200	1201	1203	rVB	336	154	0.03%	0.004%
52	8.507	1214	1217	1218	rBV2	231	247	0.05%	0.006%
53	8.525	1218	1220	1223	rVB	218	190	0.04%	0.005%
54	8.647	1234	1240	1257	rBV	230823	363758	75.49%	9.112%
55	8.756	1257	1258	1259	rBV	274	152	0.03%	0.004%
56	8.952	1285	1290	1306	rVV	38819	59651	12.38%	1.494%
57	9.110	1314	1316	1320	rVB2	192	288	0.06%	0.007%
58	9.153	1320	1323	1325	rBV	134	186	0.04%	0.005%
59	9.189	1327	1329	1334	rBV2	92	189	0.04%	0.005%
60	9.275	1340	1343	1349	rVB4	1049	1565	0.32%	0.039%
61	9.384	1356	1361	1375	rBV	168025	255851	53.09%	6.409%
62	9.549	1386	1388	1391	rVB3	229	225	0.05%	0.006%
63	9.701	1409	1413	1423	rVB2	1192	1966	0.41%	0.049%
64	9.793	1425	1428	1432	rBV2	81	162	0.03%	0.004%
65	10.055	1465	1471	1486	rBV	342236	472308	98.01%	11.831%
66	10.311	1510	1513	1514	rBV2	282	361	0.07%	0.009%
67	10.482	1537	1541	1542	rBV	204	206	0.04%	0.005%
68	10.713	1576	1579	1582	rBV	118	153	0.03%	0.004%
69	10.744	1582	1584	1586	rVV2	110	139	0.03%	0.003%
70	11.189	1652	1657	1670	rBV	206909	274275	56.92%	6.870%
71	11.476	1701	1704	1707	rVB2	134	183	0.04%	0.005%
72	11.756	1748	1750	1752	rVB2	181	161	0.03%	0.004%
73	12.018	1788	1793	1806	rBV	325046	419642	87.09%	10.511%
74	12.171	1816	1818	1824	rVB3	250	246	0.05%	0.006%
75	12.268	1832	1834	1837	rBV2	135	146	0.03%	0.004%
76	12.317	1837	1842	1854	rVV	262814	341390	70.85%	8.551%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042539.D
 Acq On : 24 Jul 2024 23:57
 Operator : JC/MD
 Sample : P3334-09 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20F2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	12.420	1857	1859	1861	rVV3	403	428	0.09%	0.011%
78	12.463	1864	1866	1869	rVB	320	255	0.05%	0.006%
79	12.683	1898	1902	1903	rBV2	132	170	0.04%	0.004%
80	12.756	1911	1914	1919	rVB2	810	1086	0.23%	0.027%
81	13.676	2063	2065	2067	rBV	179	161	0.03%	0.004%
82	14.006	2117	2119	2122	rVB2	142	156	0.03%	0.004%
83	14.048	2122	2126	2127	rBV	133	161	0.03%	0.004%
84	14.127	2135	2139	2143	rBV	1046	1571	0.33%	0.039%
85	14.219	2152	2154	2157	rBV2	125	203	0.04%	0.005%
86	14.268	2159	2162	2163	rVB2	169	153	0.03%	0.004%
87	14.530	2202	2205	2207	rBV2	172	234	0.05%	0.006%
88	14.670	2227	2228	2233	rBV3	189	270	0.06%	0.007%
89	14.786	2245	2247	2250	rBV	206	258	0.05%	0.006%
90	14.944	2271	2273	2276	rVB2	231	253	0.05%	0.006%
91	14.975	2276	2278	2280	rBV2	268	204	0.04%	0.005%
92	15.011	2280	2284	2286	rBV3	237	332	0.07%	0.008%
93	15.127	2301	2303	2304	rVB	274	169	0.04%	0.004%
94	15.139	2304	2305	2307	rBV	185	157	0.03%	0.004%
95	15.292	2328	2330	2332	rVB2	223	142	0.03%	0.004%
96	15.389	2341	2346	2351	rBV2	1749	2765	0.57%	0.069%
97	15.481	2359	2361	2365	rBV3	263	335	0.07%	0.008%
98	15.597	2379	2380	2383	rBV3	252	243	0.05%	0.006%
99	15.822	2416	2417	2419	rBV	230	161	0.03%	0.004%
100	15.969	2439	2441	2444	rBV3	192	240	0.05%	0.006%




Sum of corrected areas: 3992281

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042539.D
Acq On : 24 Jul 2024 23:57
Operator : JC/MD
Sample : P3334-09 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

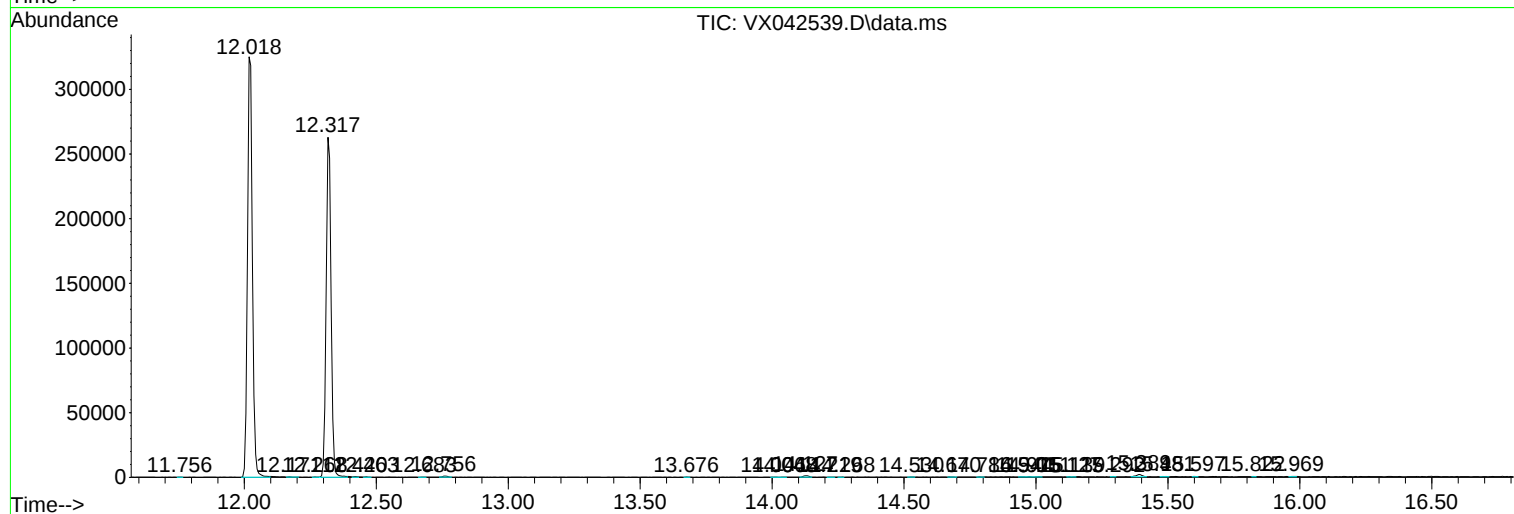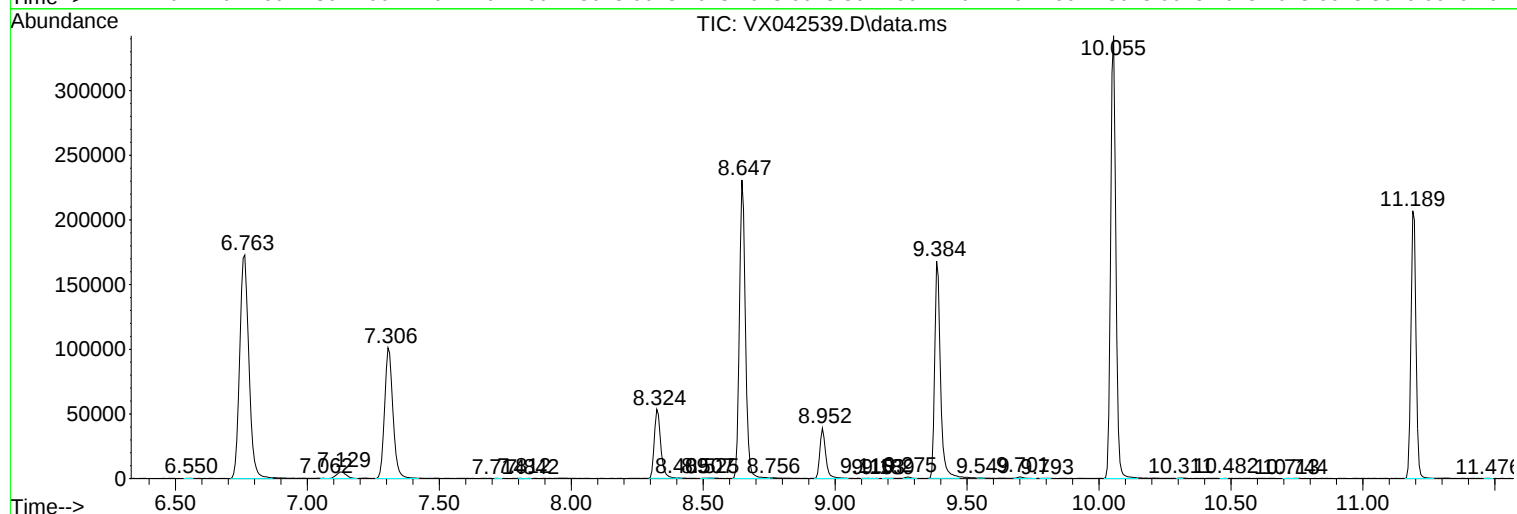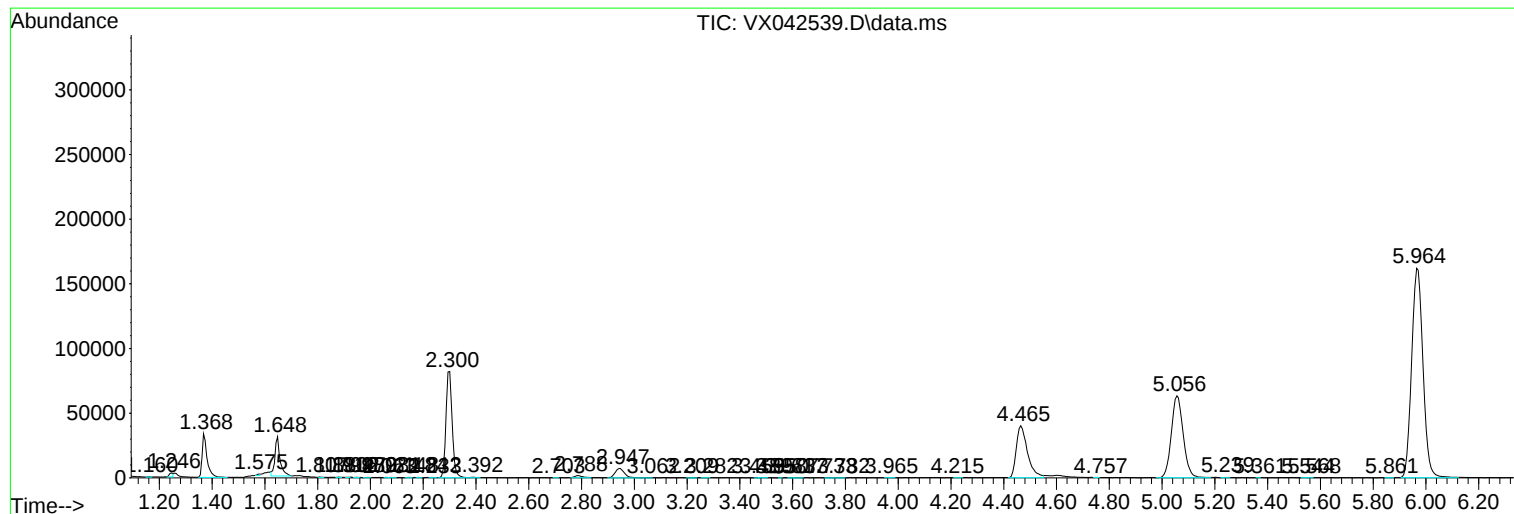

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042539.D
Acq On : 24 Jul 2024 23:57
Operator : JC/MD
Sample : P3334-09 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042539.D
Acq On : 24 Jul 2024 23:57
Operator : JC/MD
Sample : P3334-09 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20F2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc