

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042544.D
 Acq On : 25 Jul 2024 01:52
 Operator : JC/MD
 Sample : P3344-07 100X
 Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BHB23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

Signal : TIC: VX042544.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV2	3350	3258	0.68%	0.083%
2	1.368	43	46	60	rVB	31670	40875	8.58%	1.043%
3	1.612	71	86	88	rBV5	4080	14449	3.03%	0.369%
4	1.648	88	92	101	rVB	28975	40548	8.51%	1.034%
5	2.093	163	165	167	rVB	207	170	0.04%	0.004%
6	2.118	167	169	172	rBV2	149	155	0.03%	0.004%
7	2.227	185	187	188	rBV	231	165	0.03%	0.004%
8	2.300	192	199	211	rBV	77747	125691	26.37%	3.206%
9	2.386	211	213	214	rBV	238	169	0.04%	0.004%
10	2.447	221	223	224	rBV	140	103	0.02%	0.003%
11	2.605	246	249	251	rBV2	127	145	0.03%	0.004%
12	2.648	254	256	258	rBB	156	143	0.03%	0.004%
13	2.672	258	260	263	rVB	116	116	0.02%	0.003%
14	2.697	263	264	266	rBV2	209	195	0.04%	0.005%
15	2.782	273	278	286	rVB3	1145	2285	0.48%	0.058%
16	2.855	288	290	292	rBV	101	101	0.02%	0.003%
17	2.947	297	305	312	rBV	5850	13174	2.76%	0.336%
18	3.044	317	321	323	rVB	168	159	0.03%	0.004%
19	3.123	332	334	338	rBV	168	236	0.05%	0.006%
20	3.172	340	342	344	rBV	154	173	0.04%	0.004%
21	3.264	355	357	360	rBV2	142	180	0.04%	0.005%
22	3.337	368	369	371	rVB	196	108	0.02%	0.003%
23	3.361	371	373	375	rBV2	152	144	0.03%	0.004%
24	3.416	381	382	384	rBV	164	95	0.02%	0.002%
25	3.623	412	416	419	rVB2	101	150	0.03%	0.004%
26	3.672	422	424	427	rBV2	126	109	0.02%	0.003%
27	3.770	438	440	442	rBV2	145	130	0.03%	0.003%
28	3.831	446	450	451	rBV	146	129	0.03%	0.003%
29	3.855	451	454	457	rBV2	131	170	0.04%	0.004%
30	3.953	468	470	473	rBV2	83	101	0.02%	0.003%
31	4.203	509	511	513	rBV	193	181	0.04%	0.005%
32	4.233	515	516	518	rBV2	95	96	0.02%	0.002%
33	4.459	546	553	570	rBV	39160	119261	25.02%	3.042%
34	5.056	639	651	668	rBV	65613	197021	41.34%	5.025%
35	5.367	700	702	705	rVB	140	172	0.04%	0.004%
36	5.397	705	707	709	rBV2	184	189	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042544.D
 Acq On : 25 Jul 2024 01:52
 Operator : JC/MD
 Sample : P3344-07 100X
 Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BHB23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.532	725	729	730	rBV	130	168	0.04%	0.004%
38	5.739	759	763	764	rBV	139	159	0.03%	0.004%
39	5.964	789	800	824	rBV2	160045	476581	100.00%	12.155%
40	6.202	838	839	840	rBV	210	114	0.02%	0.003%
41	6.324	857	859	864	rBV	138	154	0.03%	0.004%
42	6.556	893	897	898	rBV	219	249	0.05%	0.006%
43	6.635	908	910	913	rBV2	138	120	0.03%	0.003%
44	6.757	921	930	946	rBV	171180	413079	86.68%	10.536%
45	7.123	983	990	999	rVB6	2235	6216	1.30%	0.159%
46	7.202	1000	1003	1004	rBV	141	151	0.03%	0.004%
47	7.306	1012	1020	1044	rVB	100212	222130	46.61%	5.665%
48	7.531	1056	1057	1059	rBV	151	96	0.02%	0.002%
49	7.793	1098	1100	1101	rBV	184	132	0.03%	0.003%
50	7.952	1124	1126	1129	rBV3	223	327	0.07%	0.008%
51	8.177	1161	1163	1168	rVB	137	161	0.03%	0.004%
52	8.324	1182	1187	1202	rBV	51435	89668	18.81%	2.287%
53	8.647	1233	1240	1253	rBV	220637	349158	73.26%	8.905%
54	8.878	1275	1278	1280	rBV2	191	201	0.04%	0.005%
55	8.952	1285	1290	1298	rBV	36798	56323	11.82%	1.437%
56	9.171	1323	1326	1329	rBV	174	226	0.05%	0.006%
57	9.275	1338	1343	1348	rVB2	1592	2127	0.45%	0.054%
58	9.385	1356	1361	1377	rBV	166985	255064	53.52%	6.505%
59	9.702	1409	1413	1417	rVV2	1503	2355	0.49%	0.060%
60	9.738	1417	1419	1421	rVB2	166	103	0.02%	0.003%
61	9.927	1448	1450	1453	rBV2	163	173	0.04%	0.004%
62	10.055	1465	1471	1485	rBV	334047	466839	97.96%	11.907%
63	10.208	1493	1496	1497	rVB3	202	172	0.04%	0.004%
64	10.275	1505	1507	1510	rBV2	162	196	0.04%	0.005%
65	10.317	1512	1514	1518	rVB3	308	354	0.07%	0.009%
66	10.390	1522	1526	1528	rBV2	141	151	0.03%	0.004%
67	10.512	1545	1546	1549	rBV2	187	232	0.05%	0.006%
68	10.750	1583	1585	1587	rBV	122	147	0.03%	0.004%
69	10.903	1608	1610	1611	rBV	138	113	0.02%	0.003%
70	10.963	1617	1620	1623	rBV2	143	200	0.04%	0.005%
71	11.018	1627	1629	1633	rBB2	123	132	0.03%	0.003%
72	11.073	1635	1638	1639	rBV	135	153	0.03%	0.004%
73	11.134	1647	1648	1652	rBV	114	110	0.02%	0.003%
74	11.189	1652	1657	1666	rBV	203437	270399	56.74%	6.897%
75	11.311	1673	1677	1681	rVB3	407	623	0.13%	0.016%
76	11.396	1688	1691	1696	rBV2	105	249	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042544.D
 Acq On : 25 Jul 2024 01:52
 Operator : JC/MD
 Sample : P3344-07 100X
 Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BHB23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.457	1699	1701	1704	rBV2	130	152	0.03%	0.004%
78	11.500	1706	1708	1711	rVB2	121	128	0.03%	0.003%
79	11.530	1711	1713	1716	rVB	148	159	0.03%	0.004%
80	11.561	1716	1718	1720	rBV2	116	124	0.03%	0.003%
81	11.585	1720	1722	1723	rBV	150	110	0.02%	0.003%
82	11.823	1759	1761	1763	rVB	181	152	0.03%	0.004%
83	11.854	1763	1766	1768	rBV	164	229	0.05%	0.006%
84	12.024	1788	1794	1806	rBV	306181	406142	85.22%	10.359%
85	12.317	1837	1842	1859	rBV	253802	329806	69.20%	8.412%
86	12.542	1877	1879	1881	rVB	182	121	0.03%	0.003%
87	12.646	1895	1896	1900	rBV2	165	219	0.05%	0.006%
88	12.762	1911	1915	1921	rVB3	824	1186	0.25%	0.030%
89	12.878	1930	1934	1936	rBV2	158	159	0.03%	0.004%
90	13.073	1964	1966	1967	rBV2	147	102	0.02%	0.003%
91	13.116	1970	1973	1975	rBV2	163	245	0.05%	0.006%
92	13.719	2066	2072	2073	rBV2	193	290	0.06%	0.007%
93	13.731	2073	2074	2076	rBV	118	111	0.02%	0.003%
94	13.975	2113	2114	2117	rBV	165	191	0.04%	0.005%
95	14.018	2119	2121	2125	rVV2	163	221	0.05%	0.006%
96	14.048	2125	2126	2131	rVB2	184	208	0.04%	0.005%
97	14.091	2131	2133	2134	rBV2	166	155	0.03%	0.004%
98	14.128	2135	2139	2144	rVB2	1152	1834	0.38%	0.047%
99	14.414	2185	2186	2189	rBV2	188	147	0.03%	0.004%
100	15.390	2342	2346	2351	rVB2	1844	2713	0.57%	0.069%

Sum of corrected areas: 3920755



Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042544.D
Acq On : 25 Jul 2024 01:52
Operator : JC/MD
Sample : P3344-07 100X
Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BHB23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

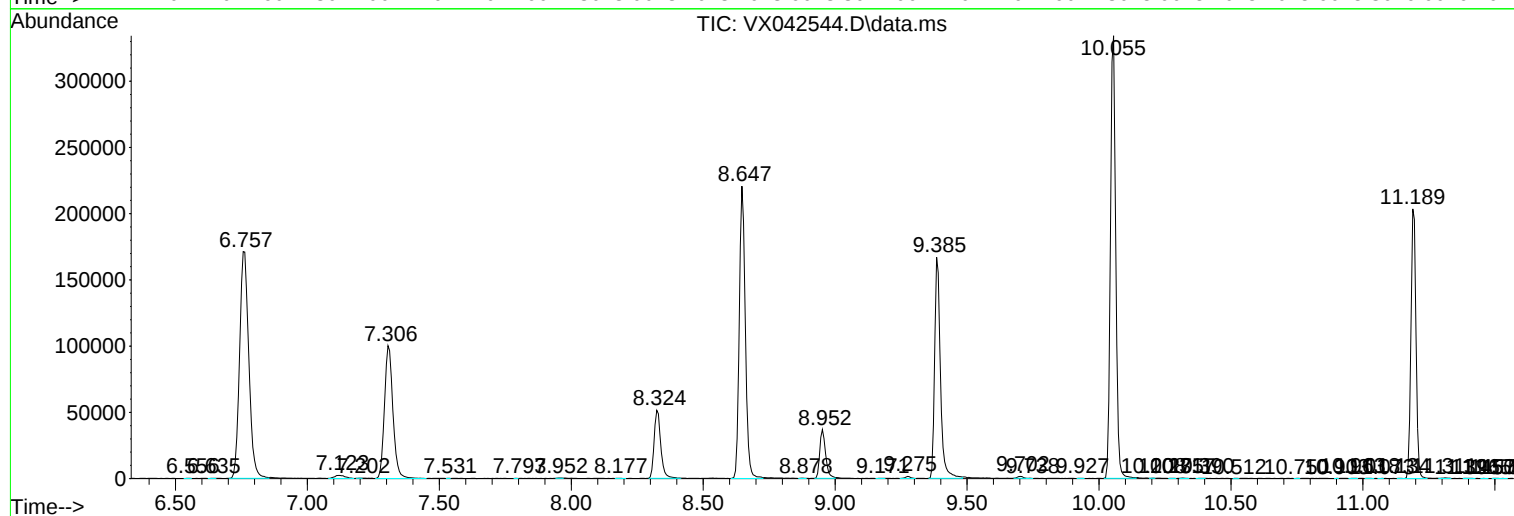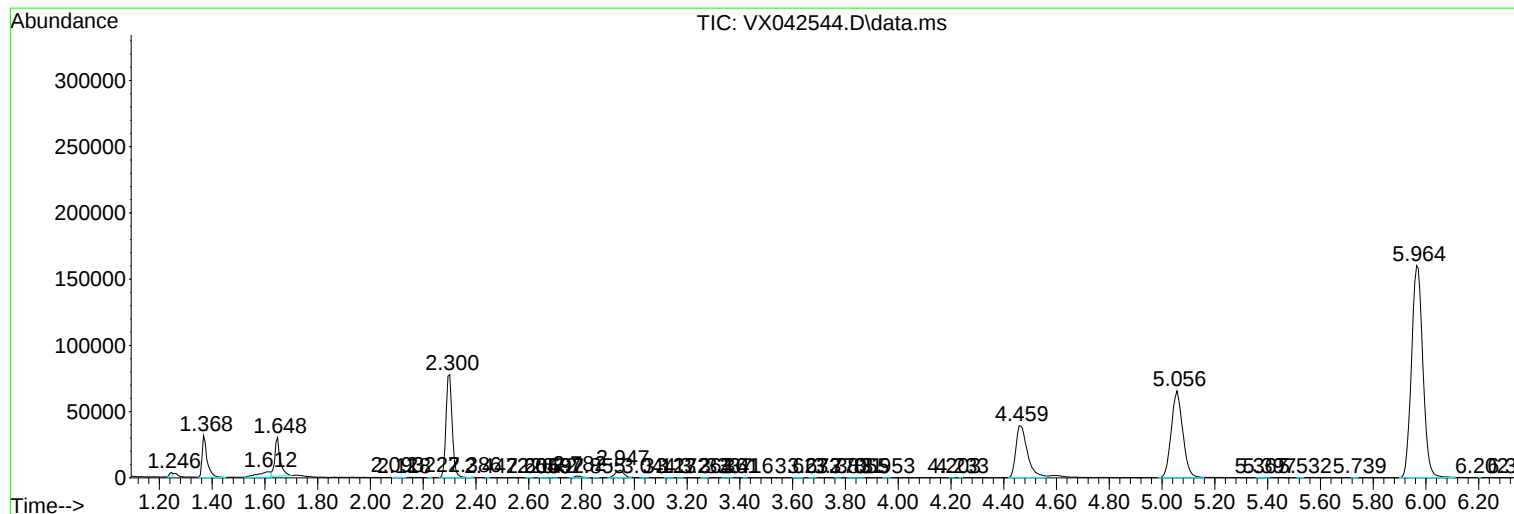

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042544.D
Acq On : 25 Jul 2024 01:52
Operator : JC/MD
Sample : P3344-07 100X
Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BHB23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042544.D
Acq On : 25 Jul 2024 01:52
Operator : JC/MD
Sample : P3344-07 100X
Misc : 4.03g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BHB23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------