

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042551.D
 Acq On : 25 Jul 2024 04:33
 Operator : JC/MD
 Sample : P3327-31 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M

Title : VOC Analysis

Signal : TIC: VX042551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	23	26	27	rBV	3222	3452	0.74%	0.096%
2	1.368	43	46	60	rVV	27228	36891	7.86%	1.025%
3	1.471	62	63	66	rBV2	350	257	0.05%	0.007%
4	1.648	89	92	102	rVB	27106	35334	7.53%	0.982%
5	1.904	132	134	135	rBV	295	245	0.05%	0.007%
6	2.184	177	180	182	rBV	187	228	0.05%	0.006%
7	2.300	192	199	209	rBV	71407	115320	24.57%	3.204%
8	2.440	220	222	226	rBV2	213	232	0.05%	0.006%
9	2.532	235	237	240	rBV	110	124	0.03%	0.003%
10	2.672	254	260	262	rBV	143	246	0.05%	0.007%
11	2.721	262	268	269	rBV2	192	328	0.07%	0.009%
12	2.788	275	279	286	rBV4	1139	2083	0.44%	0.058%
13	2.946	296	305	315	rBV2	8591	20108	4.28%	0.559%
14	3.081	325	327	328	rBV	121	85	0.02%	0.002%
15	3.099	328	330	333	rBV	146	163	0.03%	0.005%
16	3.123	333	334	338	rBV	95	105	0.02%	0.003%
17	3.257	354	356	359	rBV	126	168	0.04%	0.005%
18	3.337	365	369	371	rVV2	154	193	0.04%	0.005%
19	3.361	371	373	376	rVB	126	148	0.03%	0.004%
20	3.392	376	378	383	rBV2	105	162	0.03%	0.005%
21	3.501	394	396	398	rBV2	110	113	0.02%	0.003%
22	3.556	403	405	408	rBV	102	132	0.03%	0.004%
23	3.605	411	413	415	rBV2	116	113	0.02%	0.003%
24	3.727	432	433	436	rVB	144	111	0.02%	0.003%
25	3.788	441	443	446	rBV	138	124	0.03%	0.003%
26	3.879	452	458	463	rBV2	147	299	0.06%	0.008%
27	3.959	468	471	472	rBV	97	83	0.02%	0.002%
28	4.154	501	503	505	rVB	180	130	0.03%	0.004%
29	4.178	505	507	509	rBV2	170	174	0.04%	0.005%
30	4.245	517	518	520	rBV	120	87	0.02%	0.002%
31	4.269	520	522	523	rVV	121	81	0.02%	0.002%
32	4.318	527	530	532	rBV	103	129	0.03%	0.004%
33	4.465	546	554	570	rBV2	32826	100441	21.40%	2.791%
34	4.867	618	620	621	rVB2	162	86	0.02%	0.002%
35	5.056	640	651	668	rBV	54863	170932	36.42%	4.750%
36	5.239	679	681	684	rVB	168	135	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042551.D
 Acq On : 25 Jul 2024 04:33
 Operator : JC/MD
 Sample : P3327-31 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

37	5.269	684	686	688	rBV2	164	146	0.03%	0.004%
38	5.367	700	702	704	rBV	180	185	0.04%	0.005%
39	5.428	711	712	713	rBV	203	105	0.02%	0.003%
40	5.477	719	720	722	rBV	146	121	0.03%	0.003%
41	5.611	741	742	746	rBV2	119	130	0.03%	0.004%
42	5.964	789	800	821	rBV2	143166	416859	88.82%	11.583%
43	6.214	839	841	842	rVB2	185	121	0.03%	0.003%
44	6.495	886	887	890	rBV	176	152	0.03%	0.004%
45	6.757	922	930	952	rBV	172473	418332	89.13%	11.624%
46	7.123	984	990	998	rVB8	2016	4990	1.06%	0.139%
47	7.208	1000	1004	1006	rBV3	218	313	0.07%	0.009%
48	7.305	1012	1020	1041	rVB	87910	194358	41.41%	5.400%
49	7.446	1041	1043	1044	rBV2	124	93	0.02%	0.003%
50	7.653	1075	1077	1079	rBV2	135	143	0.03%	0.004%
51	7.952	1124	1126	1129	rBV2	227	235	0.05%	0.007%
52	8.086	1146	1148	1151	rBV	160	135	0.03%	0.004%
53	8.183	1163	1164	1166	rBV	172	122	0.03%	0.003%
54	8.232	1170	1172	1174	rVV2	104	104	0.02%	0.003%
55	8.324	1182	1187	1205	rBV	43906	76964	16.40%	2.139%
56	8.531	1219	1221	1223	rBV3	208	207	0.04%	0.006%
57	8.647	1234	1240	1251	rBV	196064	311228	66.31%	8.648%
58	8.952	1285	1290	1306	rVB	31232	47816	10.19%	1.329%
59	9.281	1339	1344	1348	rVB3	728	1154	0.25%	0.032%
60	9.390	1356	1362	1380	rBV	135292	215078	45.83%	5.976%
61	9.701	1409	1413	1419	rVB2	1122	1580	0.34%	0.044%
62	9.799	1427	1429	1434	rBV	116	115	0.02%	0.003%
63	9.970	1455	1457	1458	rVB	127	81	0.02%	0.002%
64	10.055	1465	1471	1480	rBV	341096	469330	100.00%	13.041%
65	10.311	1510	1513	1519	rVB3	423	533	0.11%	0.015%
66	10.354	1519	1520	1523	rBV	197	118	0.03%	0.003%
67	10.500	1542	1544	1545	rBV	122	101	0.02%	0.003%
68	10.628	1563	1565	1567	rBV	114	119	0.03%	0.003%
69	10.652	1567	1569	1572	rVB2	173	186	0.04%	0.005%
70	10.787	1589	1591	1593	rBV	147	163	0.03%	0.005%
71	10.841	1599	1600	1602	rBV	119	84	0.02%	0.002%
72	10.908	1609	1611	1612	rBV	164	100	0.02%	0.003%
73	11.110	1641	1644	1645	rBV	131	153	0.03%	0.004%
74	11.189	1652	1657	1667	rBV	178309	233625	49.78%	6.492%
75	11.317	1676	1678	1682	rVB	540	560	0.12%	0.016%
76	11.360	1683	1685	1688	rVV	101	88	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
 Data File : VX042551.D
 Acq On : 25 Jul 2024 04:33
 Operator : JC/MD
 Sample : P3327-31 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E20G2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Title : VOC Analysis

77	11.457	1698	1701	1704	rVB	168	210	0.04%	0.006%
78	11.488	1704	1706	1709	rBV2	84	120	0.03%	0.003%
79	11.683	1737	1738	1742	rVB	220	210	0.04%	0.006%
80	11.732	1742	1746	1749	rBV2	127	246	0.05%	0.007%
81	11.762	1749	1751	1753	rVB2	212	156	0.03%	0.004%
82	11.786	1753	1755	1756	rBV2	132	128	0.03%	0.004%
83	11.884	1767	1771	1773	rBV	101	170	0.04%	0.005%
84	11.902	1773	1774	1776	rVB	194	129	0.03%	0.004%
85	11.933	1778	1779	1782	rVB2	143	132	0.03%	0.004%
86	12.024	1788	1794	1806	rBV	313768	414128	88.24%	11.507%
87	12.317	1837	1842	1852	rBV	224965	290811	61.96%	8.081%
88	12.762	1911	1915	1919	rVB2	847	1114	0.24%	0.031%
89	12.884	1933	1935	1938	rBV2	91	110	0.02%	0.003%
90	13.140	1974	1977	1978	rBV	196	135	0.03%	0.004%
91	13.439	2024	2026	2027	rBV	151	128	0.03%	0.004%
92	13.585	2049	2050	2052	rBV	187	166	0.04%	0.005%
93	14.036	2123	2124	2126	rBV	113	84	0.02%	0.002%
94	14.127	2135	2139	2143	rBV	1184	1634	0.35%	0.045%
95	14.201	2149	2151	2154	rBV2	174	217	0.05%	0.006%
96	14.420	2185	2187	2189	rVB3	222	175	0.04%	0.005%
97	14.487	2194	2198	2202	rBV2	203	357	0.08%	0.010%
98	14.920	2268	2269	2271	rBV	213	182	0.04%	0.005%
99	15.231	2318	2320	2322	rBV2	304	238	0.05%	0.007%
100	15.389	2342	2346	2351	rVB3	2132	2841	0.61%	0.079%




Sum of corrected areas: 3598890

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042551.D
Acq On : 25 Jul 2024 04:33
Operator : JC/MD
Sample : P3327-31 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

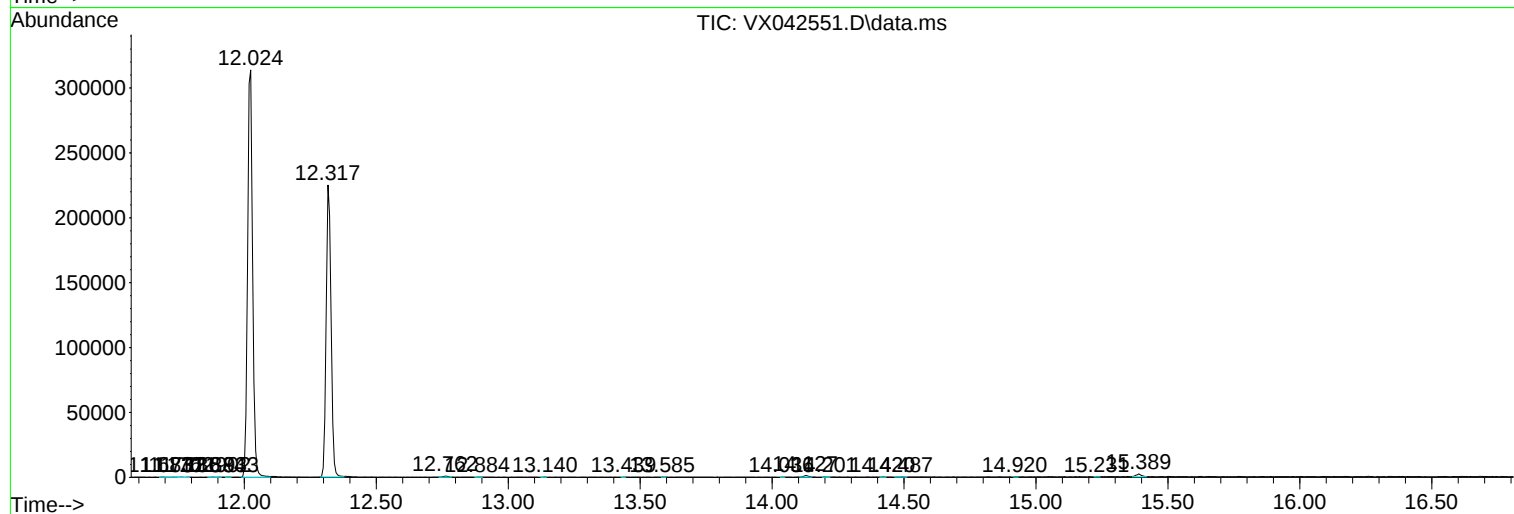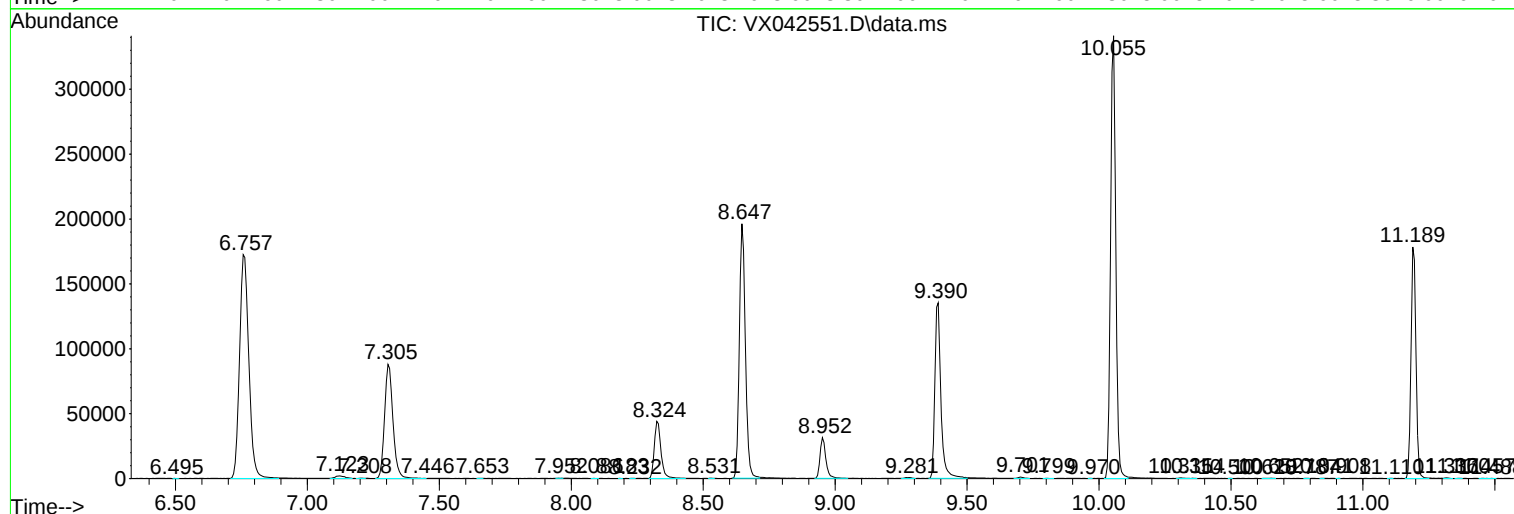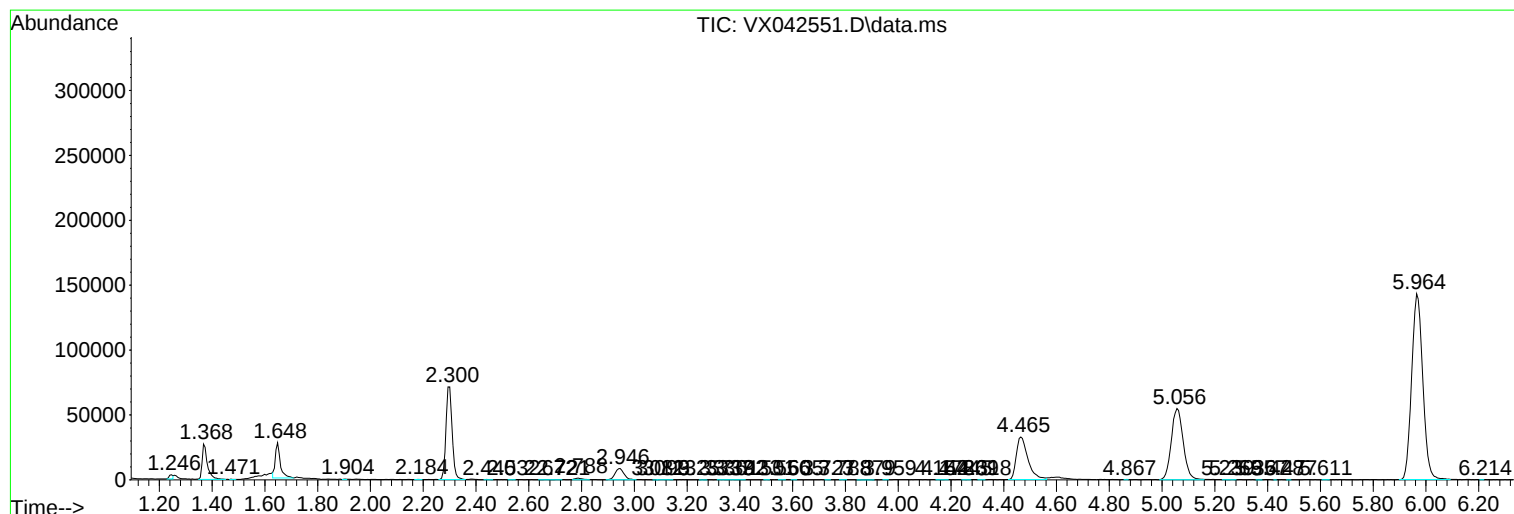

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042551.D
Acq On : 25 Jul 2024 04:33
Operator : JC/MD
Sample : P3327-31 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042551.D
Acq On : 25 Jul 2024 04:33
Operator : JC/MD
Sample : P3327-31 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E20G2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
