
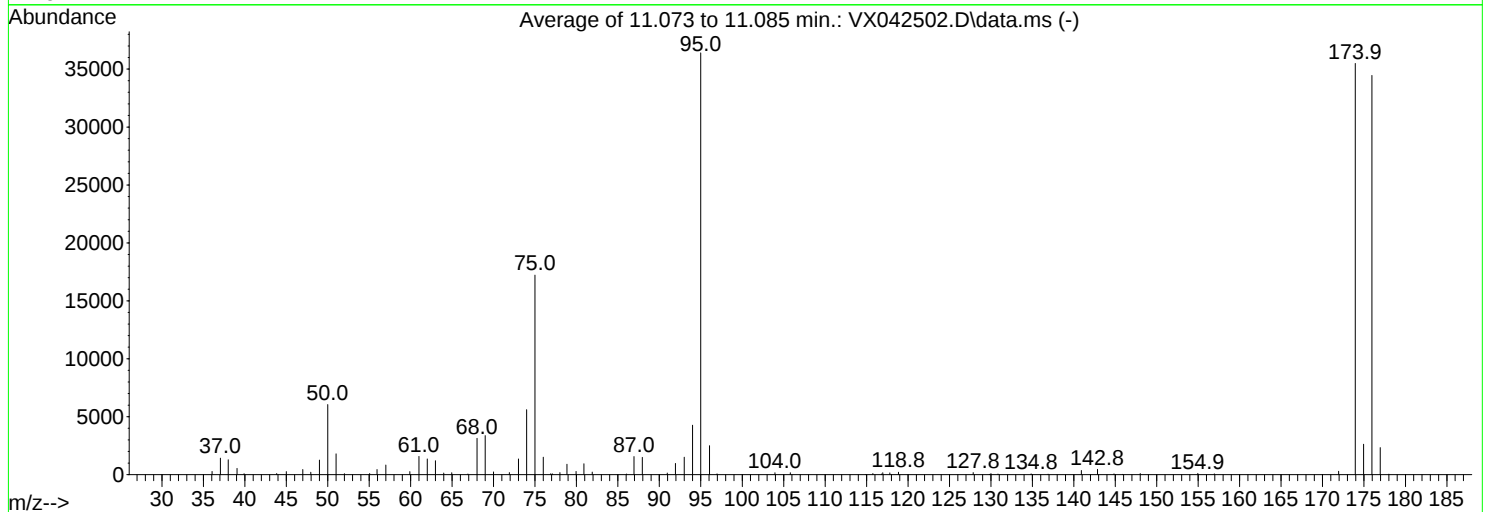


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072524\
Data File : VX042502.D
Acq On : 24 Jul 2024 08:04
Operator : JC/MD
Sample : BFB684
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB684

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM070324WMA.M
Title : VOC Analysis
Last Update : Thu Jul 25 04:44:43 2024

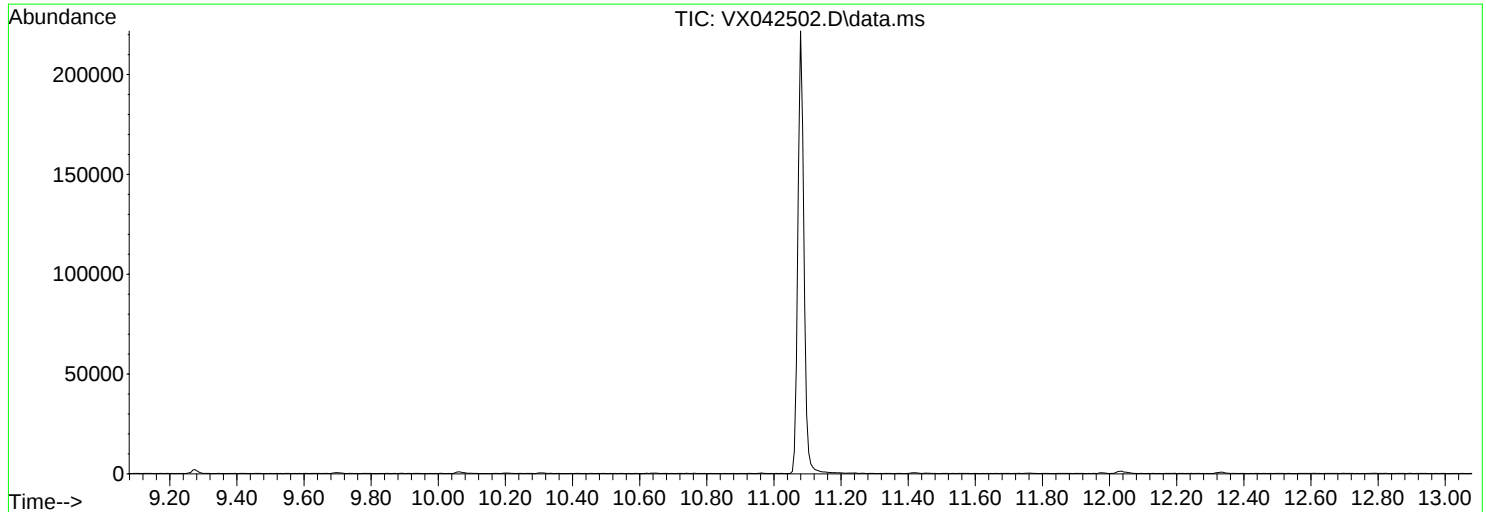

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	6049	PASS
75	95	30	80	47.3	17218	PASS
95	95	100	100	100.0	36405	PASS
96	95	5	9	6.9	2497	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	97.5	35485	PASS
175	174	5	9	7.4	2628	PASS
176	174	95	101	97.1	34456	PASS
177	176	5	9	6.8	2334	PASS

m/z	Abundance
39.90	61.0
43.80	134.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

m/z	Abundance
36.10	290.0
37.10	1484.0
38.00	1152.0
39.00	555.0
40.00	133.0
44.00	214.0
45.00	223.0
47.00	446.0
48.00	200.0
49.00	1281.0
50.00	5574.0
51.00	1708.0
52.00	97.0
55.10	86.0
55.90	434.0
57.00	814.0
59.90	281.0
61.00	1304.0
62.00	1355.0
63.00	1166.0
64.10	89.0
64.90	172.0
66.90	89.0
68.00	2923.0
69.00	2968.0
69.90	217.0
71.90	167.0
73.00	1239.0
74.00	5087.0
75.00	15726.0
76.00	1502.0
76.90	108.0
78.10	187.0
78.90	893.0
79.90	309.0
80.90	817.0
81.80	230.0
87.00	1504.0
88.00	1359.0
91.00	127.0
91.90	908.0
93.00	1446.0
94.00	3665.0
95.00	31456.0
96.10	2522.0
97.00	71.0
104.00	136.0
105.80	120.0
115.70	88.0
116.80	157.0
117.70	107.0
118.80	150.0
127.80	131.0
129.80	77.0
134.90	73.0
136.90	58.0
140.90	282.0
142.80	367.0
144.90	57.0
148.00	62.0
155.00	66.0
171.90	215.0
174.00	26096.0
175.00	1980.0
175.90	25000.0
177.00	1795.0
178.00	57.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

m/z	Abundance
36.10	324.0
37.00	1666.0
38.00	1639.0
39.00	615.0
39.90	181.0
43.90	239.0
45.00	378.0
47.00	578.0
47.90	254.0
49.00	1442.0
50.00	7578.0
51.00	2330.0
52.00	83.0
55.00	155.0
56.00	567.0
57.00	963.0
59.90	327.0
61.00	1888.0
62.00	1460.0
63.00	1443.0
63.90	224.0
65.00	202.0
68.00	3734.0
69.00	4145.0
70.00	269.0
71.80	208.0
73.00	1763.0
74.00	6833.0
75.00	21208.0
76.00	1831.0
77.10	223.0
77.90	184.0
78.90	919.0
80.00	288.0
80.90	1234.0
81.90	253.0
86.00	71.0
86.90	1868.0
87.90	1721.0
90.90	125.0
92.00	1167.0
93.00	1605.0
94.00	5183.0
95.00	44400.0
96.00	2826.0
97.00	66.0
103.90	197.0
105.80	140.0
114.90	52.0
115.70	91.0
117.00	263.0
117.80	228.0
118.90	222.0
127.90	202.0
130.00	125.0
130.90	117.0
134.80	100.0
136.90	57.0
140.90	451.0
142.90	537.0
144.80	67.0
145.90	77.0
148.00	121.0
154.90	119.0
157.00	119.0
171.90	340.0
173.90	43552.0
175.00	3266.0
175.90	41808.0
176.90	2824.0
178.00	87.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684

m/z	Abundance
36.00	226.0
37.00	1128.0
38.00	1056.0
39.10	445.0
39.90	129.0
43.90	243.0
45.00	207.0
47.00	290.0
48.00	168.0
49.00	1053.0
50.00	4996.0
51.00	1358.0
52.00	67.0
55.00	68.0
56.00	345.0
57.00	725.0
60.00	199.0
61.00	1523.0
62.00	1246.0
63.00	998.0
64.10	84.0
64.90	127.0
66.90	73.0
68.00	2749.0
69.00	2985.0
70.10	219.0
72.00	177.0
73.00	1079.0
74.00	4903.0
75.00	14721.0
76.00	1199.0
76.90	163.0
78.00	180.0
78.80	892.0
79.90	240.0
80.90	766.0
82.00	174.0
86.10	100.0
87.00	1313.0
88.00	1381.0
90.90	151.0
92.00	843.0
93.00	1487.0
94.00	3953.0
95.00	33360.0
96.00	2144.0
96.90	57.0
103.90	157.0
105.80	225.0
115.80	129.0
116.90	252.0
117.90	129.0
118.90	238.0
127.70	98.0
128.00	97.0
130.00	179.0
130.80	67.0
134.90	55.0
140.90	351.0
142.90	450.0
144.80	68.0
148.00	94.0
154.90	133.0
156.90	97.0
172.00	327.0
173.90	36808.0
174.90	2638.0
176.00	36560.0
176.90	2383.0

Instrument :
MSVOA_X
ClientSampleId :
BFB684