



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072525\
Data File : VX047127.D
Acq On : 25 Jul 2025 08:40
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Title : SW846 8260
Last Update : Tue Jul 22 03:59:51 2025

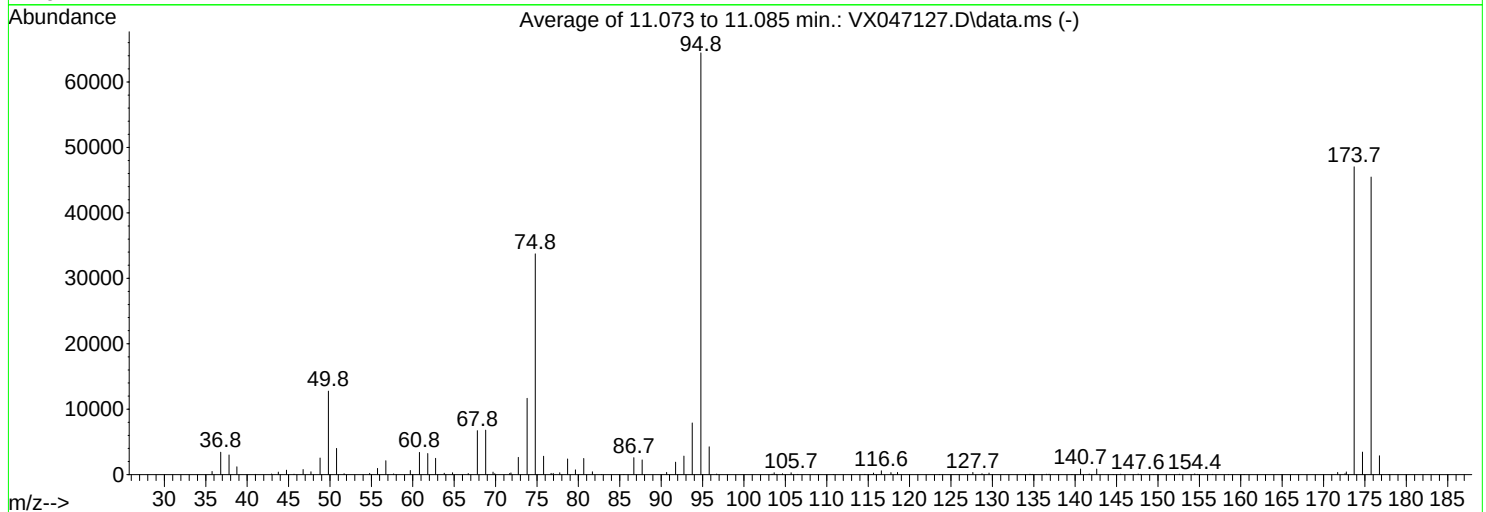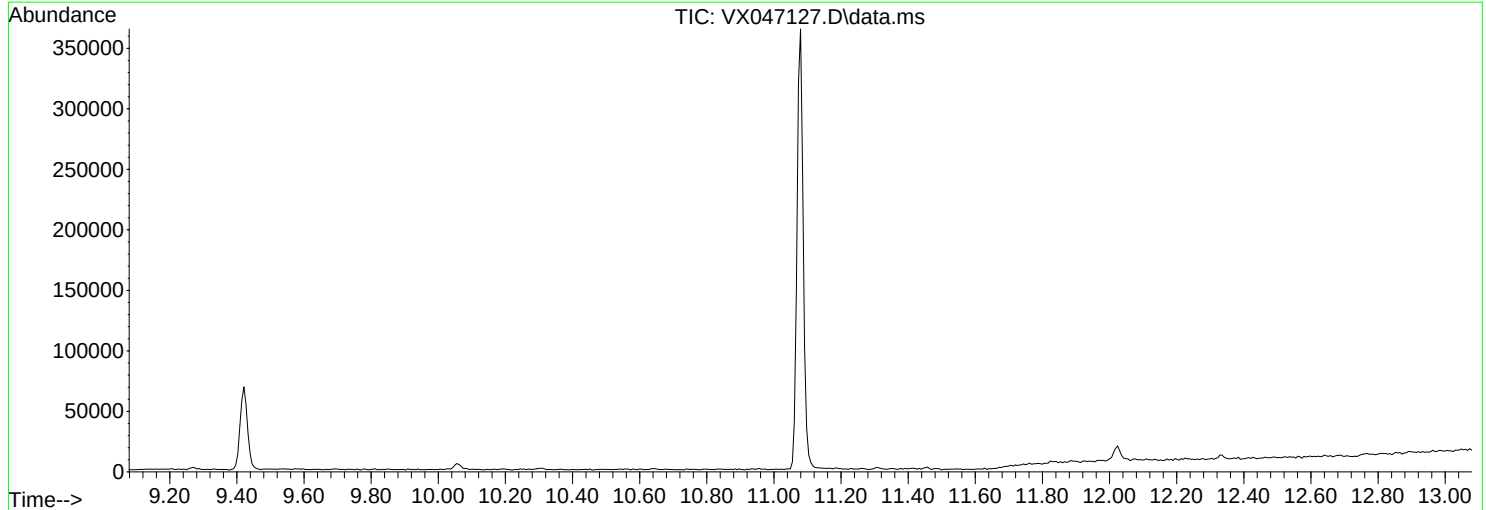

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	12754	PASS
75	95	30	60	52.4	33741	PASS
95	95	100	100	100.0	64451	PASS
96	95	5	9	6.6	4266	PASS
173	174	0.00	2	0.9	424	PASS
174	95	50	100	73.0	47048	PASS
175	174	5	9	7.3	3444	PASS
176	174	95	101	96.7	45485	PASS
177	176	5	9	6.4	2893	PASS