
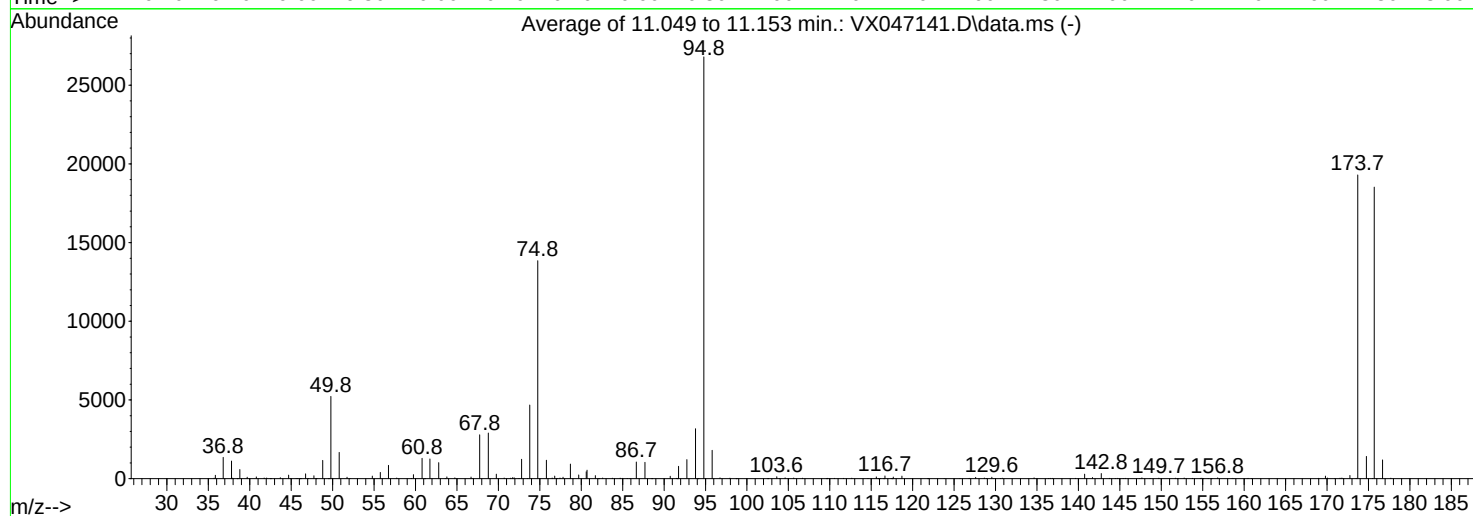


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072525\
Data File : VX047141.D
Acq On : 25 Jul 2025 14:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X072525W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Jul 26 05:39:32 2025

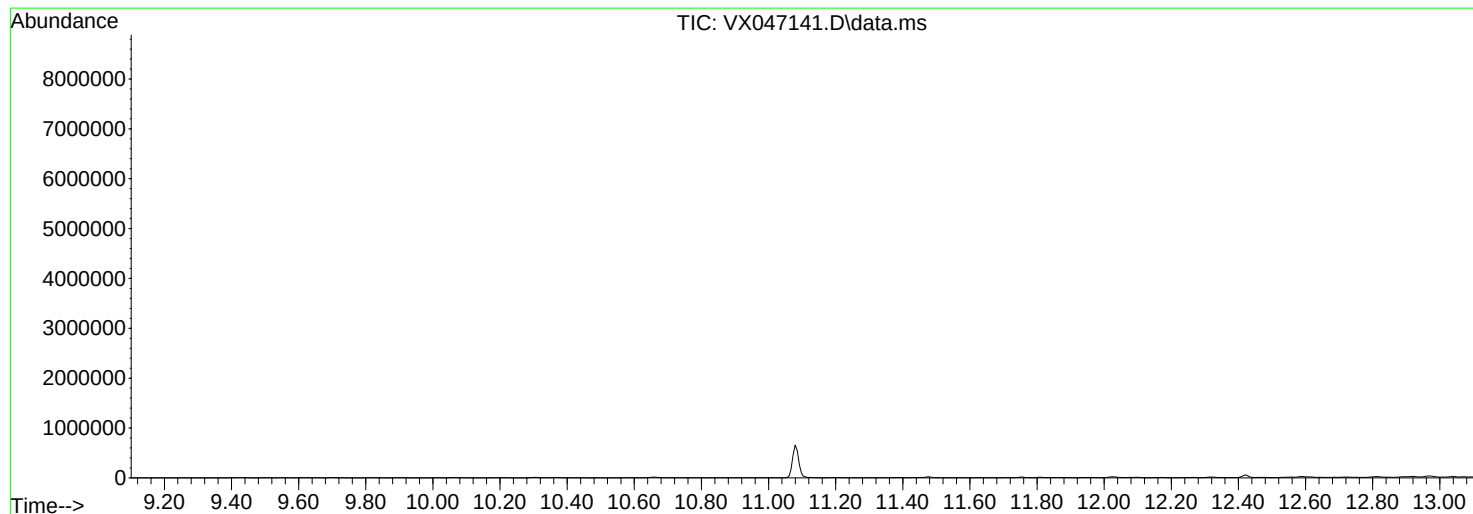

AutoFind: Averaged scan 1634 to 1651; Bkg corrected with scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	5223	PASS
75	95	30	60	51.7	13846	PASS
95	95	100	100	100.0	26800	PASS
96	95	5	9	6.7	1798	PASS
173	174	0.00	2	1.0	201	PASS
174	95	50	100	72.0	19299	PASS
175	174	5	9	7.3	1418	PASS
176	174	95	101	96.0	18527	PASS
177	176	5	9	6.4	1194	PASS