

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072618\
 Data File : VX003692.D
 Acq On : 27 Jul 2018 02:26
 Operator : JC/SP
 Sample : J4154-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-TB-2018-1

Quant Time: Jul 27 17:21:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 27 02:16:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	92914	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.87	114	141942	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.12	117	133622	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	68001	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.07	65	77011	55.95	ug/l	0.00
Spiked Amount	50.000		Recovery	=	111.90%	
35) Dibromofluoromethane	5.51	113	62768	54.09	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.18%	
50) Toluene-d8	8.72	98	229127	51.74	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.48%	
62) 4-Bromofluorobenzene	11.14	95	75737	46.89	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.78%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072618\
Data File : VX003692.D
Acq On : 27 Jul 2018 02:26
Operator : JC/SP
Sample : J4154-10
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-TB-2018-1

Quant Time: Jul 27 17:21:05 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 27 02:16:51 2018
Response via : Initial Calibration

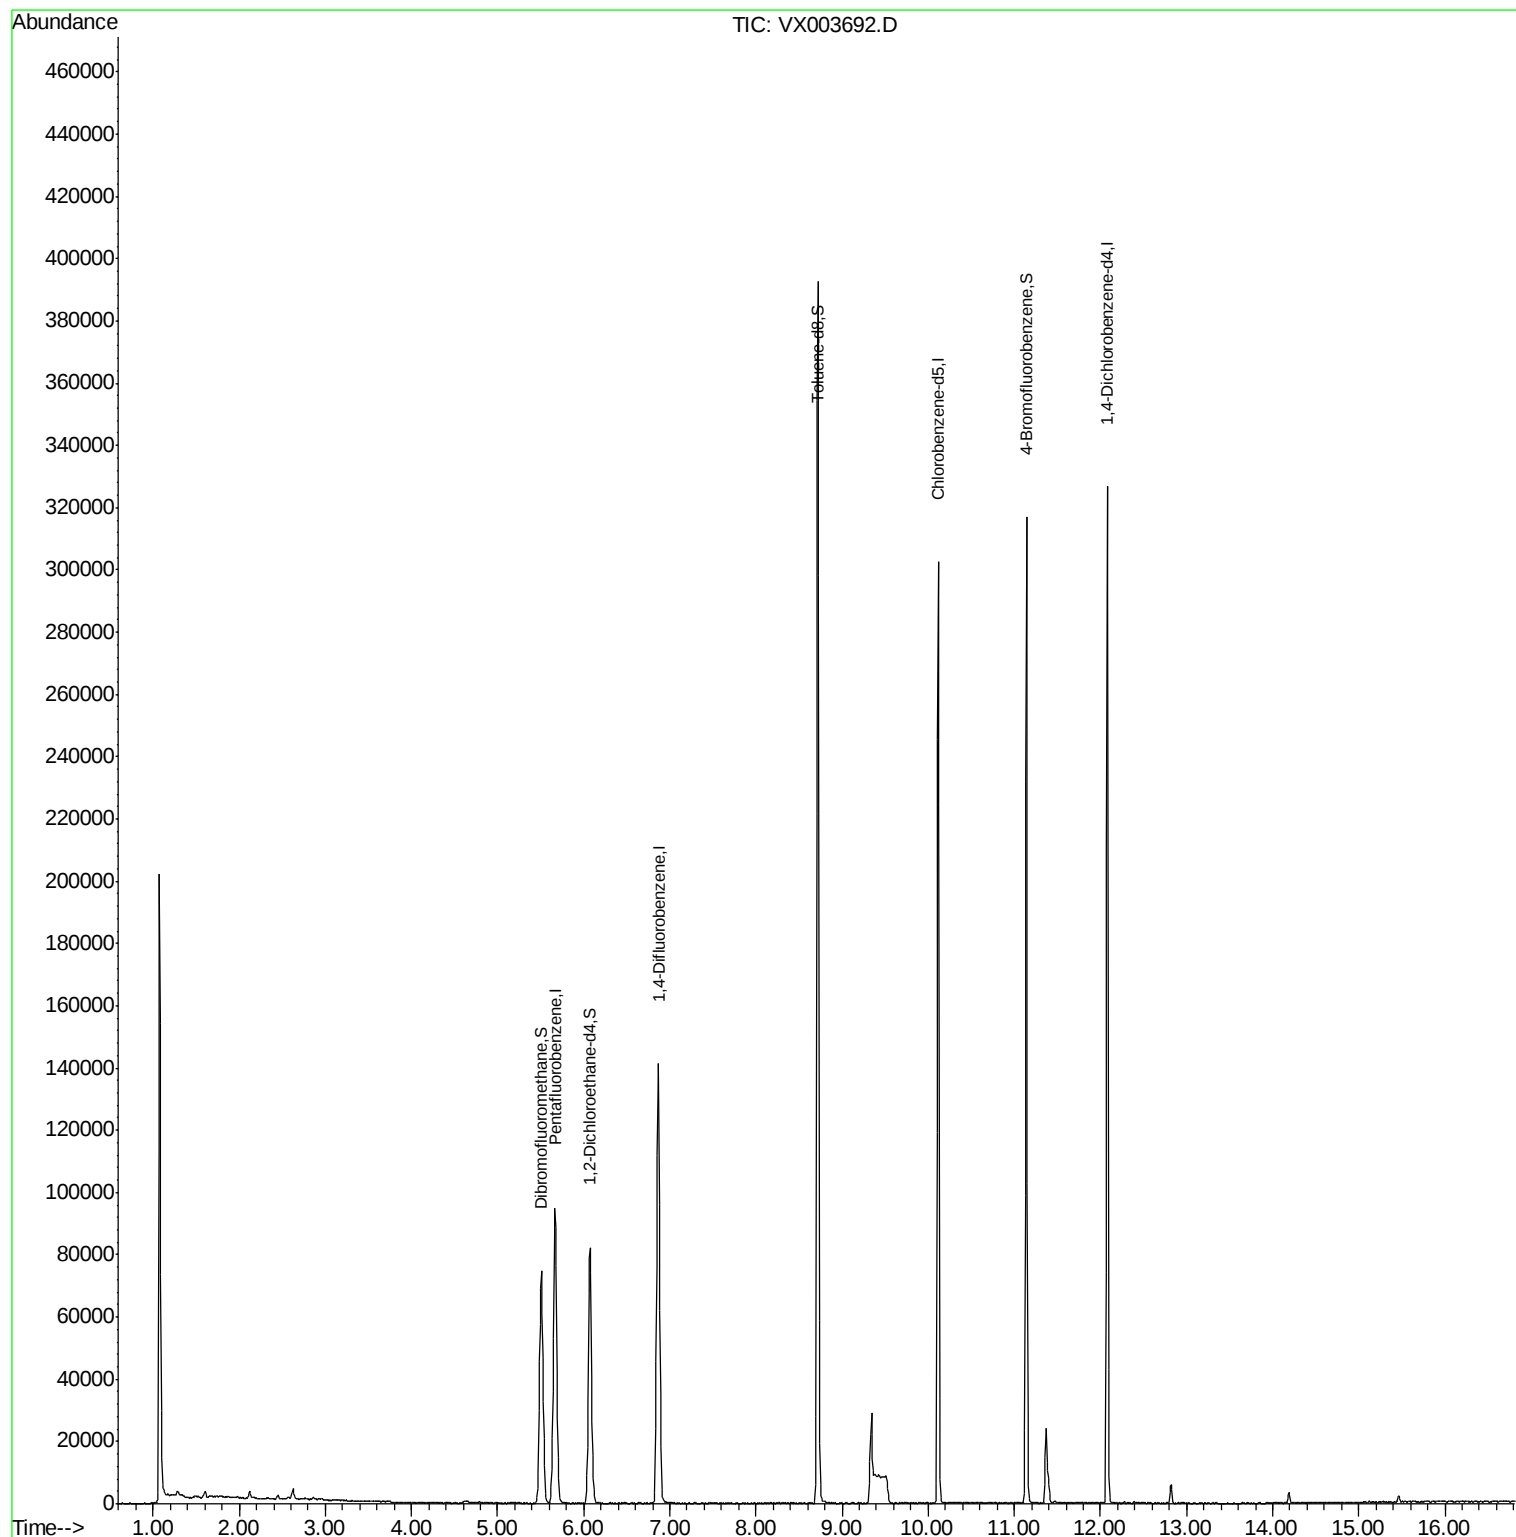



#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 5.67 min Scan# 833

Delta R.T. 0.00 min

Lab File: VX003692.D

Acq: 27 Jul 2018 02:26

Instrument :

MSVOA_X

ClientSampleId :


FL-TB-2018-1

Tot Ion:168 Resp: 92914

Ion Ratio Lower Upper




168 100

99 53.1 49.5 74.3

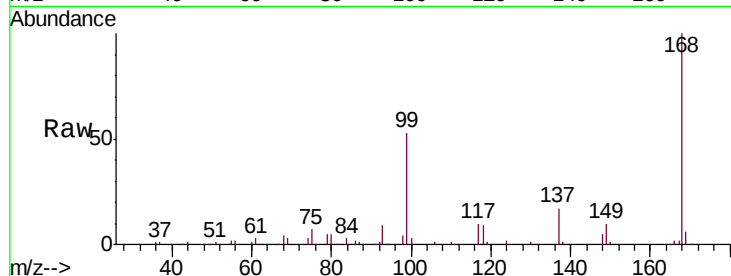

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

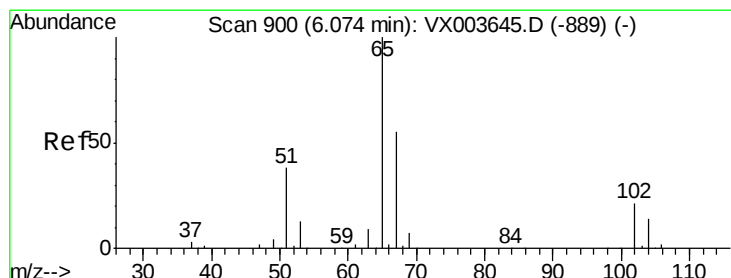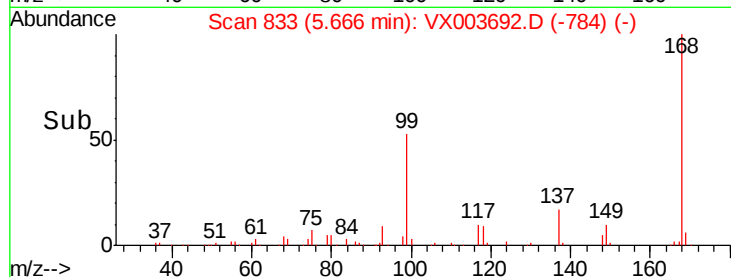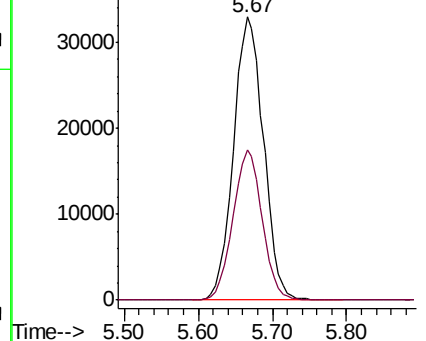

#33

1,2-Dichloroethane-d4

Concen: 55.95 ug/l

RT: 6.07 min Scan# 900

Delta R.T. 0.00 min

Lab File: VX003692.D


Acq: 27 Jul 2018 02:26

Tgt Ion: 65 Resp: 77011

Ion Ratio Lower Upper



65 100


67 53.0 0.0 107.8

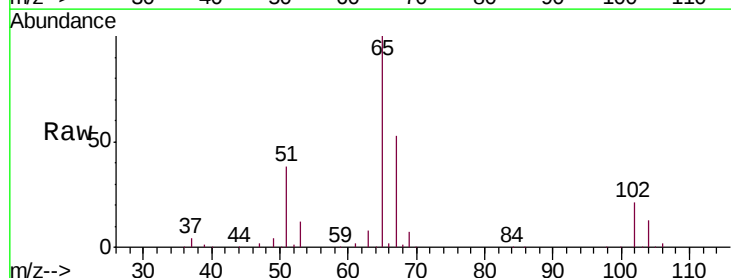

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

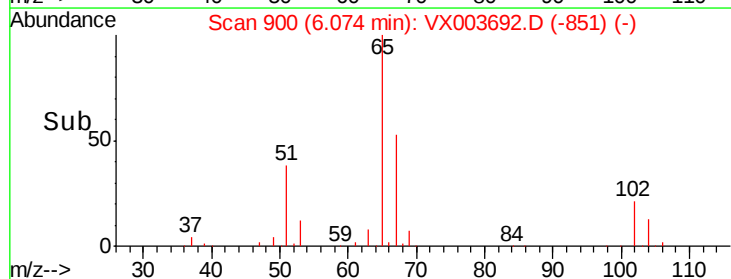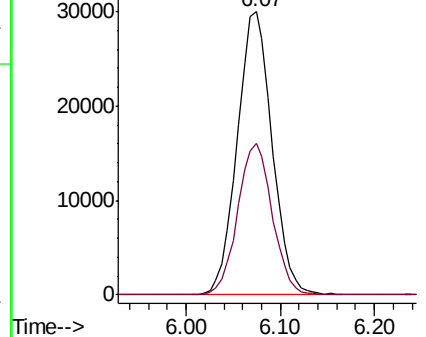


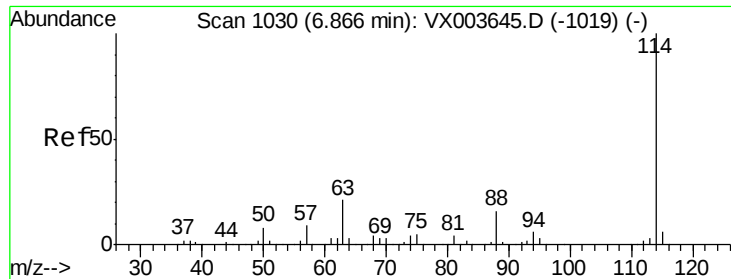




#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.87 min Scan# 1030
Delta R.T. 0.00 min
Lab File: VX003692.D
Acq: 27 Jul 2018 02:26

Instrument :
MSVOA_X
ClientSampleId :
FL-TB-2018-1

Tot Ion:114 Resp: 141942
Ion Ratio Lower Upper
114 100
63 19.9 0.0 41.0
88 15.2 0.0 31.8

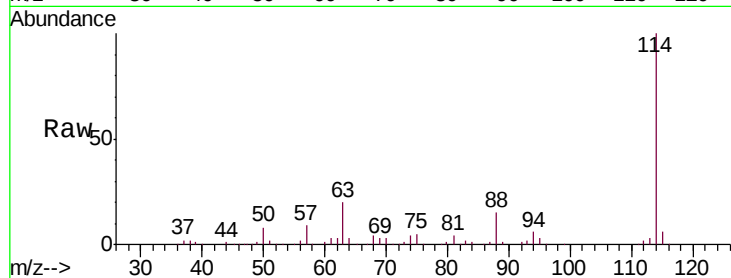


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VX0
Ion 87.90 (87.60 to 88.60): VX0

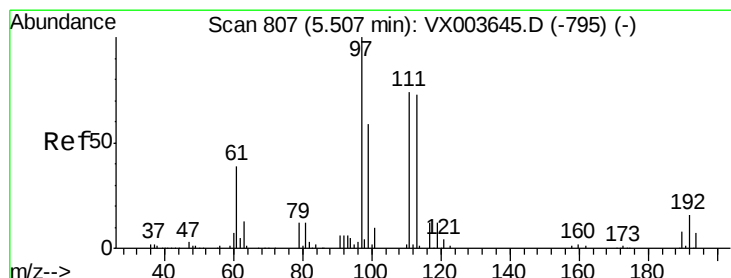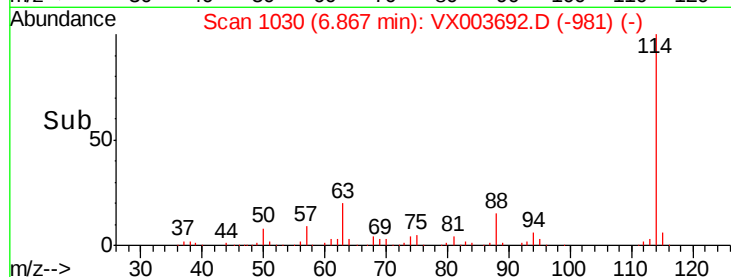
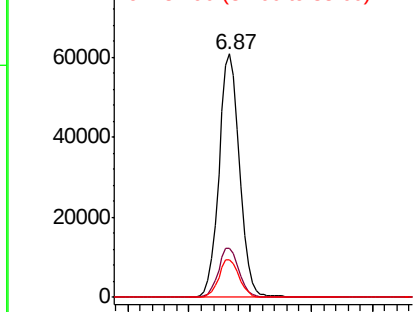



#35
Dibromofluoromethane
Concen: 54.09 ug/l
RT: 5.51 min Scan# 807
Delta R.T. 0.00 min
Lab File: VX003692.D
Acq: 27 Jul 2018 02:26

Tgt Ion:113 Resp: 62768
Ion Ratio Lower Upper
113 100
111 102.1 81.2 121.8
192 22.1 18.2 27.4

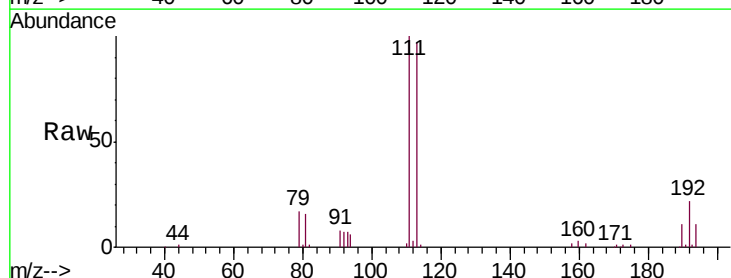

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

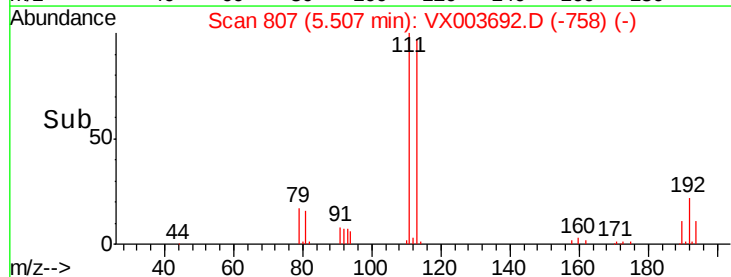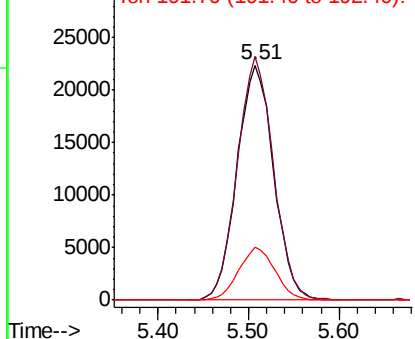

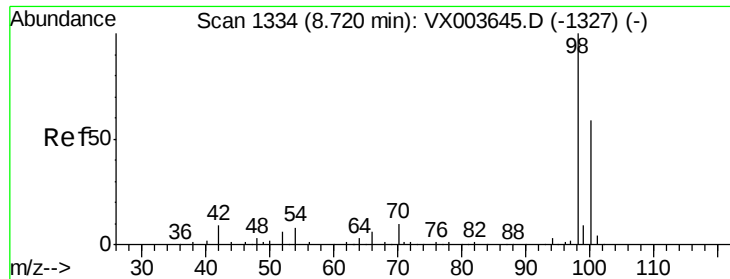

#50

Toluene-d8

Concen: 51.74 ug/l

RT: 8.72 min Scan# 1334

Delta R.T. 0.00 min

Lab File: VX003692.D

Acq: 27 Jul 2018 02:26

Instrument :

MSVOA_X

ClientSampleId :


FL-TB-2018-1

Tot Ion: 98 Resp: 229127

Ion Ratio Lower Upper




98 100

100 63.1 50.9 76.3

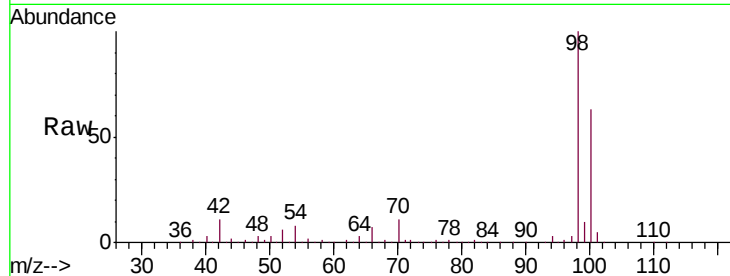

Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V

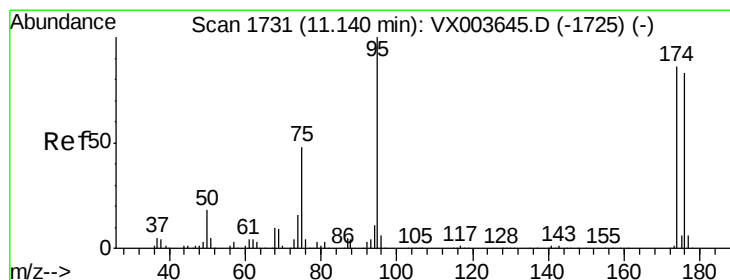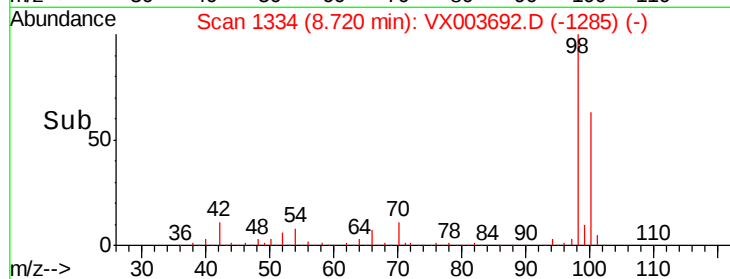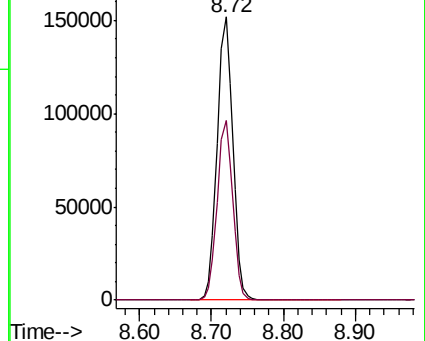

#62

4-Bromofluorobenzene

Concen: 46.89 ug/l

RT: 11.14 min Scan# 1731

Delta R.T. 0.00 min

Lab File: VX003692.D

Acq: 27 Jul 2018 02:26


Tgt Ion: 95 Resp: 75737

Ion Ratio Lower Upper

95 100

174 90.4 0.0 179.0



176 86.4 0.0 173.0

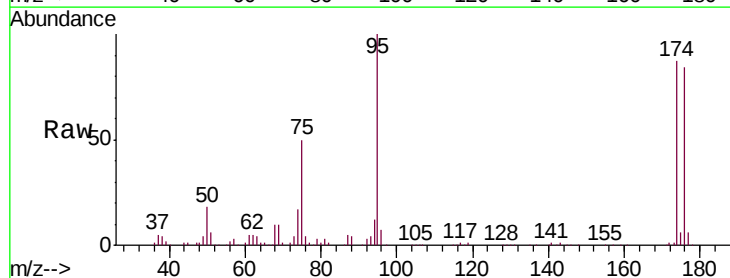


Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

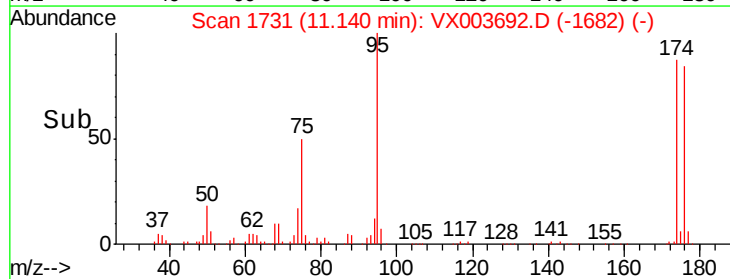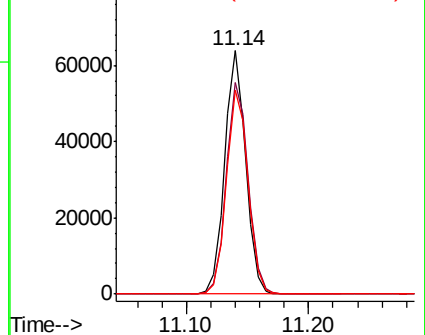


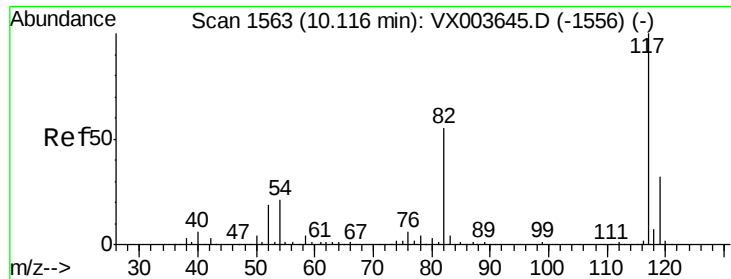




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.12 min Scan# 1563
Delta R.T. 0.00 min
Lab File: VX003692.D
Acq: 27 Jul 2018 02:26

Instrument :
MSVOA_X
ClientSampled :
FL-TB-2018-1

Tot Ion:117 Resp: 133622
Ion Ratio Lower Upper
117 100
82 54.9 44.3 66.5
119 31.4 25.6 38.4

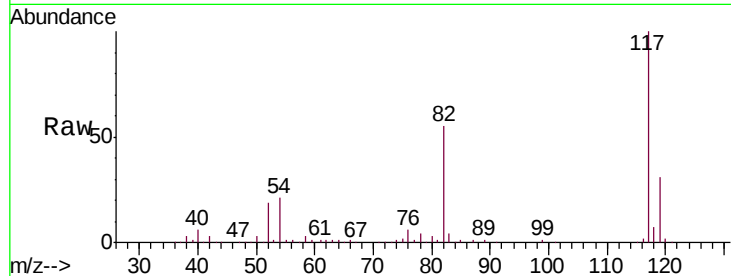


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

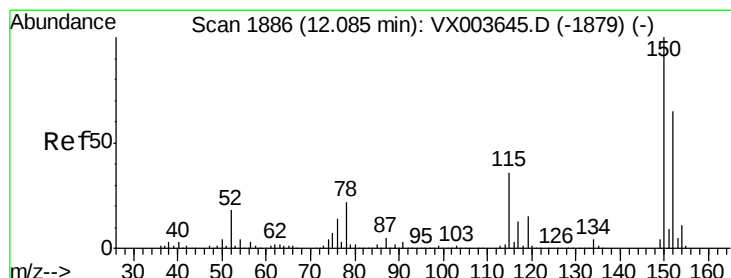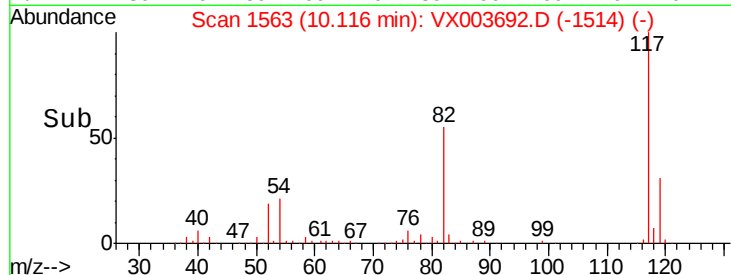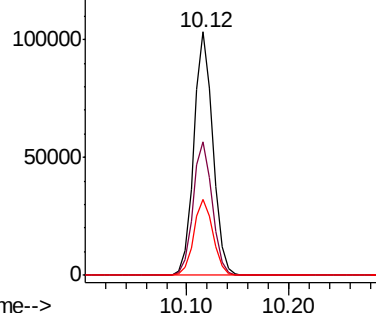

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.08 min Scan# 1885
Delta R.T. -0.01 min
Lab File: VX003692.D
Acq: 27 Jul 2018 02:26

Tgt Ion:152 Resp: 68001
Ion Ratio Lower Upper
152 100
115 57.1 40.0 119.9
150 158.2 0.0 348.4

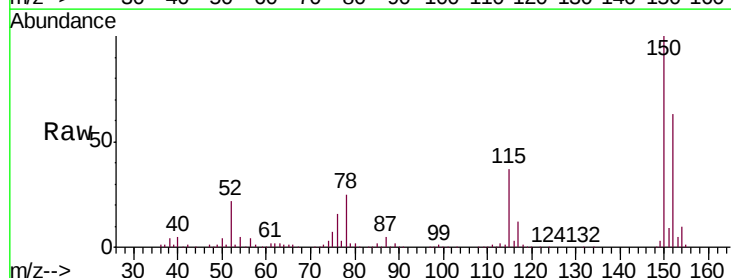

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

