

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072618\
 Data File : VX003708.D
 Acq On : 27 Jul 2018 09:33
 Operator : JC/SP
 Sample : J4114-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 KY030LC058-W-180720

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	67	80	94	rBV	365626	435997	75.76%	13.016%
2	5.507	796	807	822	rBV	63565	182952	31.79%	5.462%
3	5.666	822	833	846	rBV	87703	237629	41.29%	7.094%
4	6.068	889	899	913	rBV	73799	189240	32.88%	5.649%
5	6.867	1018	1030	1044	rBV	140900	326813	56.79%	9.756%
6	8.720	1327	1334	1344	rBV	387459	575510	100.00%	17.181%
7	9.336	1430	1435	1440	rBV	24759	48246	8.38%	1.440%
8	10.116	1557	1563	1574	rBV	290258	396505	68.90%	11.837%
9	11.140	1726	1731	1742	rVB	345724	424261	73.72%	12.666%
10	11.372	1763	1769	1778	rBV	22680	49910	8.67%	1.490%
11	12.079	1880	1885	1894	rBV	390120	472352	82.08%	14.101%
12	12.823	2000	2007	2012	rBV	7006	10290	1.79%	0.307%


Sum of corrected areas: 3349705

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072618\
Data File : VX003708.D
Acq On : 27 Jul 2018 09:33
Operator : JC/SP
Sample : J4114-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY030LC058-W-180720

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

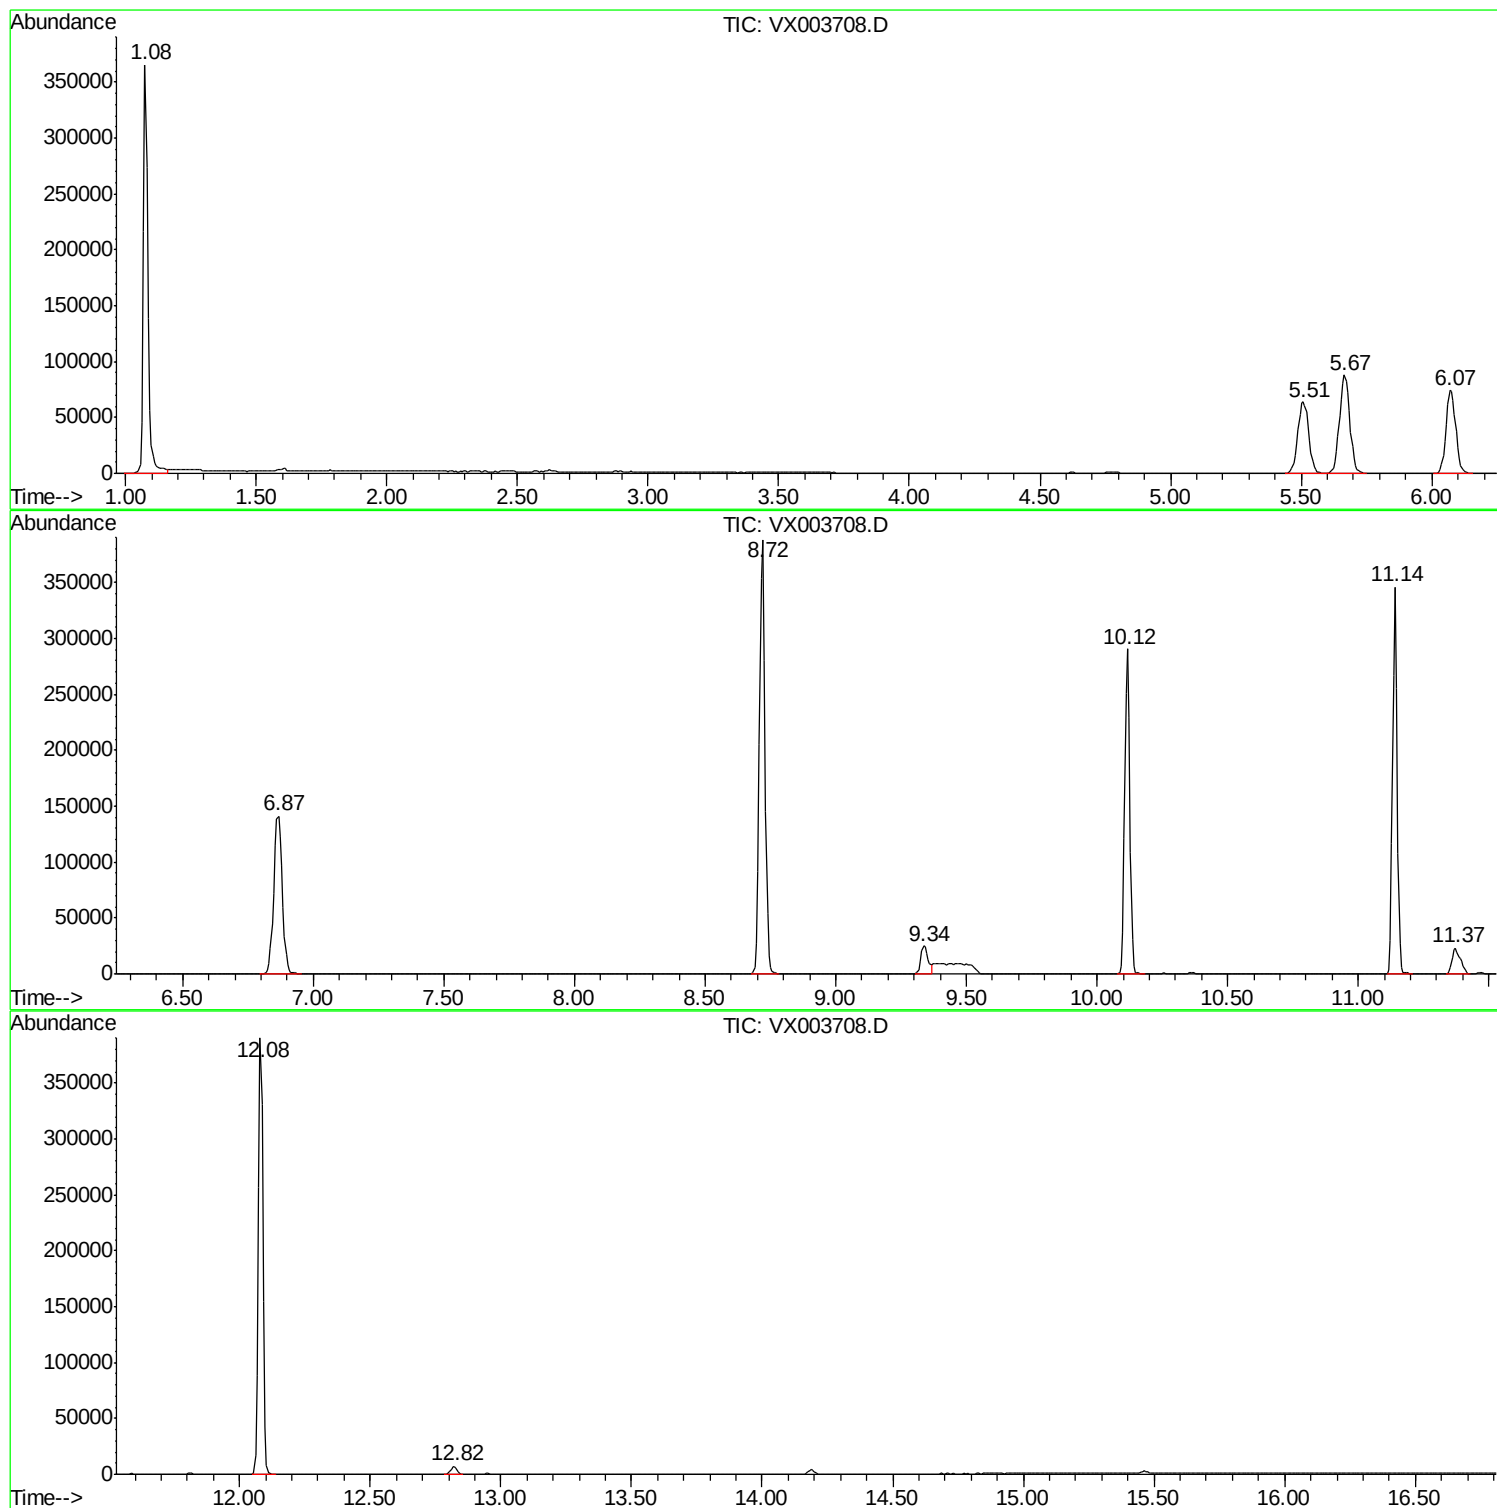

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072618\
Data File : VX003708.D
Acq On : 27 Jul 2018 09:33
Operator : JC/SP
Sample : J4114-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY030LC058-W-180720










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Cyclotrisiloxane, hexamethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.34	6.08 ug/l	48246	Chlorobenzene-d5	10.12

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclotrisiloxane, hexamethyl-	222	C6H18O3Si3	000541-05-9	91
2		Arsenous acid, tris(trimethylsil...	342	C9H27AsO3Si3	055429-29-3	56
3		Benzo[h]quinoline, 2,4-dimethyl-	207	C15H13N	000605-67-4	42
4		5-Methyl-2-phenylindolizine	207	C15H13N	036944-99-7	39
5		Cyclopentene-1-carboxylic acid, ...	332	C23H24O2	1000159-40-6	38

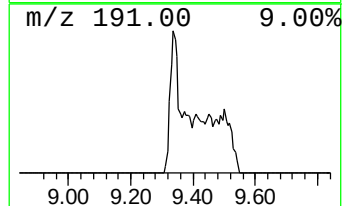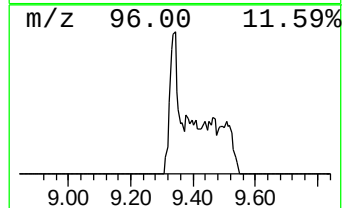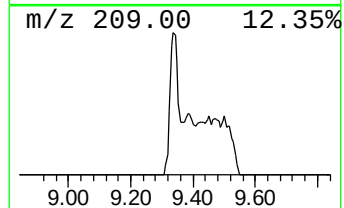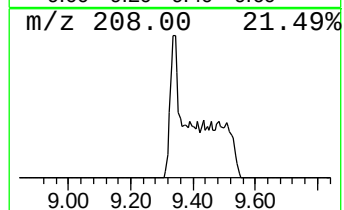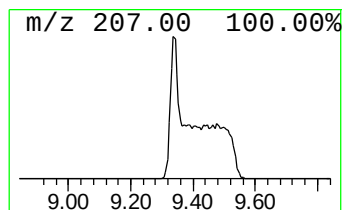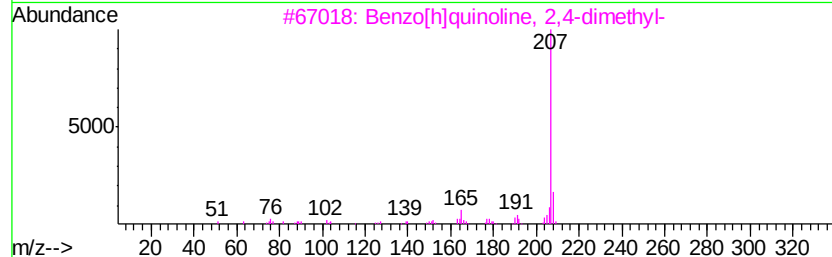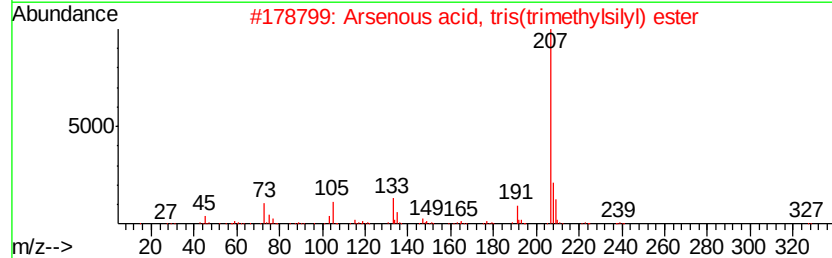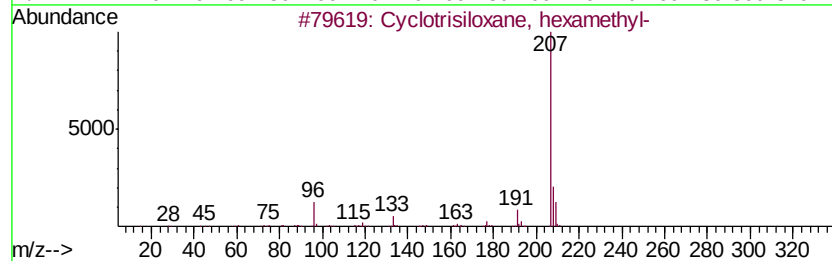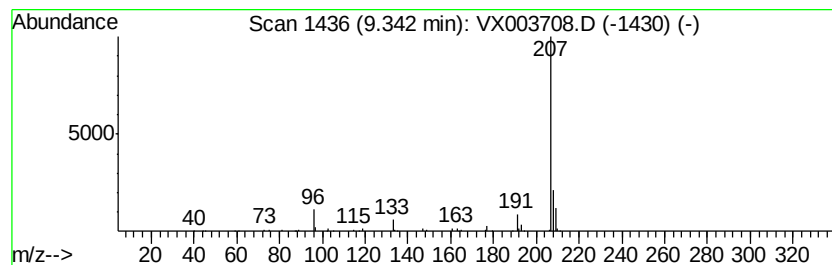

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072618\
Data File : VX003708.D
Acq On : 27 Jul 2018 09:33
Operator : JC/SP
Sample : J4114-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 43 Sample Multiplier: 1










Instrument :
MSVOA_X
ClientSampleId :
KY030LC058-W-180720

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Cyclotetrasiloxane, octamet... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.37	5.28 ug/l	49910	1,4-Dichlorobenzene-d4	12.08
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1		Cyclotetrasiloxane, octamethyl-	296 C8H24O4Si4	000556-67-2 74
2		7H-Dibenzo[b,q]carbazole, 7-methyl-	281 C21H15N	003557-49-1 72
3		Benzoic acid, 3-methyl-2-trimeth...	296 C14H24O3Si2	1000153-57-1 64
4		Cobalt, (.eta.5-2,4-cyclopentadi...	282 C13H10CoF3	055991-82-7 59
5		2',6'-Dihydroxyacetophenone, bis...	296 C14H24O3Si2	1000352-81-3 56

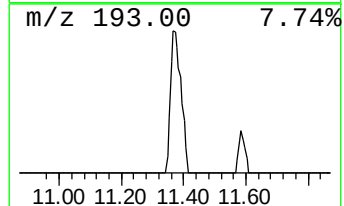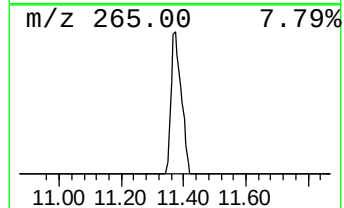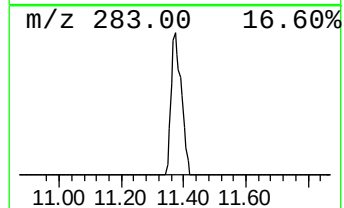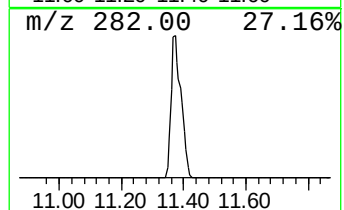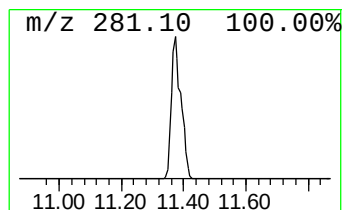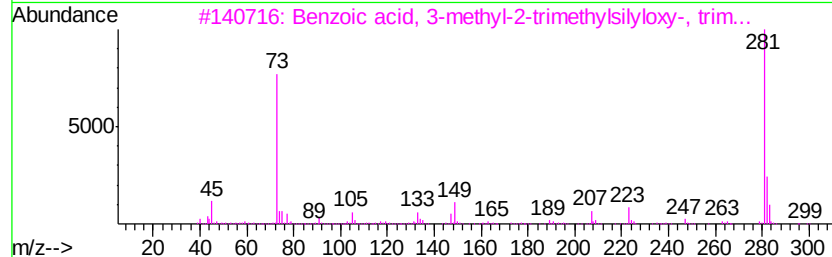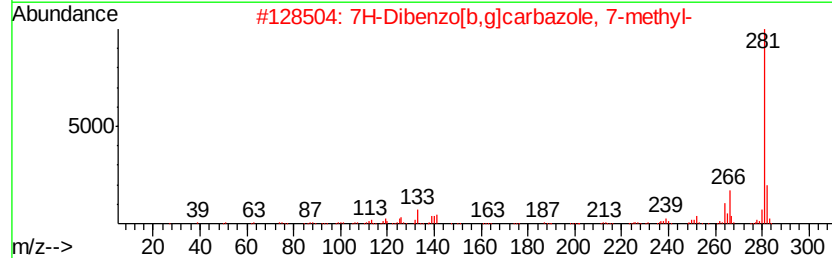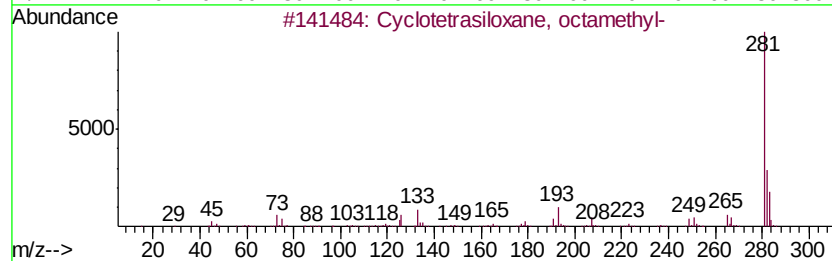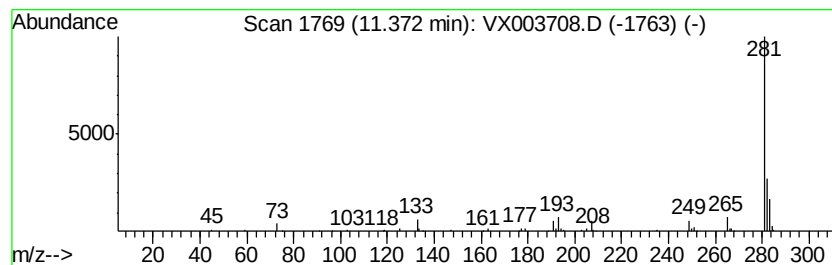

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX072618\
Data File : VX003708.D
Acq On : 27 Jul 2018 09:33
Operator : JC/SP
Sample : J4114-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
KY030LC058-W-180720

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclotrisiloxane,...	9.34	6.1	ug/l	48246	3	10.12	396505	50.0
Cyclotetrasiloxan...	11.37	5.3	ug/l	49910	4	12.08	472352	50.0