

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072618\
 Data File : VX003709.D
 Acq On : 27 Jul 2018 10:00
 Operator : JC/SP
 Sample : J4154-04MS
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0506MS

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.075	68	80	90	rBV	338797	416804	32.07%	1.106%
2	1.197	97	100	108	rVB	97835	94295	7.25%	0.250%
3	1.325	118	121	128	rVB	115944	120933	9.30%	0.321%
4	1.404	131	134	144	rVV	123639	126027	9.70%	0.334%
5	1.489	144	148	157	rVV	95012	113699	8.75%	0.302%
6	1.636	169	172	179	rVB	113823	110471	8.50%	0.293%
7	1.721	181	186	193	rBV	72888	95562	7.35%	0.254%
8	1.928	214	220	239	rVB	153180	247777	19.06%	0.658%
9	2.190	257	263	274	rBV	148464	201250	15.48%	0.534%
10	2.294	275	280	287	rVV	45683	73071	5.62%	0.194%
11	2.373	287	293	301	rVV2	290300	571987	44.01%	1.518%
12	2.453	301	306	311	rVV	164999	276109	21.24%	0.733%
13	2.507	311	315	320	rVV	79457	140279	10.79%	0.372%
14	2.568	320	325	332	rVV	131150	223023	17.16%	0.592%
15	2.629	332	335	342	rVV	9410	16879	1.30%	0.045%
16	2.727	343	351	356	rVV2	167195	300425	23.11%	0.797%
17	2.782	356	360	366	rVV	68108	121683	9.36%	0.323%
18	2.855	366	372	393	rVB	156902	309370	23.80%	0.821%
19	3.081	401	409	415	rBV2	63626	142694	10.98%	0.379%
20	3.160	415	422	426	rVV2	392478	829852	63.84%	2.202%
21	3.209	426	430	447	rVB	202865	451687	34.75%	1.199%
22	3.696	499	510	521	rVB	108755	264047	20.31%	0.701%
23	3.830	521	532	536	rBV	293133	704260	54.18%	1.869%
24	3.879	536	540	555	rVB	193942	464306	35.72%	1.232%
25	4.592	642	657	668	rBV3	144486	434390	33.42%	1.153%
26	4.708	668	676	684	rBV2	146882	396124	30.48%	1.051%
27	4.800	684	691	698	rBV	96233	212373	16.34%	0.564%
28	4.885	698	705	718	rVB3	66976	245033	18.85%	0.650%
29	5.031	718	729	730	rBV3	72573	173326	13.33%	0.460%
30	5.165	743	751	757	rBV	188827	567288	43.64%	1.505%
31	5.501	793	806	812	rBV3	175302	524595	40.36%	1.392%
32	5.574	812	818	826	rVV	145860	448967	34.54%	1.191%
33	5.665	826	833	838	rVV	99976	292940	22.54%	0.777%
34	5.726	838	843	848	rVV	116540	320863	24.69%	0.852%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072618\
 Data File : VX003709.D
 Acq On : 27 Jul 2018 10:00
 Operator : JC/SP
 Sample : J4154-04MS
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FL-0506MS

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
 Title : SW846 8260

35	5.800	848	855	871	rVB3	202536	606815	46.68%	1.610%
36	6.074	888	900	905	rBV2	83060	218828	16.84%	0.581%
37	6.147	905	912	918	rBV	240808	589802	45.38%	1.565%
38	6.275	929	933	943	rVB2	7689	18552	1.43%	0.049%
39	6.470	954	965	983	rBV2	99243	247036	19.01%	0.656%
40	6.860	1021	1029	1044	rBV	153876	356103	27.40%	0.945%
41	7.214	1077	1087	1100	rBV	156722	336150	25.86%	0.892%
42	7.464	1117	1128	1133	rBV	193081	424740	32.68%	1.127%
43	7.519	1133	1137	1151	rVV	159750	304799	23.45%	0.809%
44	7.665	1154	1161	1170	rVV	103472	203219	15.63%	0.539%
45	7.781	1170	1180	1192	rVV2	160927	341390	26.26%	0.906%
46	7.903	1192	1200	1218	rVB2	174498	379315	29.18%	1.007%
47	8.195	1240	1248	1263	rBV	35732	65232	5.02%	0.173%
48	8.439	1281	1288	1296	rBV	156374	239804	18.45%	0.636%
49	8.653	1316	1323	1329	rBV	781143	1199600	92.29%	3.184%
50	8.720	1329	1334	1340	rVV	347387	552294	42.49%	1.466%
51	8.787	1340	1345	1363	rVB	387529	585158	45.02%	1.553%
52	9.043	1379	1387	1401	rBV	163265	236567	18.20%	0.628%
53	9.183	1404	1410	1413	rBV	209571	296301	22.80%	0.786%
54	9.220	1413	1416	1426	rVB	224307	310408	23.88%	0.824%
55	9.335	1428	1435	1439	rBV	305441	484626	37.28%	1.286%
56	9.372	1439	1441	1447	rVB	206506	280375	21.57%	0.744%
57	9.500	1457	1462	1471	rVB	759499	1008680	77.60%	2.677%
58	9.585	1471	1476	1481	rVV	148632	208895	16.07%	0.554%
59	9.646	1481	1486	1488	rVV	158523	204156	15.71%	0.542%
60	9.677	1488	1491	1498	rVB	113798	154979	11.92%	0.411%
61	10.116	1557	1563	1565	rBV	295534	419655	32.29%	1.114%
62	10.140	1565	1567	1575	rVV	378008	443330	34.11%	1.177%
63	10.226	1575	1581	1583	rVV	258637	373246	28.72%	0.991%
64	10.256	1583	1586	1597	rVV	510732	630479	48.51%	1.673%
65	10.360	1597	1603	1615	rVB	962353	1247364	95.96%	3.310%
66	10.707	1653	1660	1677	rBV2	678227	1153170	88.72%	3.060%
67	10.860	1680	1685	1689	rBV	125143	169398	13.03%	0.450%
68	10.902	1689	1692	1705	rVB	226270	253699	19.52%	0.673%
69	11.018	1706	1711	1716	rVV	514439	668022	51.39%	1.773%
70	11.079	1716	1721	1726	rVV	130692	164013	12.62%	0.435%
71	11.140	1726	1731	1737	rVB	303920	373905	28.77%	0.992%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072618\
Data File : VX003709.D
Acq On : 27 Jul 2018 10:00
Operator : JC/SP
Sample : J4154-04MS
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0506MS

Integration Parameters: RTEINT.P

Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Title : SW846 8260

72	11.262	1743	1751	1755	rBV2	395575	745752	57.37%	1.979%
73	11.299	1755	1757	1763	rVV2	249690	425965	32.77%	1.130%
74	11.360	1763	1767	1773	rVV	526678	703958	54.16%	1.868%
75	11.420	1773	1777	1783	rVV	457631	605478	46.58%	1.607%
76	11.512	1786	1792	1802	rVB2	1051338	1299812	100.00%	3.449%
77	11.774	1829	1835	1838	rBV2	723809	1036270	79.72%	2.750%
78	11.811	1838	1841	1846	rVB	638568	745754	57.37%	1.979%
79	11.951	1858	1864	1871	rBV	506231	622740	47.91%	1.653%
80	12.030	1871	1877	1880	rBV	435118	537393	41.34%	1.426%
81	12.067	1880	1883	1887	rBV2	587330	1052433	80.97%	2.793%
82	12.390	1931	1936	1947	rVB	870604	1062744	81.76%	2.820%
83	12.597	1965	1970	1977	rBV	280310	369616	28.44%	0.981%
84	13.006	2024	2037	2047	rVB2	114176	161390	12.42%	0.428%
85	13.164	2058	2063	2070	rBV	15236	19594	1.51%	0.052%
86	13.347	2087	2093	2099	rBV	523124	632511	48.66%	1.679%
87	13.652	2137	2143	2148	rBV	368601	469676	36.13%	1.246%
88	13.786	2159	2165	2169	rBV	253908	314048	24.16%	0.833%
89	13.835	2169	2173	2183	rVB	502054	614498	47.28%	1.631%
90	14.024	2198	2204	2209	rBV	390090	479469	36.89%	1.272%


Sum of corrected areas: 37681595

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072618\
Data File : VX003709.D
Acq On : 27 Jul 2018 10:00
Operator : JC/SP
Sample : J4154-04MS
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0506MS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

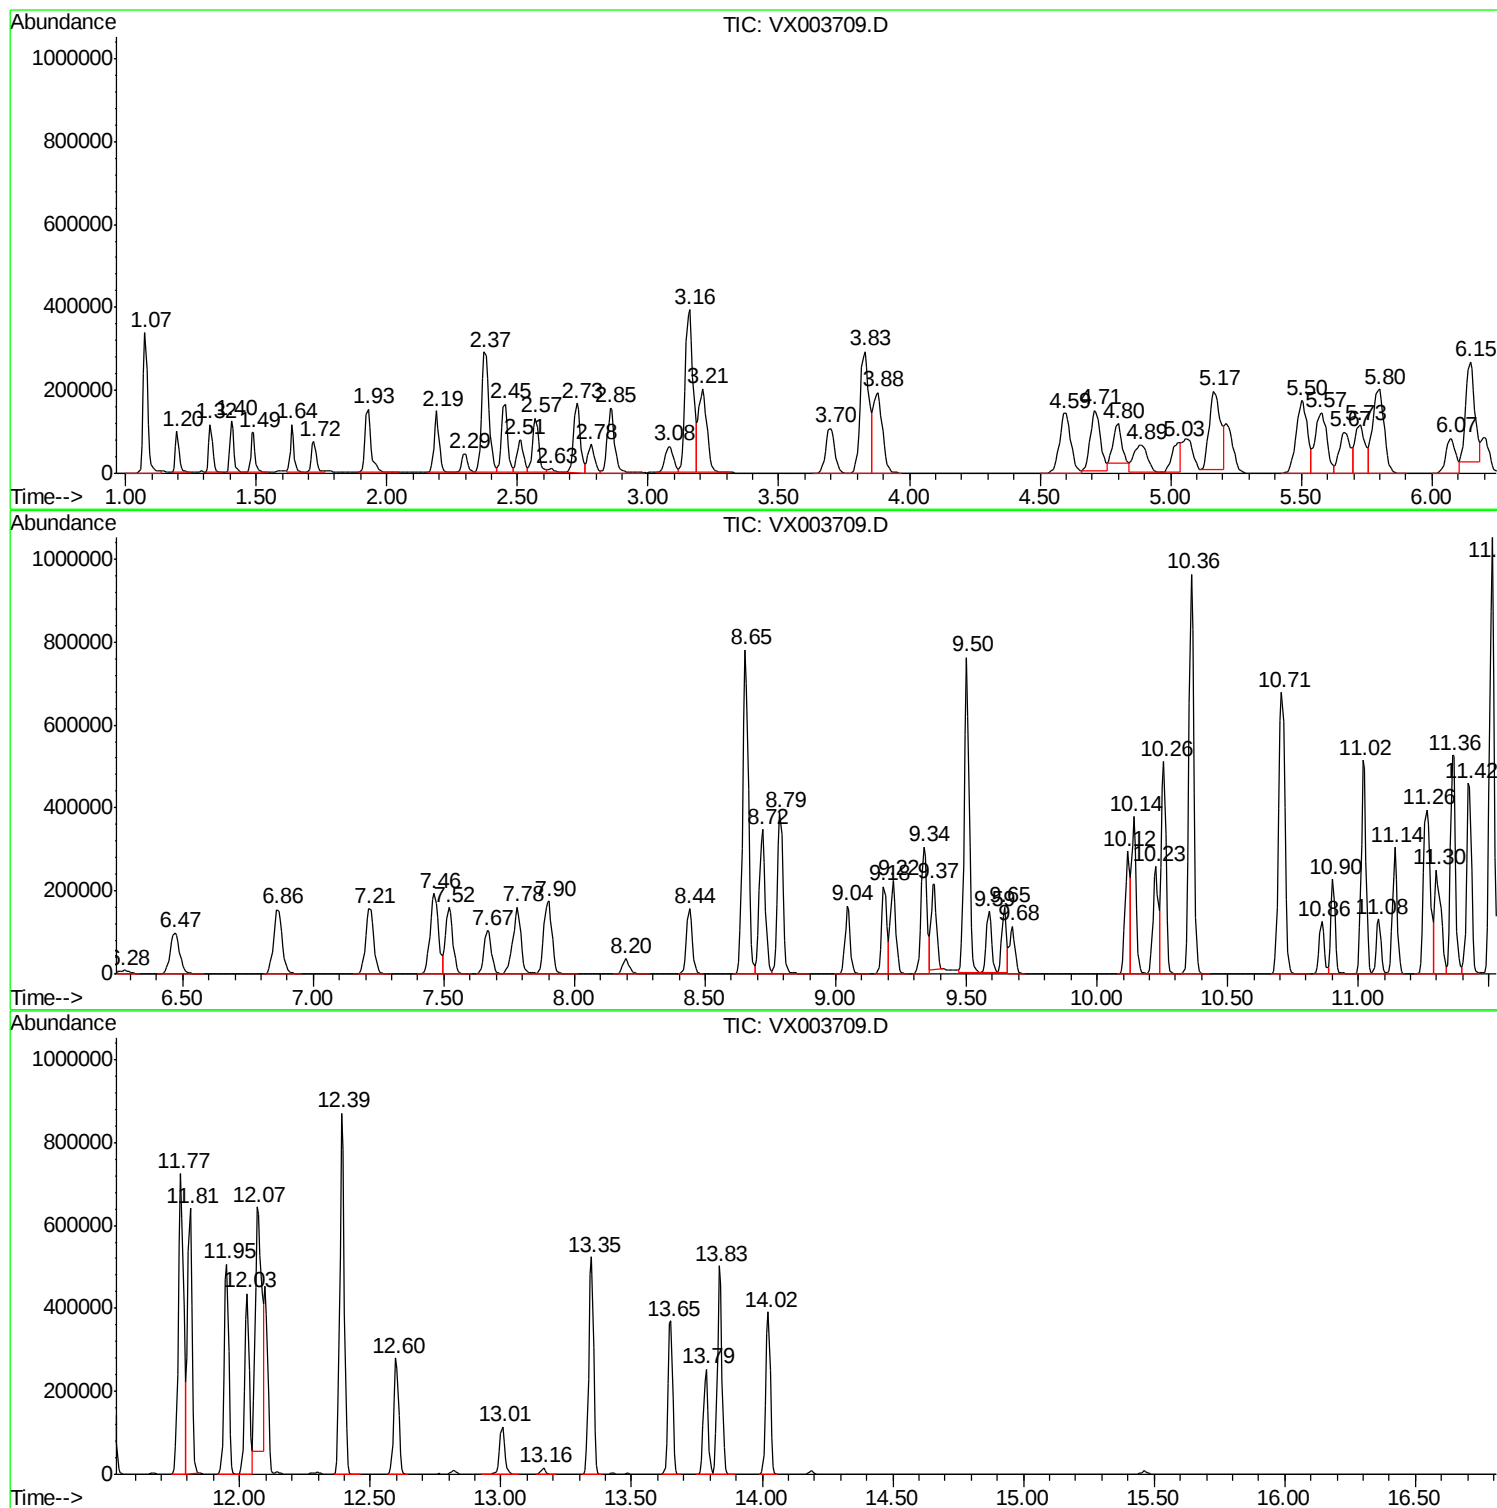

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX072618\
Data File : VX003709.D
Acq On : 27 Jul 2018 10:00
Operator : JC/SP
Sample : J4154-04MS
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0506MS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX072618\
Data File : VX003709.D
Acq On : 27 Jul 2018 10:00
Operator : JC/SP
Sample : J4154-04MS
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FL-0506MS

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc