


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX072618\
Data File : VX003669.D
Acq On : 26 Jul 2018 10:12
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072418W.M
Title : SW846 8260
Last Update : Fri Jul 27 02:16:51 2018

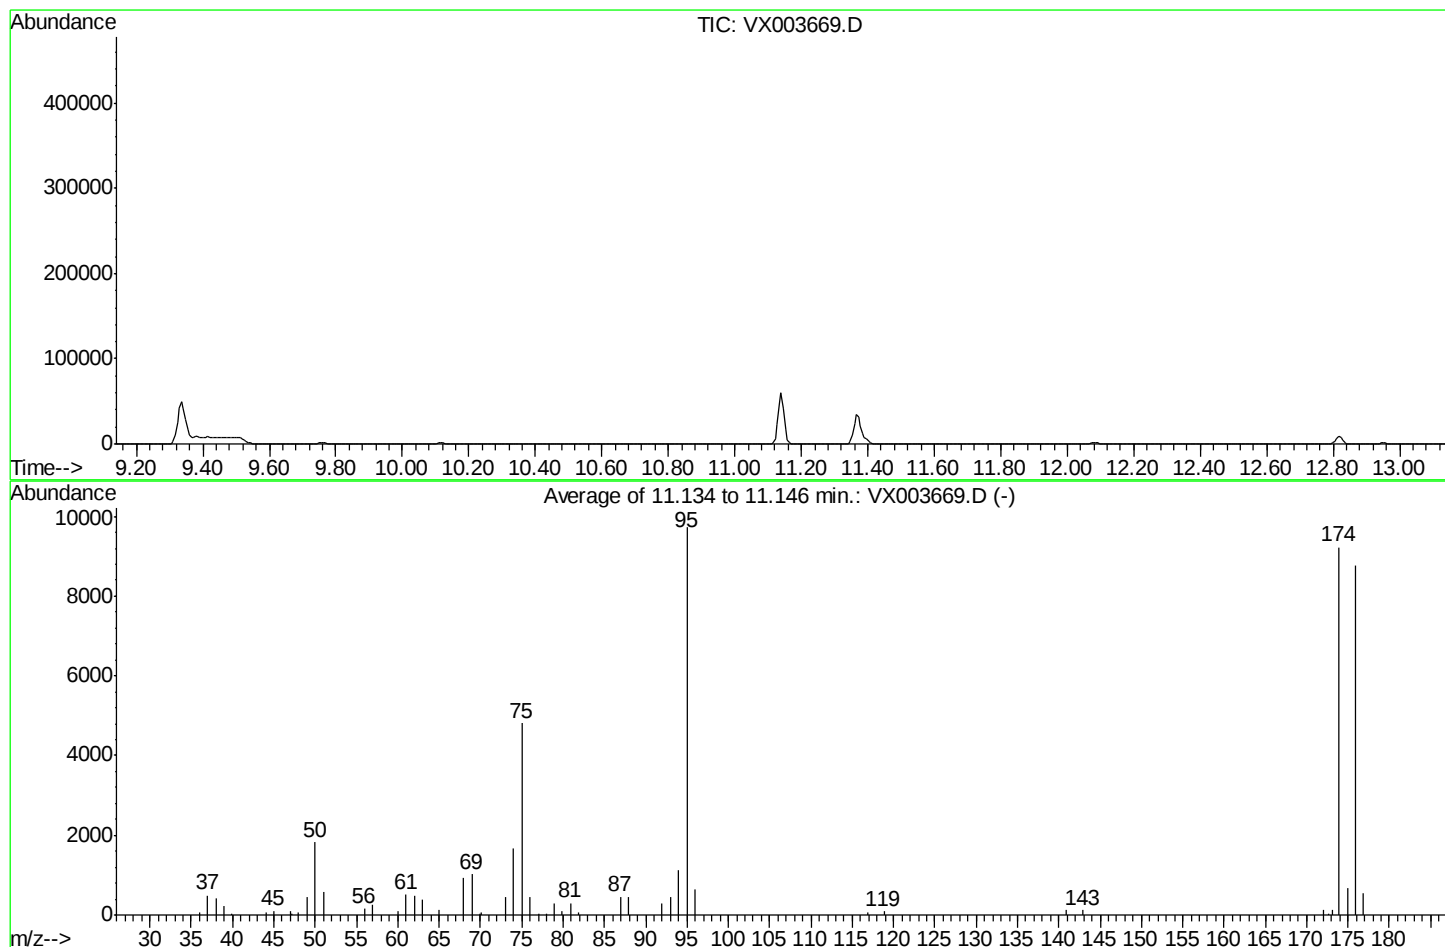

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1724

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	1824	PASS
75	95	30	60	49.4	4805	PASS
95	95	100	100	100.0	9727	PASS
96	95	5	9	6.6	638	PASS
173	174	0.00	2	1.2	115	PASS
174	95	50	100	94.9	9231	PASS
175	174	5	9	7.4	679	PASS
176	174	95	101	95.2	8784	PASS
177	176	5	9	6.3	550	PASS