

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
 Data File : VX023440.D
 Acq On : 26 Jul 2021 10:46
 Operator : JC/MD
 Sample : VX0726MBL01
 Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 27 03:25:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 06:05:38 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	203035	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	346586	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	299668	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	118584	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	131294	51.84	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 103.68%			
35) Dibromofluoromethane	5.397	113	108093	49.88	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.76%			
50) Toluene-d8	8.653	98	407293	51.16	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 102.32%			
62) 4-Bromofluorobenzene	11.085	95	130401	48.17	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 96.34%			
Target Compounds						Qvalue
3) Chloromethane	1.300	50	703	0.32	ug/l #	84
6) Chloroethane	1.697	64	309	0.23	ug/l	100
10) Methyl Iodide	2.459	142	1305	0.52	ug/l #	97
11) Tert butyl alcohol	2.965	59	218	0.38	ug/l	99
13) Acrolein	2.245	56	341	2.52	ug/l #	35
15) Acrylonitrile	3.074	53	424	0.32	ug/l #	85
16) Acetone	2.386	43	1444	1.16	ug/l	94
17) Carbon Disulfide	2.507	76	2046	0.42	ug/l	97
18) Methyl Acetate	2.709	43	649	0.22	ug/l #	54
20) Methylene Chloride	2.806	84	1280	0.53	ug/l #	54
21) trans-1,2-Dichloroethene	3.093	96	432	0.20	ug/l #	80
29) Tetrahydrofuran	5.031	42	366	0.29	ug/l #	60
31) Cyclohexane	5.556	56	4537	1.21	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	15935	5.08	ug/l #	46
38) Carbon Tetrachloride	5.562	117	20856	6.54	ug/l #	16
49) 1,4-Dioxane	7.677	88	95	1.57	ug/l #	28
53) t-1,3-Dichloropropene	8.988	75	308	1.89	ug/l #	70
60) Dibromochloromethane	9.281	129	242	2.07	ug/l #	11
76) 1,2,3-Trichloropropane	11.085	75	67322	25.80	ug/l #	39
81) trans-1,4-Dichloro-2-b...	11.085	75	67322	69.37	ug/l #	12
82) 4-Chlorotoluene	11.457	91	1437	0.21	ug/l	97
86) p-Isopropyltoluene	12.012	119	1694	0.23	ug/l #	69
87) 1,3-Dichlorobenzene	11.969	146	1218	0.31	ug/l	96
88) 1,4-Dichlorobenzene	11.969	146	1218	0.30	ug/l	97
89) n-Butylbenzene	12.335	91	1928	0.28	ug/l	95
90) Hexachloroethane	12.548	117	90	1.96	ug/l #	54
91) 1,2-Dichlorobenzene	12.335	146	860	0.22	ug/l	88
93) 1,2,4-Trichlorobenzene	13.591	180	1114	0.46	ug/l	91
94) Hexachlorobutadiene	13.731	225	453	0.42	ug/l	90
95) Naphthalene	13.780	128	1890	0.23	ug/l #	93
96) 1,2,3-Trichlorobenzene	13.963	180	931	0.38	ug/l	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023440.D
Acq On : 26 Jul 2021 10:46
Operator : JC/MD
Sample : VX0726MBL01
Misc : 5.0g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 27 03:25:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 06:05:38 2021
Response via : Initial Calibration




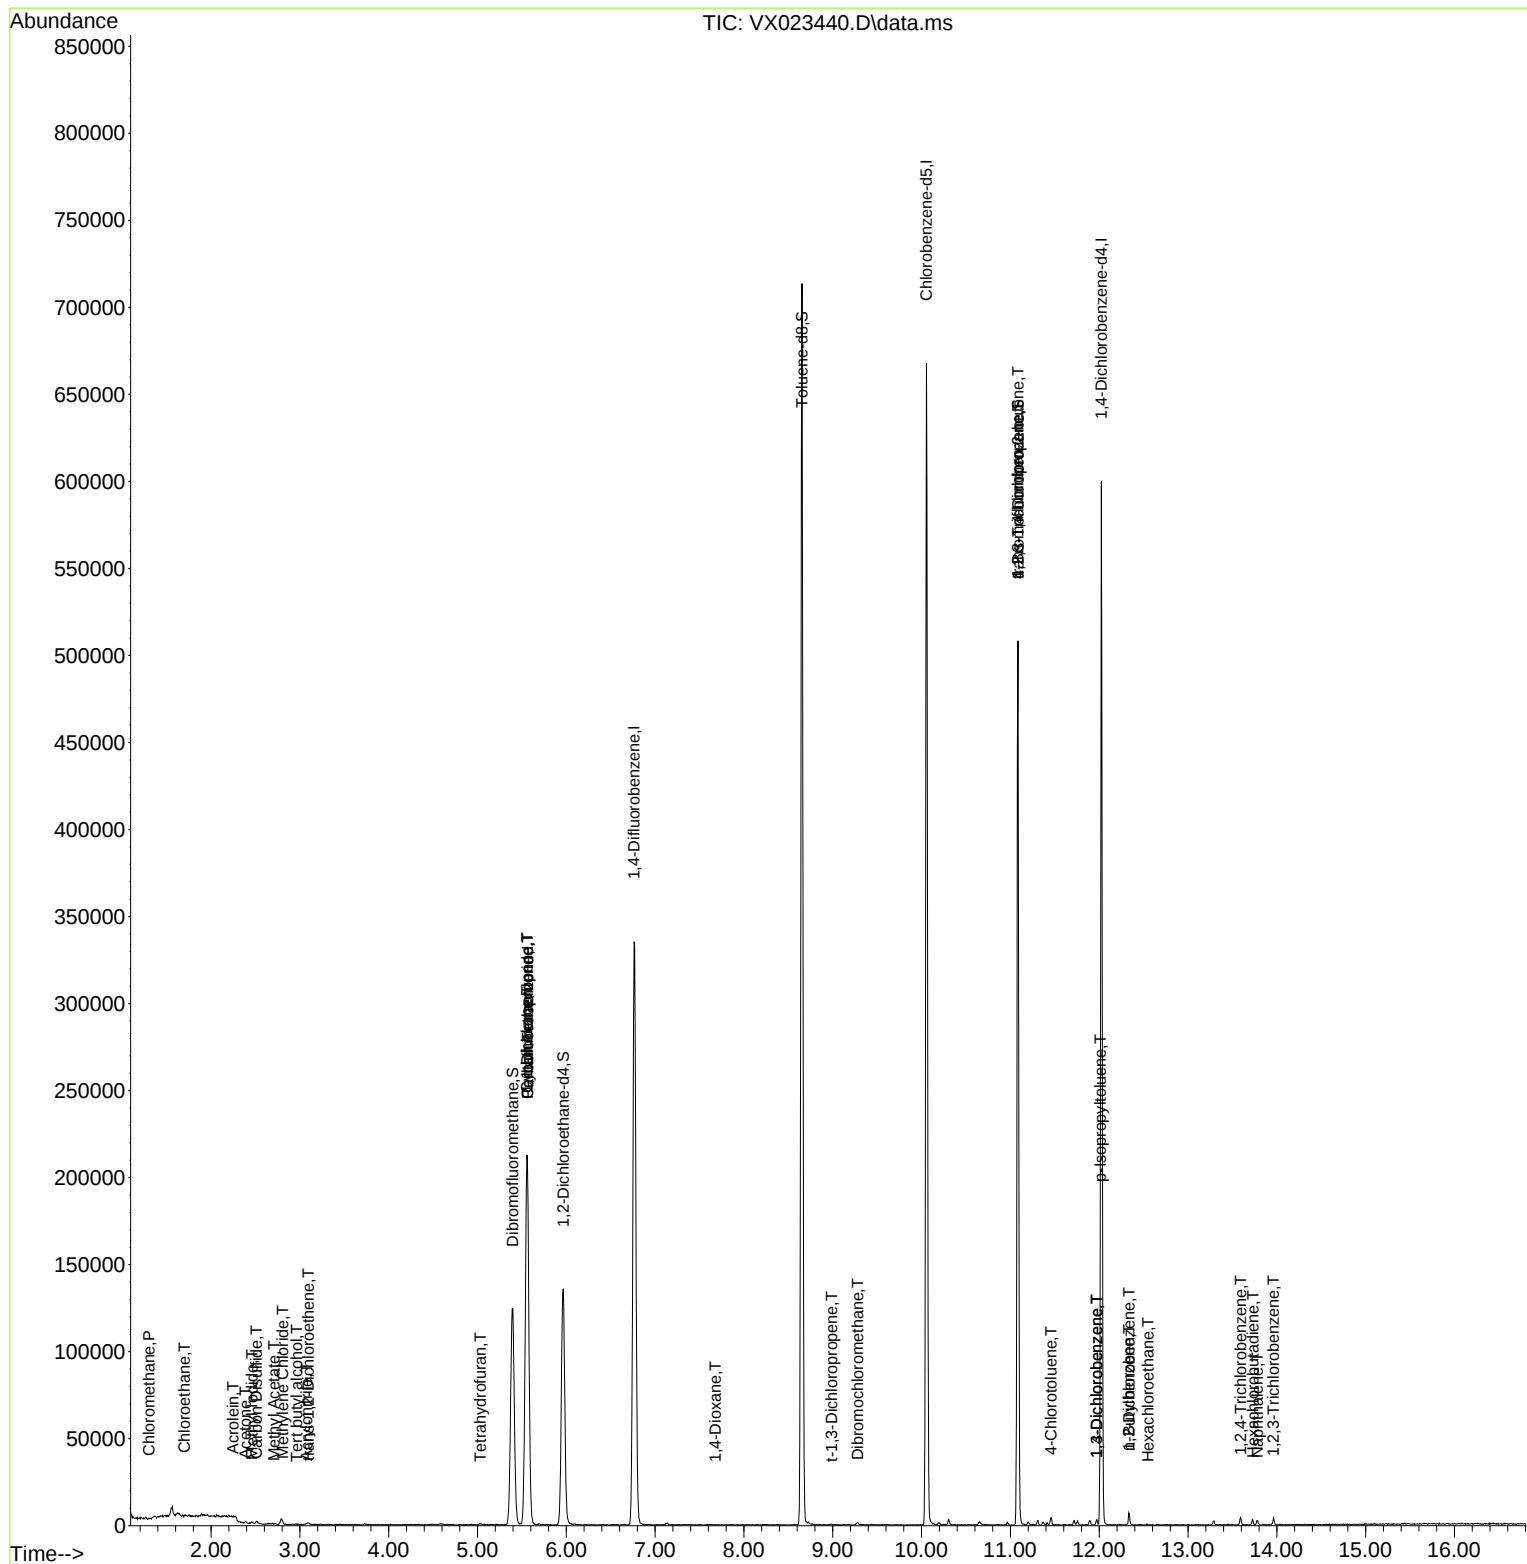




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 203035
Ion Ratio Lower Upper
168 100
99 55.9 45.8 68.6

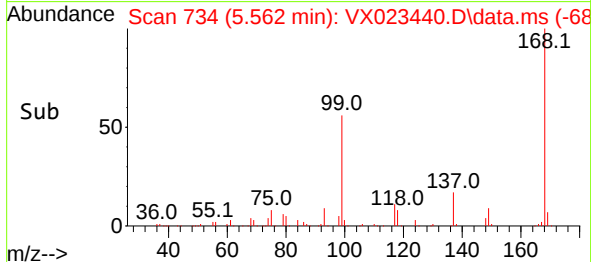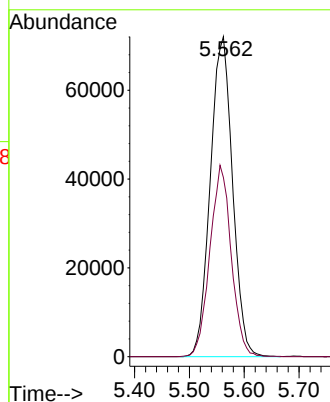

#3
Chloromethane
Concen: 0.32 ug/l
RT: 1.300 min Scan# 35
Delta R.T. 0.006 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 50 Resp: 703
Ion Ratio Lower Upper
50 100
52 41.9 26.4 39.6#


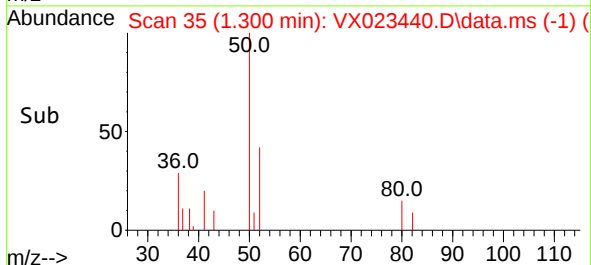

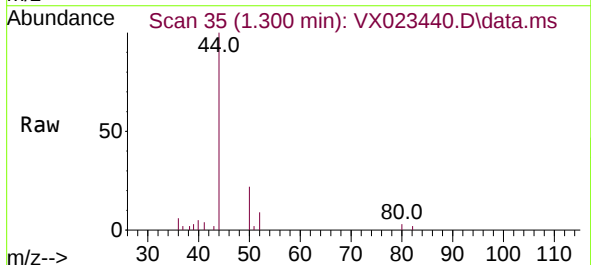


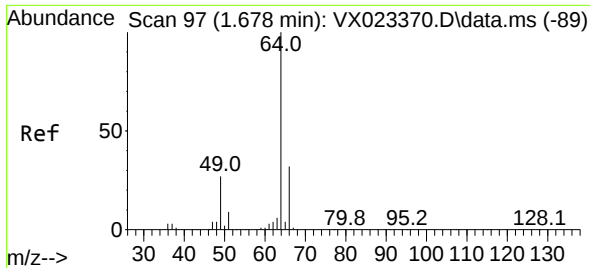

#6
Chloroethane
Concen: 0.23 ug/l
RT: 1.697 min Scan# 100
Delta R.T. 0.019 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 64 Resp: 309
Ion Ratio Lower Upper
64 100
66 31.6 25.4 38.0

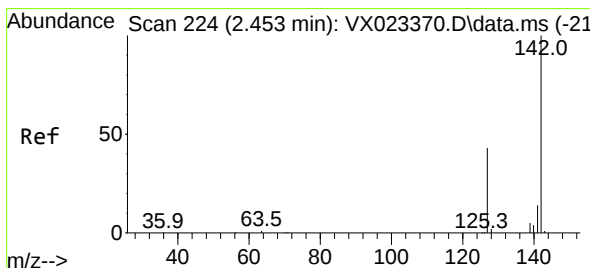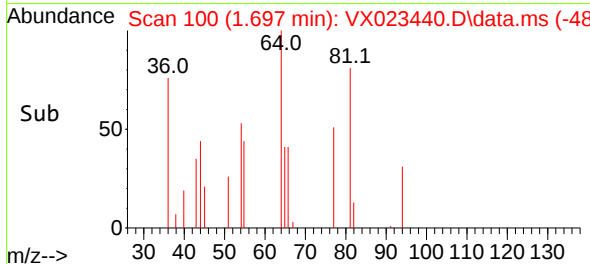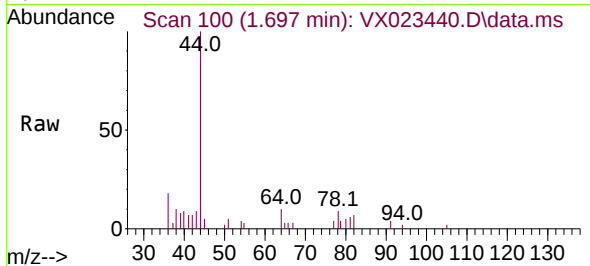

#10
Methyl Iodide
Concen: 0.52 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 142 Resp: 1305
Ion Ratio Lower Upper
142 100
127 40.5 33.3 49.9
141 17.1 11.4 17.0#

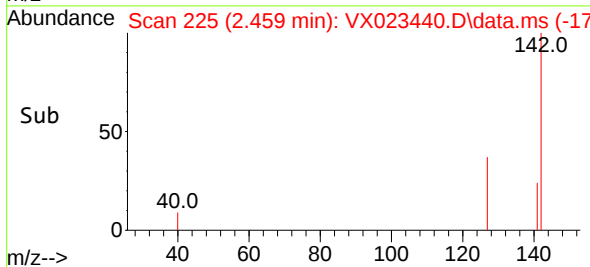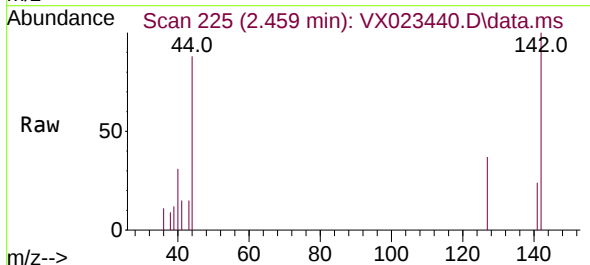







#11

Tert butyl alcohol
Concen: 0.38 ug/l
RT: 2.965 min Scan# 308
Delta R.T. -0.018 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Instrument :
MSVOA_X
ClientSampled :




Tgt Ion: 59 Resp: 218
Ion Ratio Lower Upper
59 100
57 10.1 7.8 11.8

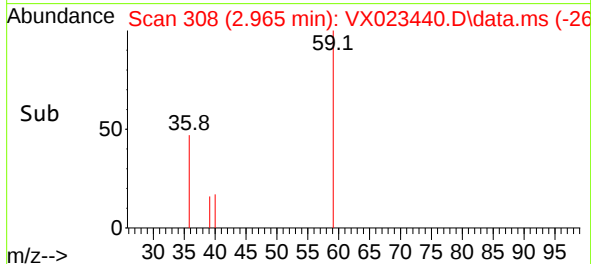


#13

Acrolein
Concen: 2.52 ug/l
RT: 2.245 min Scan# 190
Delta R.T. 0.006 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 56 Resp: 341
Ion Ratio Lower Upper
56 100
55 123.8 56.4 84.6#




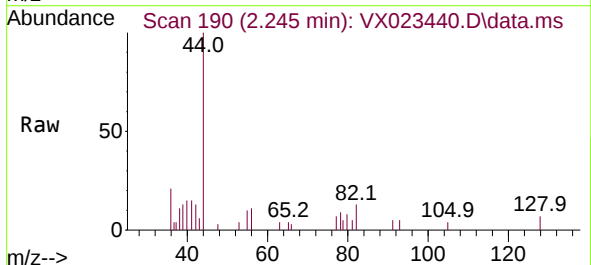




#15
Acrylonitrile
Concen: 0.32 ug/l
RT: 3.074 min Scan# 326
Delta R.T. -0.001 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 53 Resp: 424
Ion Ratio Lower Upper
53 100
52 87.7 65.3 97.9
51 15.1 28.2 42.2#

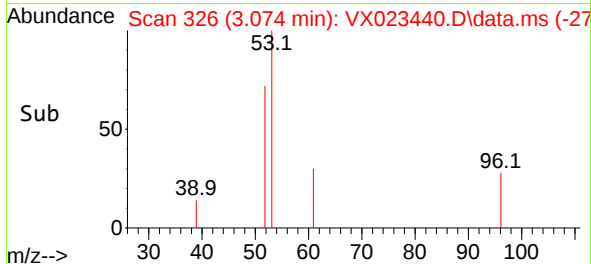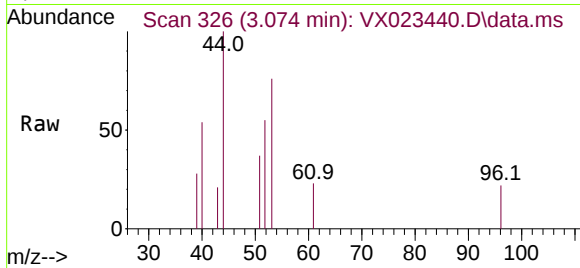

#16
Acetone
Concen: 1.16 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 43 Resp: 1444
Ion Ratio Lower Upper
43 100
58 31.1 27.8 41.8


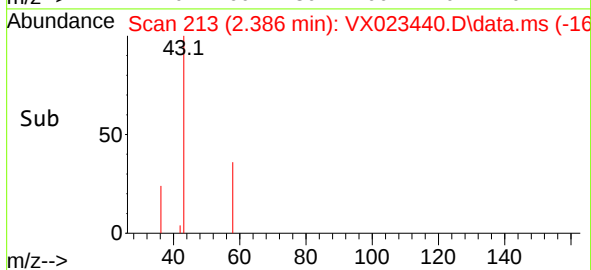

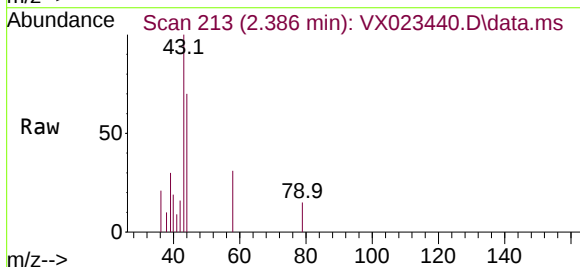




#17
Carbon Disulfide
Concen: 0.42 ug/l
RT: 2.507 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 76 Resp: 2046
Ion Ratio Lower Upper
76 100
78 10.0 7.2 10.8

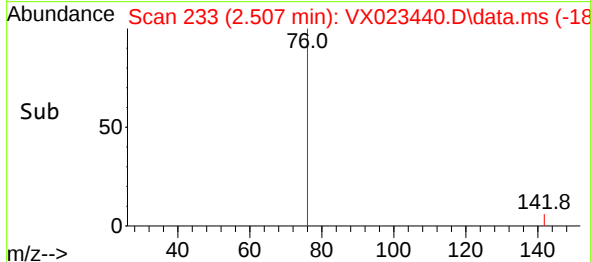

#18
Methyl Acetate
Concen: 0.22 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46


Tgt Ion: 43 Resp: 649
Ion Ratio Lower Upper
43 100
74 3.4 21.9 32.9#

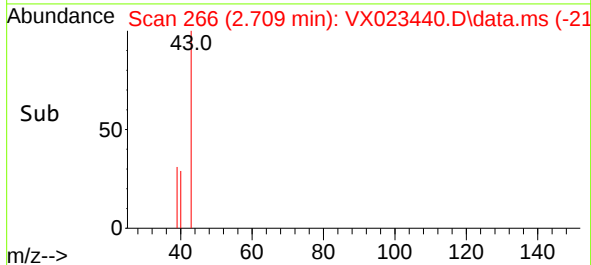






#20
Methylene Chloride
Concen: 0.53 ug/l
RT: 2.806 min Scan# 282
Delta R.T. 0.012 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Instrument :
MSVOA_X
ClientSampled :







Tgt Ion: 84 Resp: 1280
Ion Ratio Lower Upper
84 100
49 50.3 88.6 132.8#
51 19.2 27.0 40.6#
86 34.4 50.3 75.5#

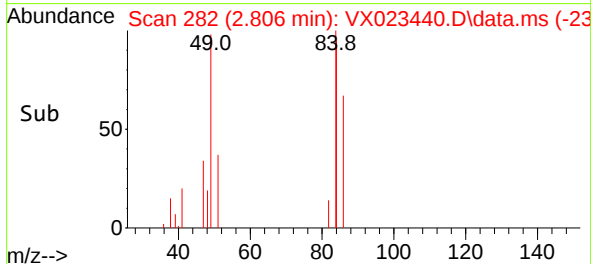

#21
trans-1,2-Dichloroethene
Concen: 0.20 ug/l
RT: 3.093 min Scan# 329
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 96 Resp: 432
Ion Ratio Lower Upper
96 100
61 153.9 107.7 161.5
98 41.6 50.4 75.6#



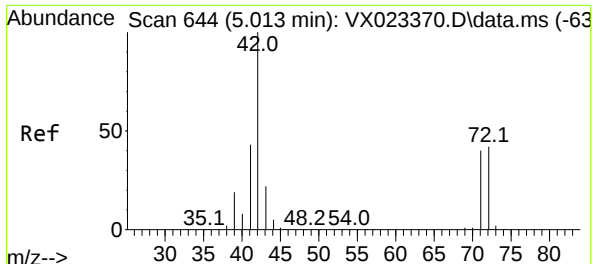

#29

Tetrahydrofuran

Concen: 0.29 ug/l

RT: 5.031 min Scan# 647





Delta R.T. 0.018 min

Lab File: VX023440.D

Acq: 26 Jul 2021 10:46

Tgt Ion:	42	Resp:	366
Ion	Ratio	Lower	Upper
42	100		
72	13.1	41.7	62.5#
71	32.0	38.4	57.6#

Instrument :
MSVOA_X
ClientSampleId :

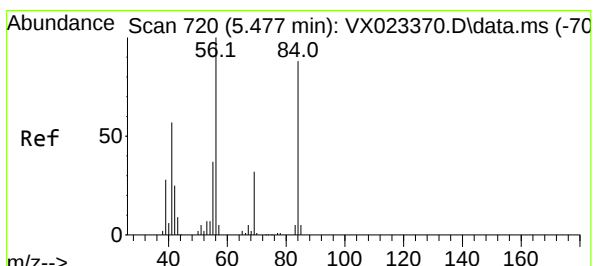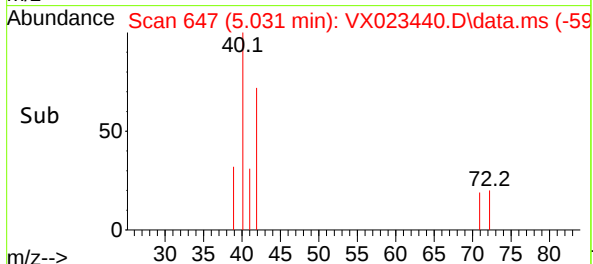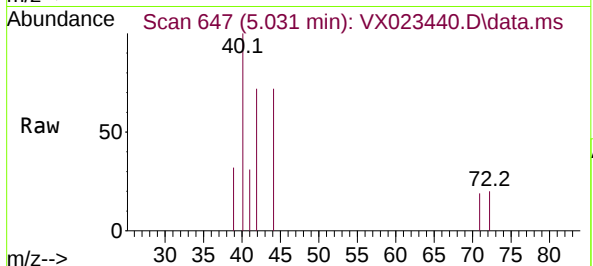

#31

Cyclohexane

Concen: 1.21 ug/l




RT: 5.556 min Scan# 733


Delta R.T. 0.079 min

Lab File: VX023440.D

Acq: 26 Jul 2021 10:46

Tgt Ion:	56	Resp:	4537
Ion	Ratio	Lower	Upper
56	100		
69	152.9	25.3	37.9#
84	154.4	71.4	107.0#

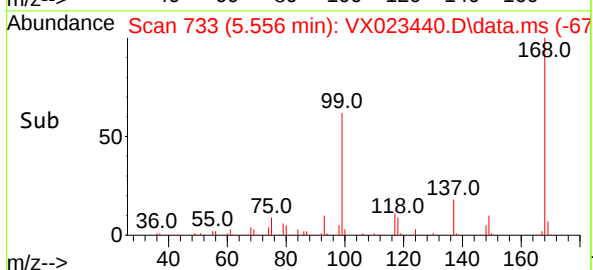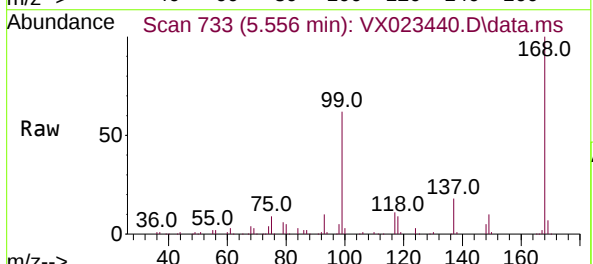

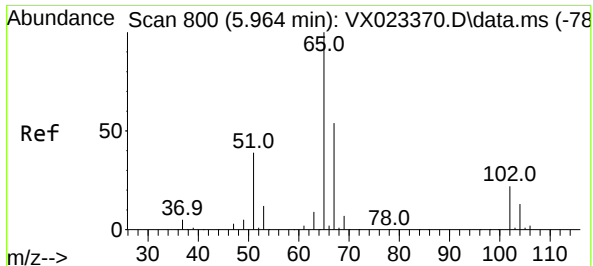

#33

1,2-Dichloroethane-d4

Concen: 51.84 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX023440.D

Acq: 26 Jul 2021 10:46

Tgt Ion: 65 Resp: 131294

Ion Ratio Lower Upper





65 100

67 53.1 0.0 105.4

Instrument :

MSVOA_X

ClientSampled :

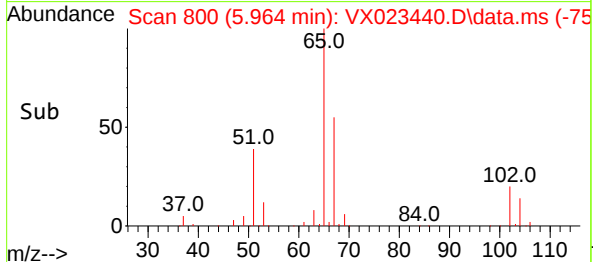

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.006 min

Lab File: VX023440.D

Acq: 26 Jul 2021 10:46




Tgt Ion: 114 Resp: 346586


Ion Ratio Lower Upper

114 100

63 19.8 0.0 40.8

88 15.4 0.0 32.8

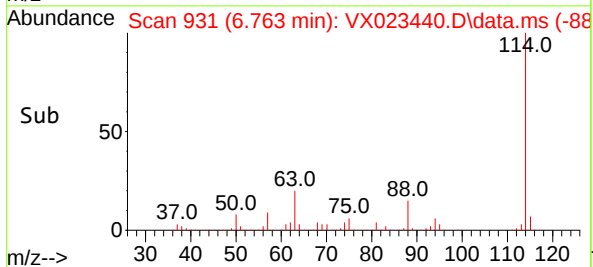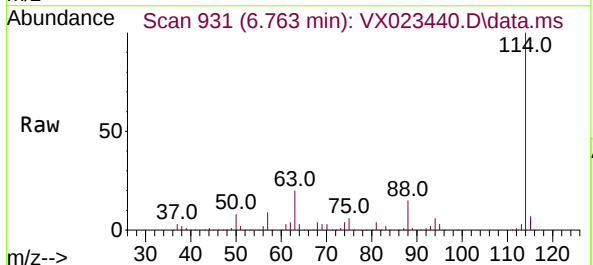

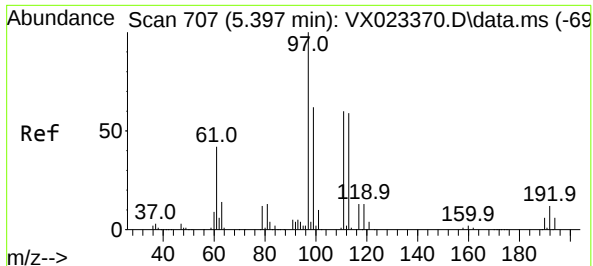

#35

Dibromofluoromethane

Concen: 49.88 ug/l

RT: 5.397 min Scan# 707

Delta R.T. 0.000 min

Lab File: VX023440.D

Acq: 26 Jul 2021 10:46





Tgt Ion:113 Resp: 108093

Ion Ratio Lower Upper

113 100

111 103.1 81.9 122.9

192 20.6 16.7 25.1

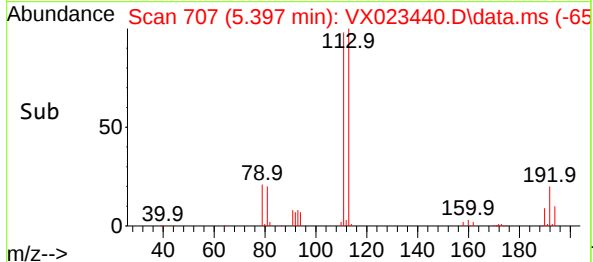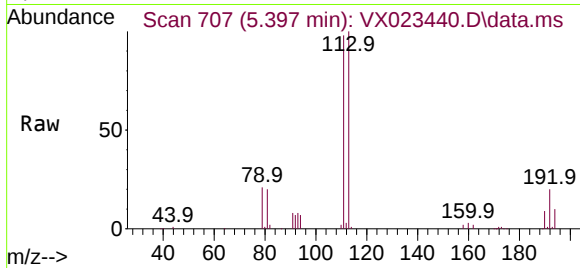

#36

1,1-Dichloropropene

Concen: 5.08 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX023440.D

Acq: 26 Jul 2021 10:46




Tgt Ion: 75 Resp: 15935


Ion Ratio Lower Upper

75 100

110 5.7 18.1 54.4#


77 0.0 25.3 37.9#

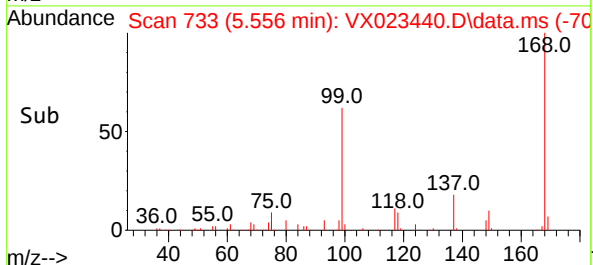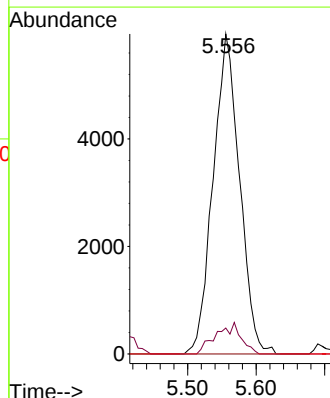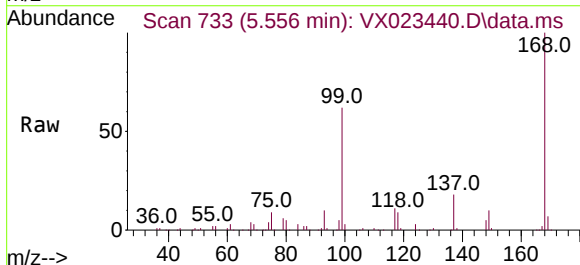



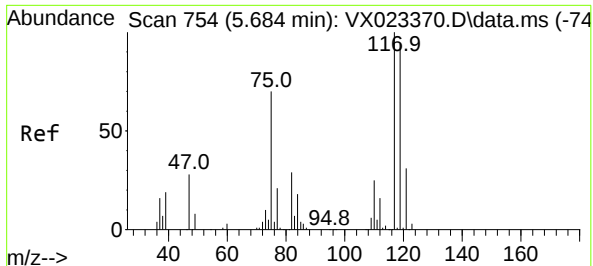


#38
Carbon Tetrachloride
Concen: 6.54 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.122 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 20856
Ion Ratio Lower Upper
117 100
119 4.3 76.2 114.2#
121 0.0 24.8 37.2#

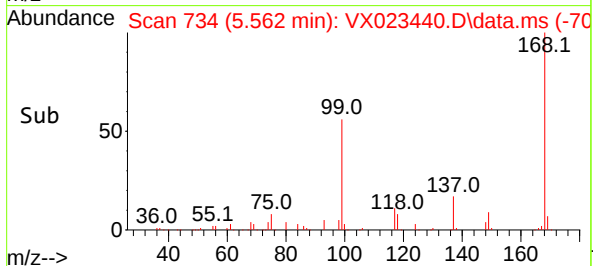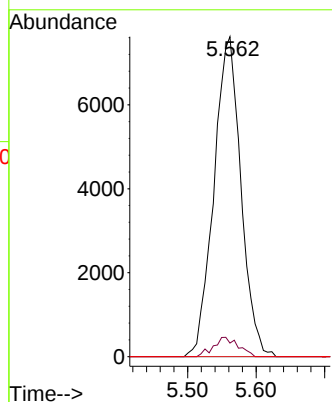

#49
1,4-Dioxane
Concen: 1.57 ug/l
RT: 7.677 min Scan# 1081
Delta R.T. 0.012 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 88 Resp: 95
Ion Ratio Lower Upper
88 100
43 51.6 23.2 34.8#
58 0.0 55.0 82.4#




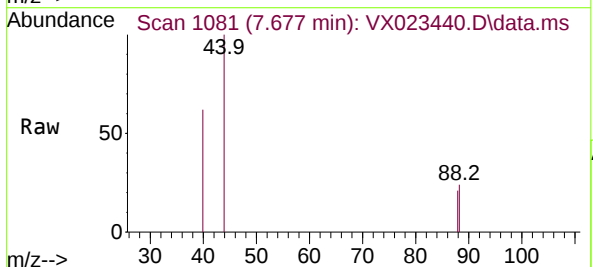


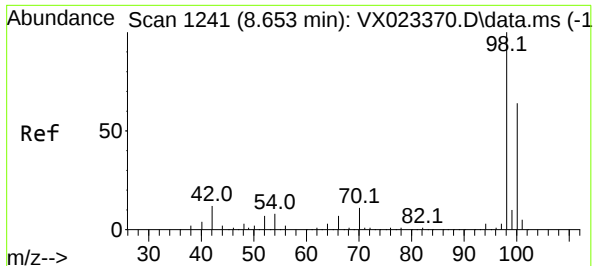

#50
Toluene-d8
Concen: 51.16 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 98 Resp: 407293
Ion Ratio Lower Upper
98 100
100 63.8 51.9 77.9

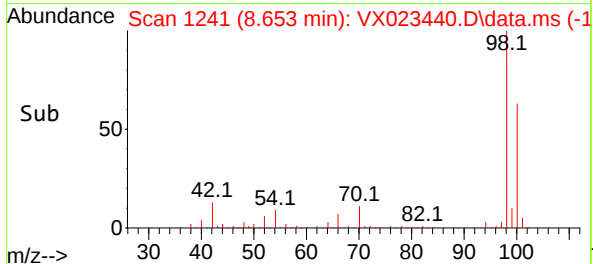

#53
t-1,3-Dichloropropene
Concen: 1.89 ug/l
RT: 8.988 min Scan# 1296
Delta R.T. 0.006 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 75 Resp: 308
Ion Ratio Lower Upper
75 100
77 47.6 24.9 37.3#


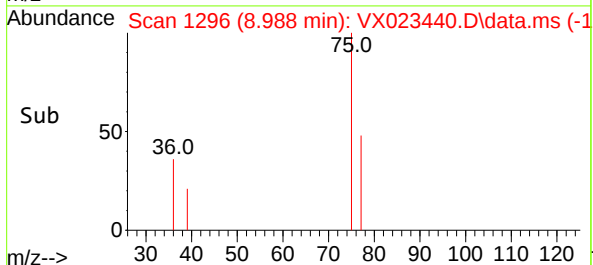

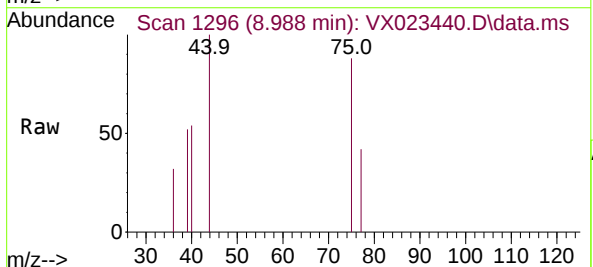


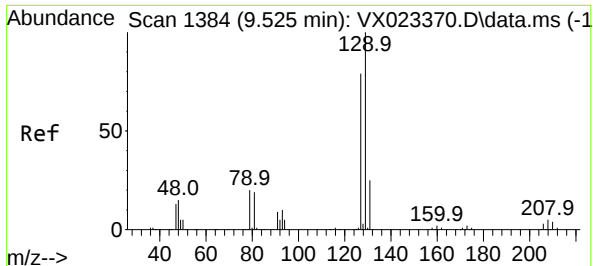

#60
Dibromochloromethane
Concen: 2.07 ug/l
RT: 9.281 min Scan# 1344
Delta R.T. -0.244 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:129 Resp: 242
Ion Ratio Lower Upper
129 100
127 0.0 38.4 115.2#

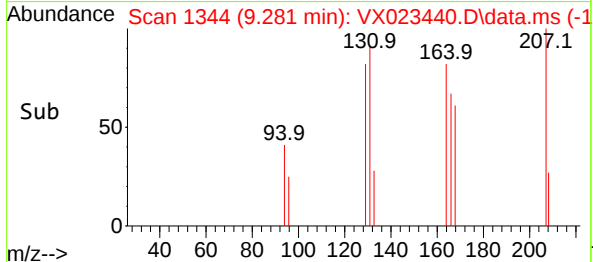

#62
4-Bromofluorobenzene
Concen: 48.17 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 95 Resp: 130401
Ion Ratio Lower Upper
95 100
174 82.6 0.0 154.6
176 78.1 0.0 155.8


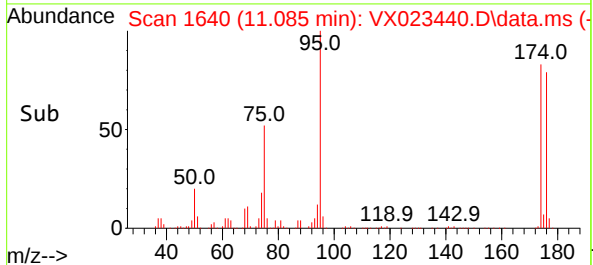

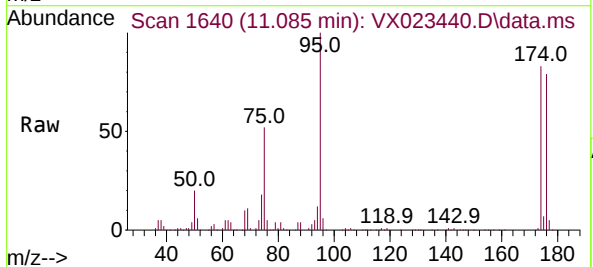




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:117 Resp: 299668
Ion Ratio Lower Upper
117 100
82 56.4 47.4 71.2
119 32.1 26.6 39.8

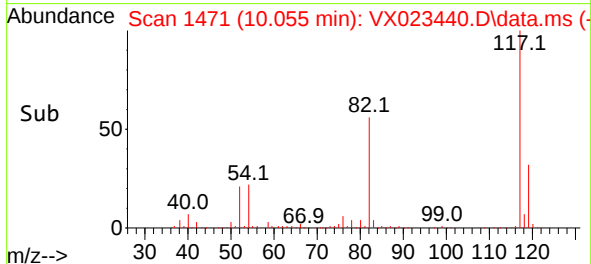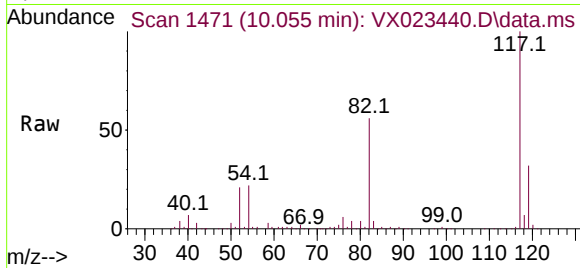

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion:152 Resp: 118584
Ion Ratio Lower Upper
152 100
115 59.0 41.1 123.3
150 157.4 0.0 349.0


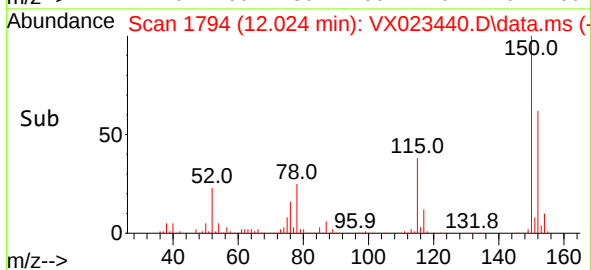






#76
1,2,3-Trichloropropane
Concen: 25.80 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 75 Resp: 67322
Ion Ratio Lower Upper
75 100
77 1.2 19.1 57.5#

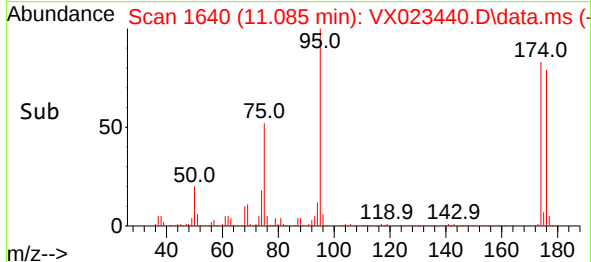

#81
trans-1,4-Dichloro-2-butene
Concen: 69.37 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.061 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 75 Resp: 67322
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.1 37.9 56.9#









#82
4-Chlorotoluene
Concen: 0.21 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 1437
Ion Ratio Lower Upper
91 100
126 31.5 14.9 44.5

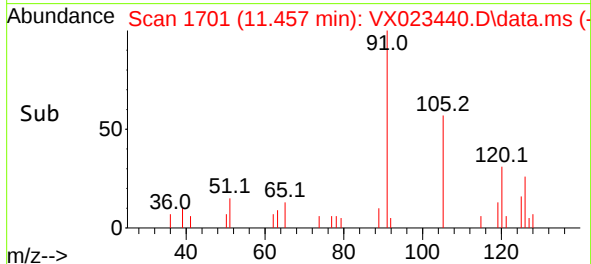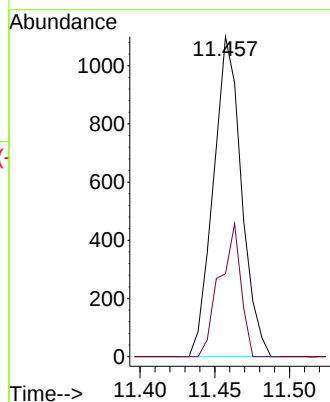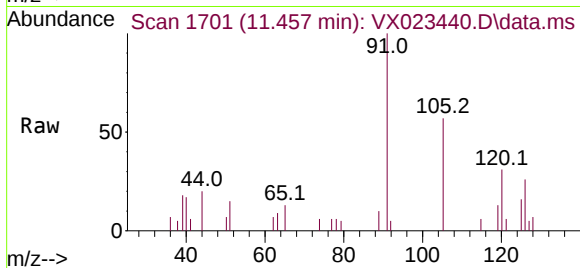

#86
p-Isopropyltoluene
Concen: 0.23 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 119 Resp: 1694
Ion Ratio Lower Upper
119 100
134 34.3 12.9 38.7
91 46.3 11.7 35.0#

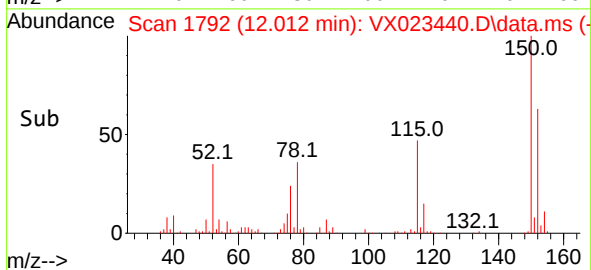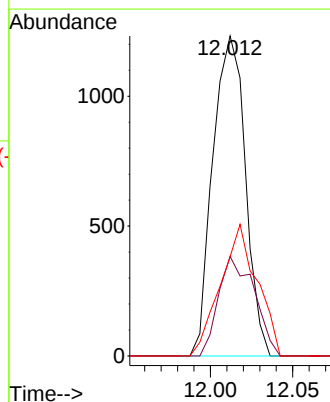



#87

1,3-Dichlorobenzene

Concen: 0.31 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. -0.006 min

Lab File: VX023440.D

Acq: 26 Jul 2021 10:46





Tgt Ion:146 Resp: 1218

Ion Ratio Lower Upper

146 100

111 34.2 20.2 60.5

148 63.0 31.9 95.7

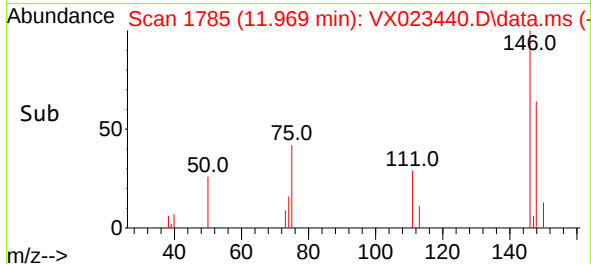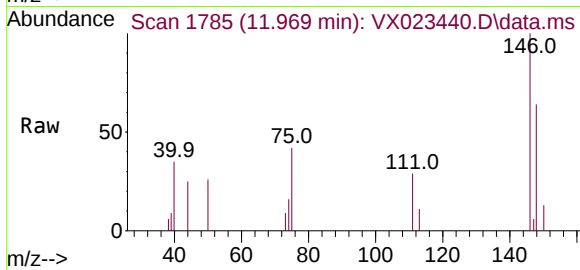

#88

1,4-Dichlorobenzene

Concen: 0.30 ug/l

RT: 11.969 min Scan# 1785

Delta R.T. -0.073 min

Lab File: VX023440.D

Acq: 26 Jul 2021 10:46




Tgt Ion:146 Resp: 1218


Ion Ratio Lower Upper

146 100

111 34.2 19.6 58.8

148 63.0 31.6 95.0



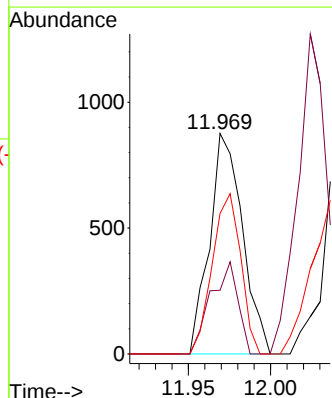
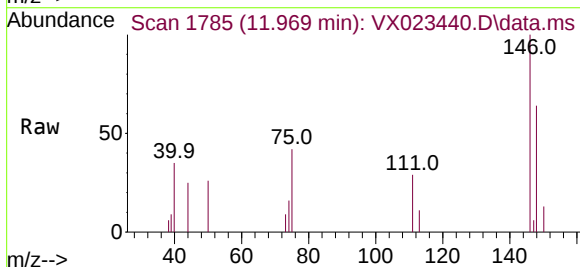




#89
n-Butylbenzene
Concen: 0.28 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion: 91 Resp: 1928
Ion Ratio Lower Upper
91 100
92 52.6 27.4 82.0
134 21.0 13.2 39.5

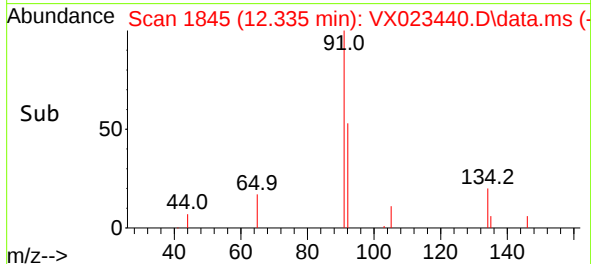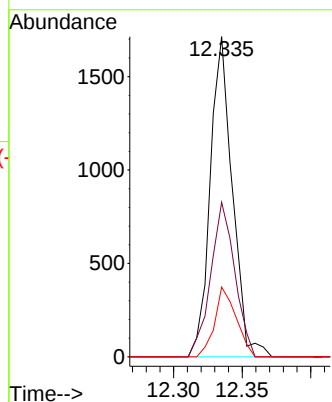

#90
Hexachloroethane
Concen: 1.96 ug/l
RT: 12.548 min Scan# 1880
Delta R.T. 0.006 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion: 117 Resp: 90
Ion Ratio Lower Upper
117 100
201 40.0 40.4 121.2#



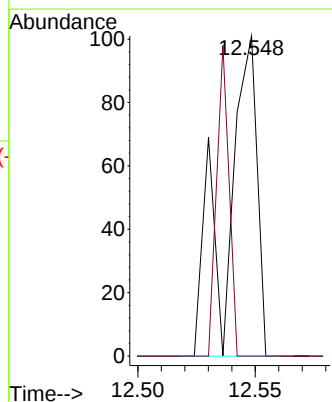





#91
1,2-Dichlorobenzene
Concen: 0.22 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.006 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:146 Resp: 860
Ion Ratio Lower Upper
146 100
111 51.7 20.8 62.2
148 70.3 31.9 95.5

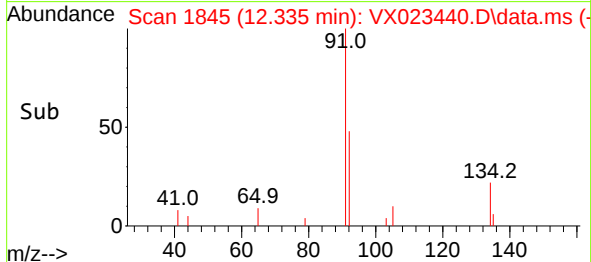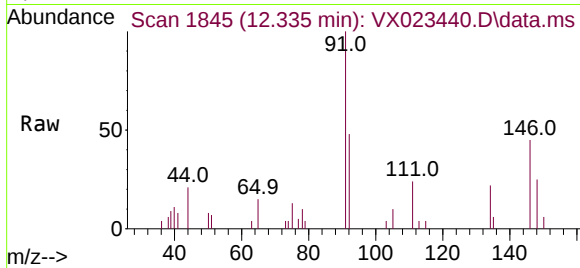

#93
1,2,4-Trichlorobenzene
Concen: 0.46 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion:180 Resp: 1114
Ion Ratio Lower Upper
180 100
182 85.5 47.7 143.1
145 33.0 15.0 45.0




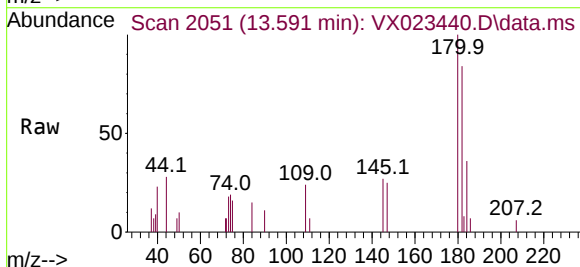




#94
Hexachlorobutadiene
Concen: 0.42 ug/l
RT: 13.731 min Scan# 2074
Delta R.T. 0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46




Instrument :
MSVOA_X
ClientSampled :


Tgt Ion:225 Resp: 453
Ion Ratio Lower Upper
225 100
223 77.0 31.1 93.2
227 64.0 31.6 95.0

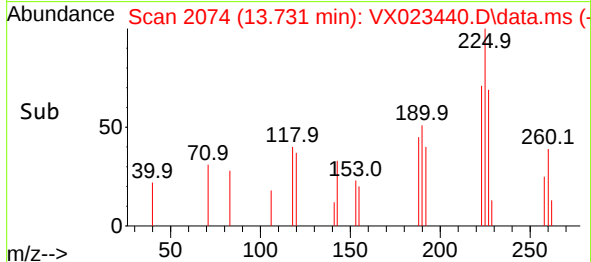

#95
Naphthalene
Concen: 0.23 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX023440.D
Acq: 26 Jul 2021 10:46

Tgt Ion:128 Resp: 1890
Ion Ratio Lower Upper
128 100
127 9.4 10.3 15.5#
129 12.5 8.8 13.2

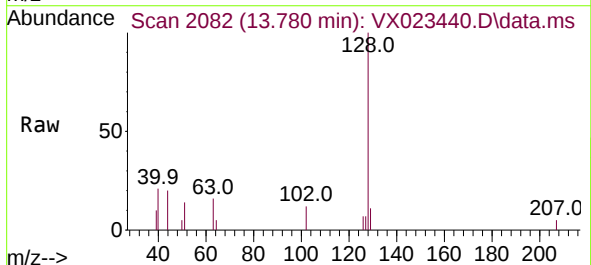



#96
 1,2,3-Trichlorobenzene
 Concen: 0.38 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. -0.000 min
 Lab File: VX023440.D
 Acq: 26 Jul 2021 10:46

Instrument :
 MSVOA_X
 ClientSampleId :

Tgt Ion:180 Resp: 931
 Ion Ratio Lower Upper
 180 100
 182 110.2 47.6 142.9
 145 26.2 16.1 48.3

