

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
 Data File : VX023444.D
 Acq On : 26 Jul 2021 12:29
 Operator : JC/MD
 Sample : M3145-20 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-1-PDB

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rBV	103878	93268	9.04%	1.589%
2	1.562	70	78	83	rBV3	7036	15774	1.53%	0.269%
3	5.397	695	707	720	rBV	118753	348082	33.74%	5.931%
4	5.562	722	734	748	rVB	201395	567810	55.03%	9.675%
5	5.964	789	800	811	rBV	129349	346991	33.63%	5.913%
6	6.769	918	932	951	rBV	320322	759277	73.59%	12.938%
7	8.653	1234	1241	1250	rBV	670694	1031749	100.00%	17.581%
8	9.274	1337	1343	1352	rVB	379762	557772	54.06%	9.504%
9	10.055	1465	1471	1485	rBV	616918	857268	83.09%	14.608%
10	11.085	1634	1640	1653	rVB	487579	605324	58.67%	10.315%
11	12.024	1788	1794	1802	rBV	549930	685334	66.42%	11.678%


Sum of corrected areas: 5868649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023444.D
Acq On : 26 Jul 2021 12:29
Operator : JC/MD
Sample : M3145-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-1-PDB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

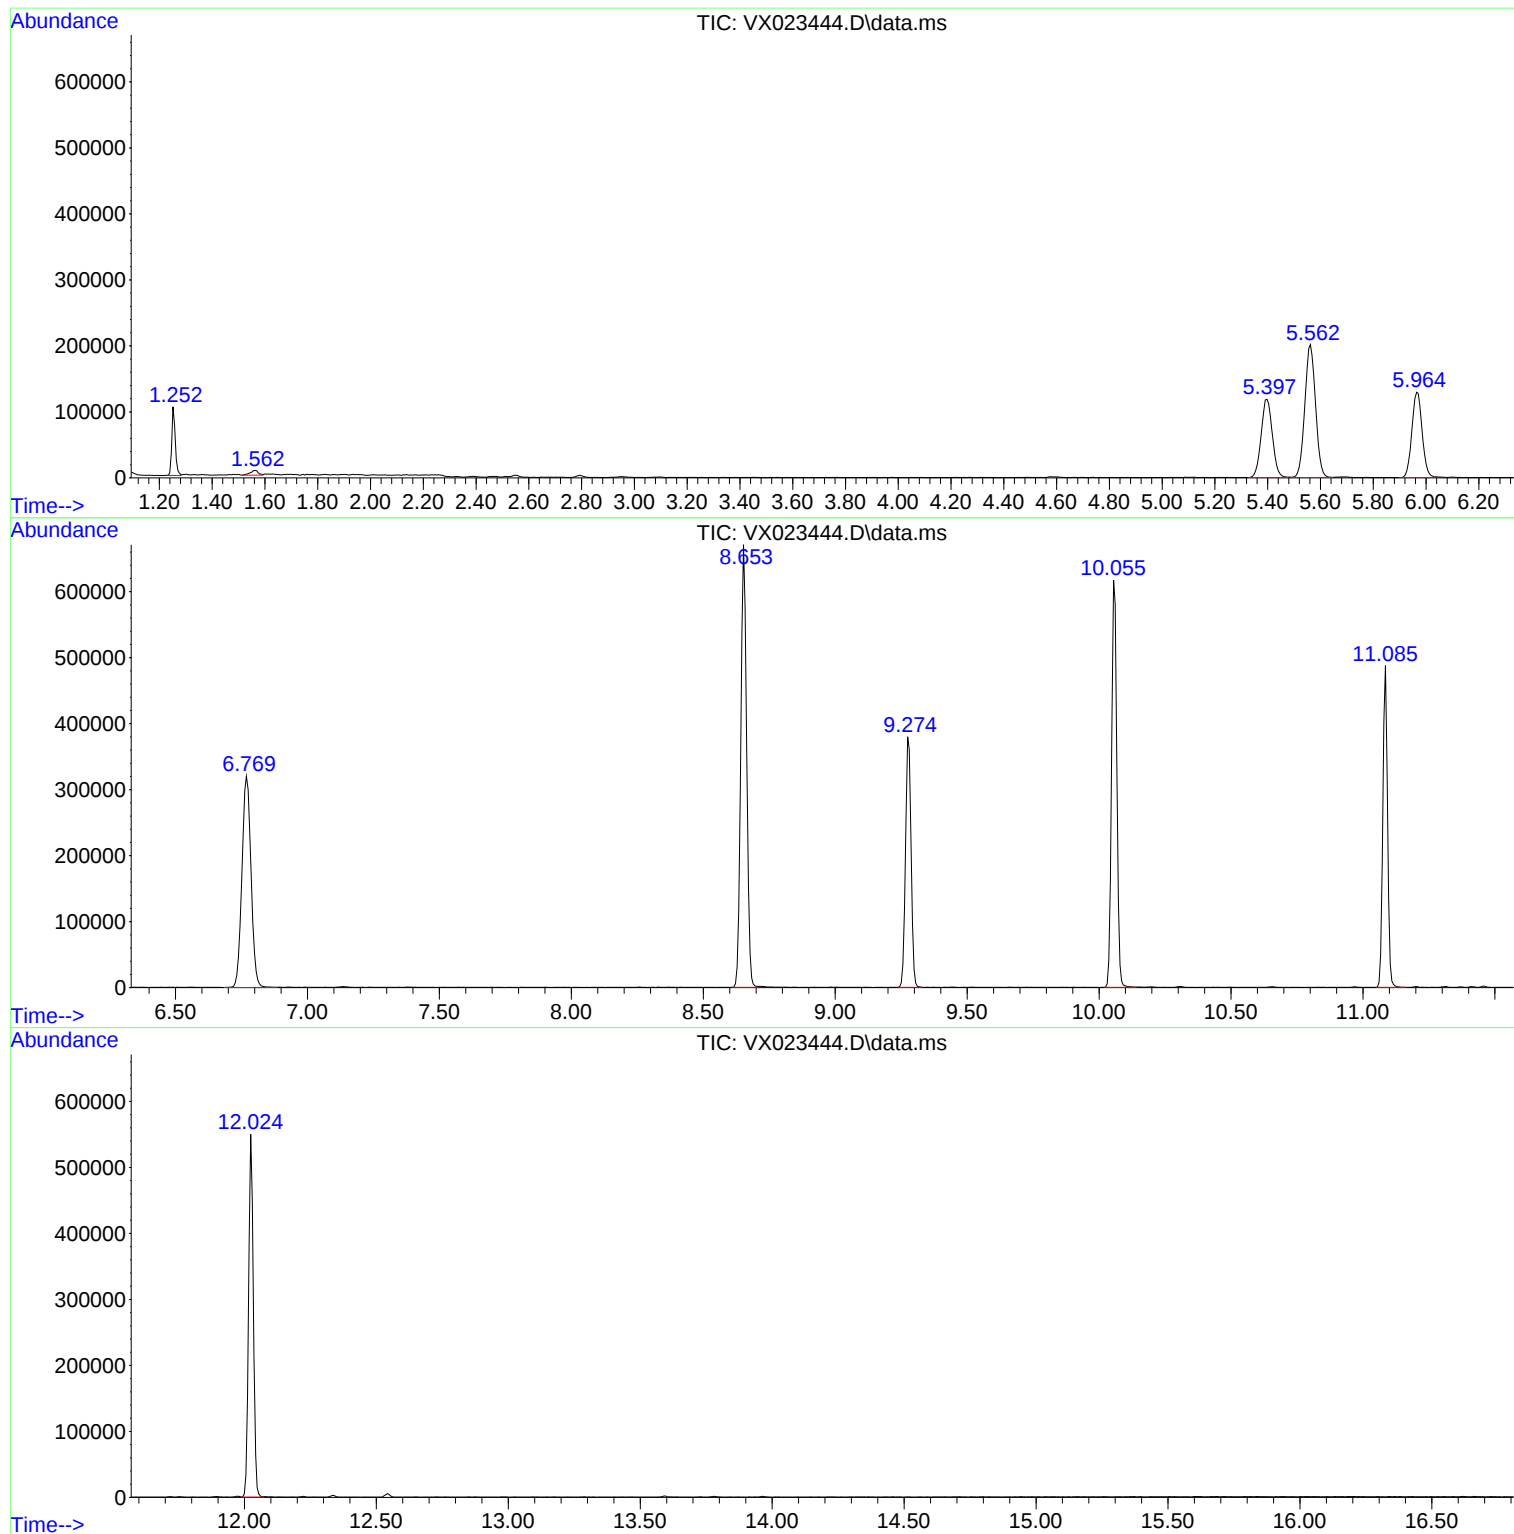

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023444.D
Acq On : 26 Jul 2021 12:29
Operator : JC/MD
Sample : M3145-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-1-PDB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023444.D
Acq On : 26 Jul 2021 12:29
Operator : JC/MD
Sample : M3145-20 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-1-PDB

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
