

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
 Data File : VX023447.D
 Acq On : 26 Jul 2021 13:39
 Operator : JC/MD
 Sample : M3145-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-10-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	69	79	82	rBV2	6136	12616	1.39%	0.279%
2	2.550	230	240	247	rVB2	5162	10266	1.13%	0.227%
3	4.501	551	560	570	rBV	12949	34099	3.76%	0.754%
4	5.397	696	707	721	rBV	103303	300226	33.14%	6.642%
5	5.562	721	734	747	rBV2	177415	496286	54.78%	10.980%
6	5.964	789	800	814	rBV	116128	302258	33.36%	6.687%
7	6.769	920	932	948	rBV	278547	657822	72.61%	14.553%
8	8.653	1234	1241	1255	rBV	588976	905946	100.00%	20.043%
9	10.055	1465	1471	1480	rBV	553262	752335	83.04%	16.644%
10	11.085	1634	1640	1651	rBV	406234	512852	56.61%	11.346%
11	12.024	1788	1794	1803	rBV	440203	535324	59.09%	11.843%


Sum of corrected areas: 4520030

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023447.D
Acq On : 26 Jul 2021 13:39
Operator : JC/MD
Sample : M3145-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-10-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

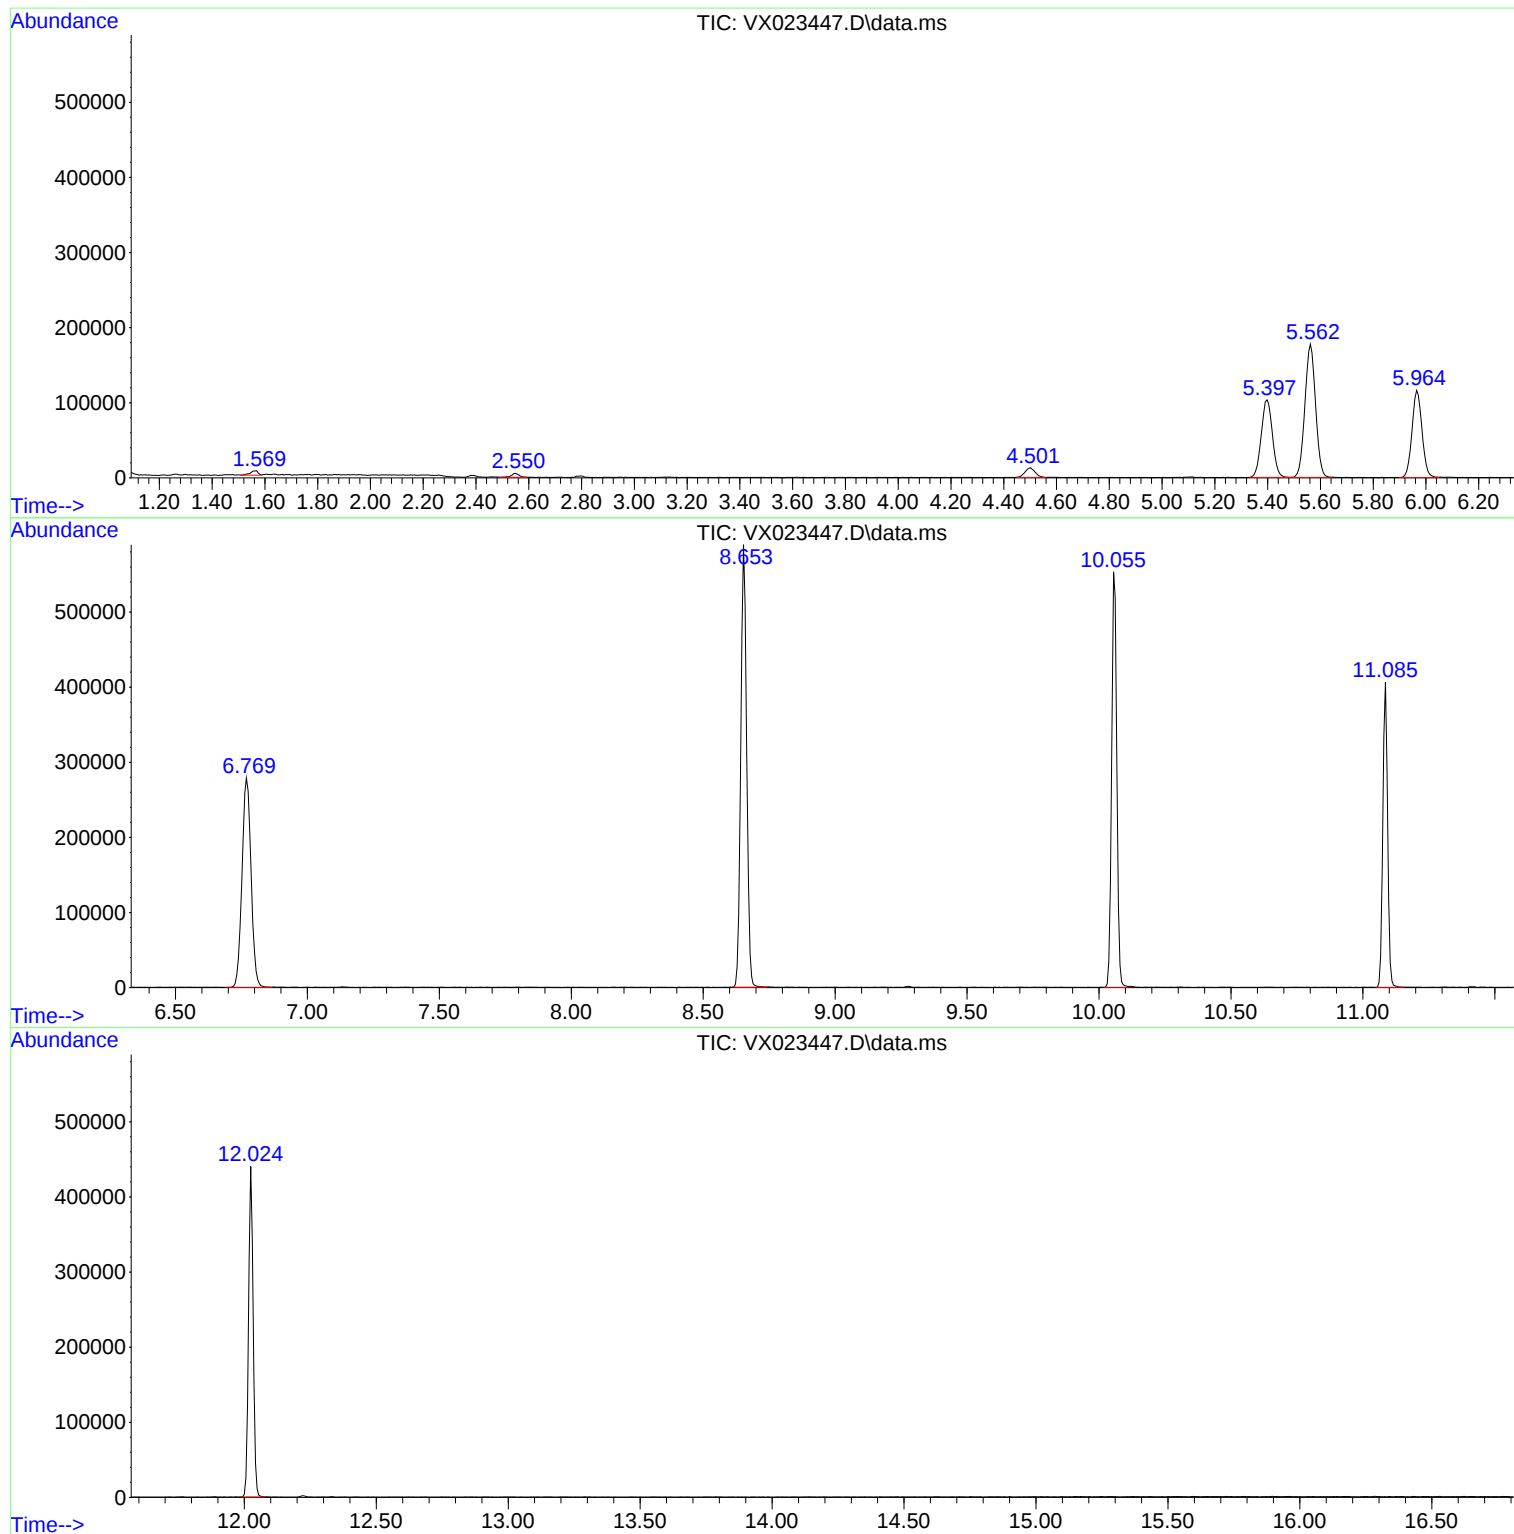

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023447.D
Acq On : 26 Jul 2021 13:39
Operator : JC/MD
Sample : M3145-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-10-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023447.D
Acq On : 26 Jul 2021 13:39
Operator : JC/MD
Sample : M3145-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-10-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
