

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
 Data File : VX023452.D
 Acq On : 26 Jul 2021 15:37
 Operator : JC/MD
 Sample : M3146-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-MW-1D(ONSITE)

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.550	232	240	248	rBV	5733	10537	1.22%	0.245%
2	5.397	695	707	722	rBV	100334	285900	33.23%	6.659%
3	5.562	722	734	748	rVB2	165866	468380	54.44%	10.909%
4	5.964	790	800	817	rBV	109028	290253	33.74%	6.760%
5	6.769	921	932	943	rBV	264438	624503	72.59%	14.546%
6	7.129	983	991	1000	rBV3	8871	18444	2.14%	0.430%
7	8.653	1234	1241	1250	rBV	562911	860345	100.00%	20.039%
8	9.275	1338	1343	1348	rVB3	11400	16575	1.93%	0.386%
9	10.055	1465	1471	1489	rVB	523399	712398	82.80%	16.593%
10	11.085	1634	1640	1651	rBV	388745	485446	56.42%	11.307%
11	12.024	1789	1794	1804	rBV	426149	520660	60.52%	12.127%


Sum of corrected areas: 4293441

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023452.D
Acq On : 26 Jul 2021 15:37
Operator : JC/MD
Sample : M3146-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-1D(ONSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

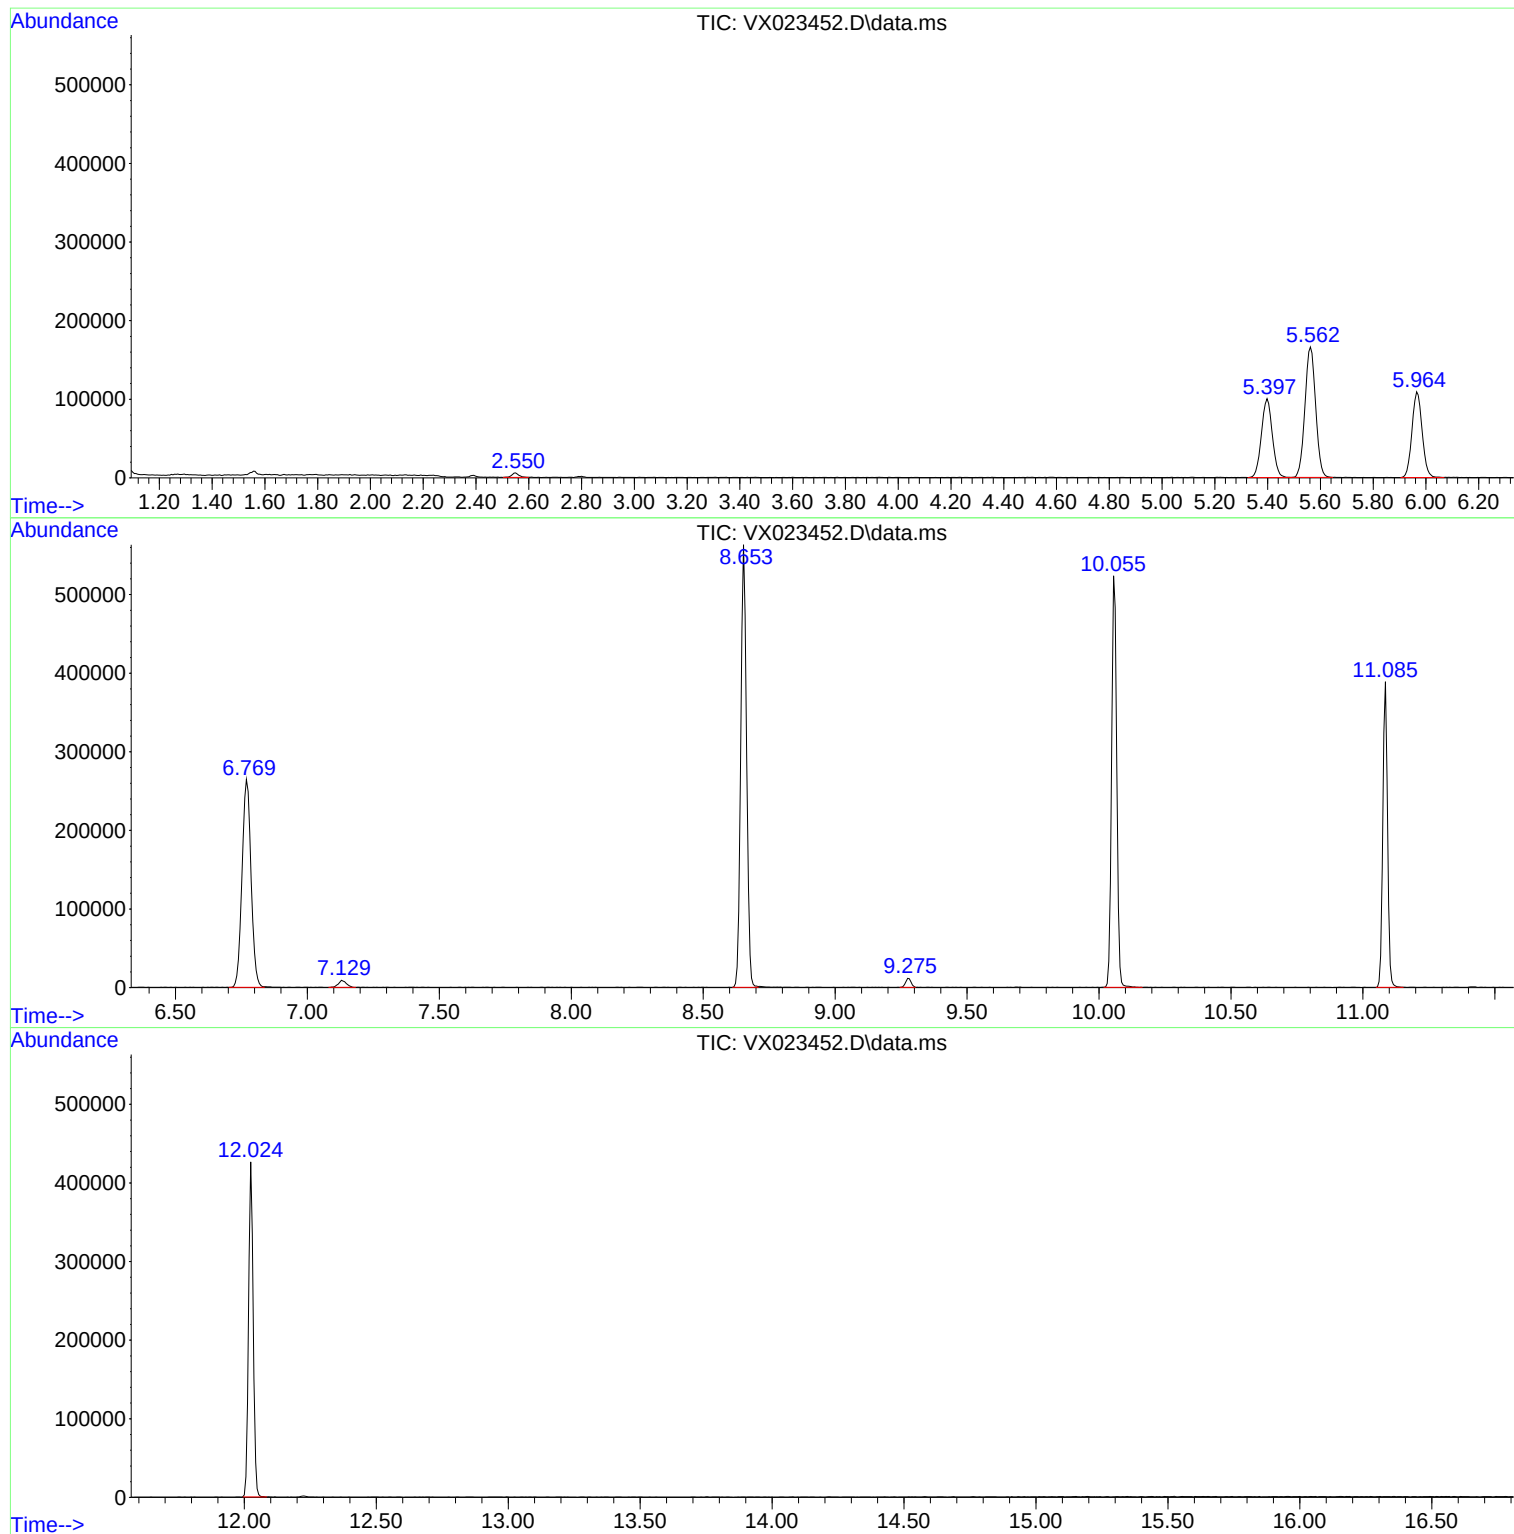

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023452.D
Acq On : 26 Jul 2021 15:37
Operator : JC/MD
Sample : M3146-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-1D(ONSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023452.D
Acq On : 26 Jul 2021 15:37
Operator : JC/MD
Sample : M3146-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-MW-1D(ONSITE)

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
