

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
 Data File : VX023456.D
 Acq On : 26 Jul 2021 17:12
 Operator : JC/MD
 Sample : M3146-03 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-6-PS

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Title : SW846 8260

Signal : TIC: VX023456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rBV	171838	150214	16.70%	3.191%
2	1.563	70	78	84	rVB6	5346	11726	1.30%	0.249%
3	5.397	694	707	719	rBV2	106418	302390	33.62%	6.424%
4	5.562	722	734	751	rVB	171516	490909	54.58%	10.429%
5	5.964	790	800	819	rBV	115344	302062	33.58%	6.417%
6	6.769	922	932	945	rBV	275403	652139	72.51%	13.855%
7	8.653	1233	1241	1253	rBV	591716	899439	100.00%	19.109%
8	10.055	1465	1471	1486	rBV	551918	762900	84.82%	16.208%
9	11.085	1634	1640	1653	rBV	426981	539962	60.03%	11.472%
10	12.024	1789	1794	1806	rVB	479323	595191	66.17%	12.645%




Sum of corrected areas: 4706932

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023456.D
Acq On : 26 Jul 2021 17:12
Operator : JC/MD
Sample : M3146-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

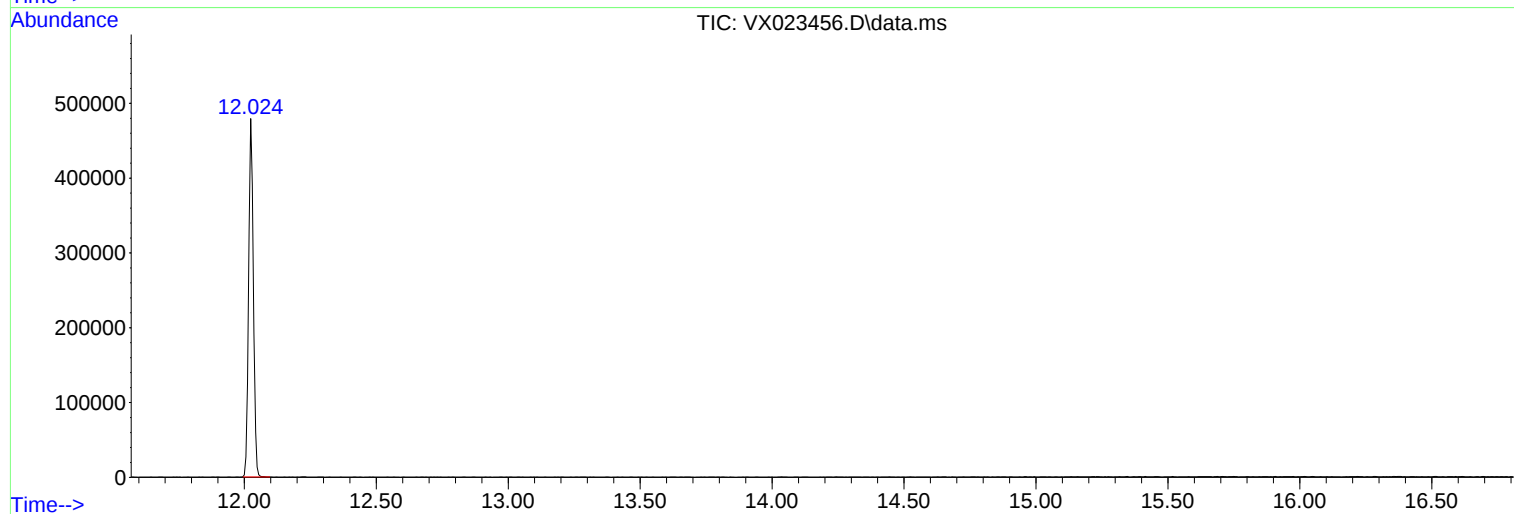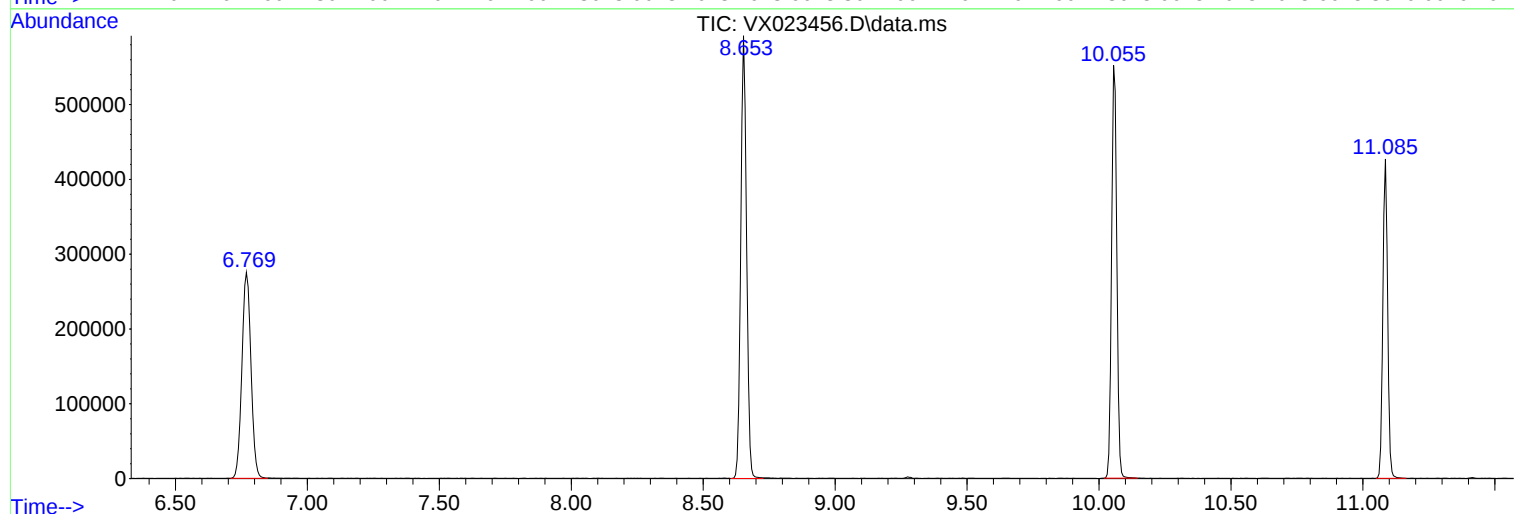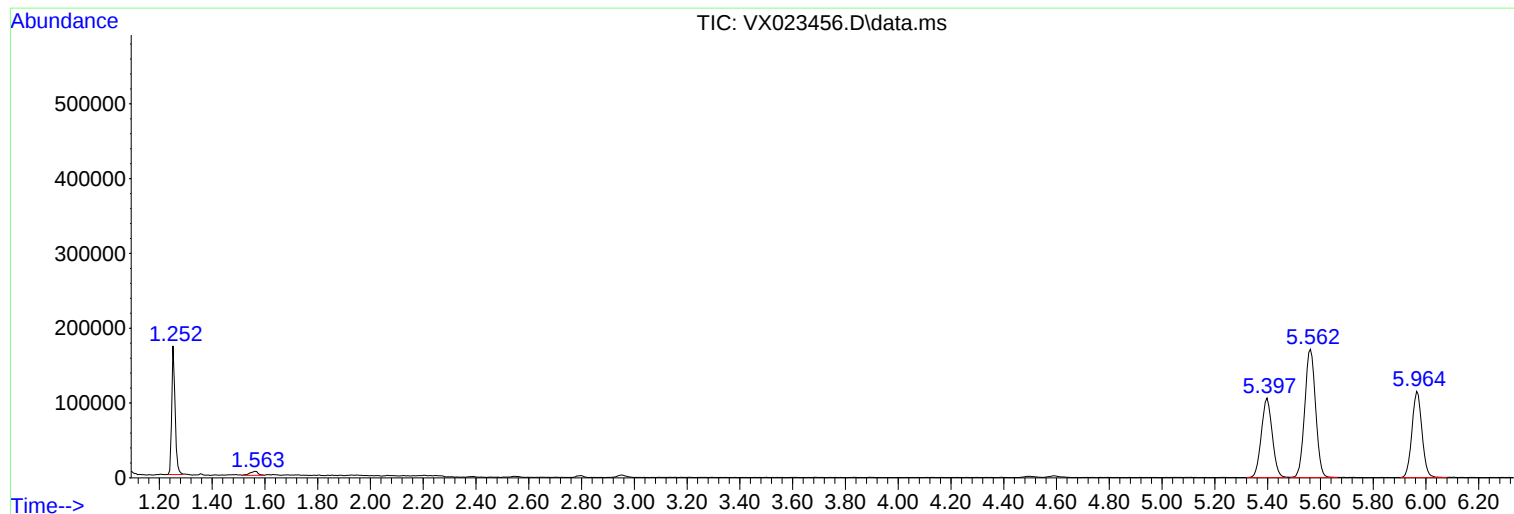

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023456.D
Acq On : 26 Jul 2021 17:12
Operator : JC/MD
Sample : M3146-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023456.D
Acq On : 26 Jul 2021 17:12
Operator : JC/MD
Sample : M3146-03 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------