

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
 Data File : VX023460.D
 Acq On : 26 Jul 2021 18:46
 Operator : JC/MD
 Sample : M3146-12 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-3-PS

Integration Parameters: RTEINT.P
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
 Title : SW846 8260

Signal : TIC: VX023460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	33	rBV	168088	150742	17.36%	3.258%
2	5.397	695	707	721	rBV	102784	296040	34.09%	6.398%
3	5.562	723	734	748	rVB	166955	473762	54.55%	10.240%
4	5.964	789	800	815	rBV	111100	297917	34.30%	6.439%
5	6.769	920	932	953	rBV	271481	641007	73.81%	13.854%
6	8.653	1234	1241	1251	rBV	563309	868497	100.00%	18.771%
7	9.275	1337	1343	1350	rVB	45674	66291	7.63%	1.433%
8	10.055	1465	1471	1486	rBV	536534	733870	84.50%	15.861%
9	11.085	1634	1640	1652	rBV	410064	515445	59.35%	11.140%
10	12.024	1789	1794	1803	rBV	480704	583199	67.15%	12.605%


Sum of corrected areas: 4626770

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023460.D
Acq On : 26 Jul 2021 18:46
Operator : JC/MD
Sample : M3146-12 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-3-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

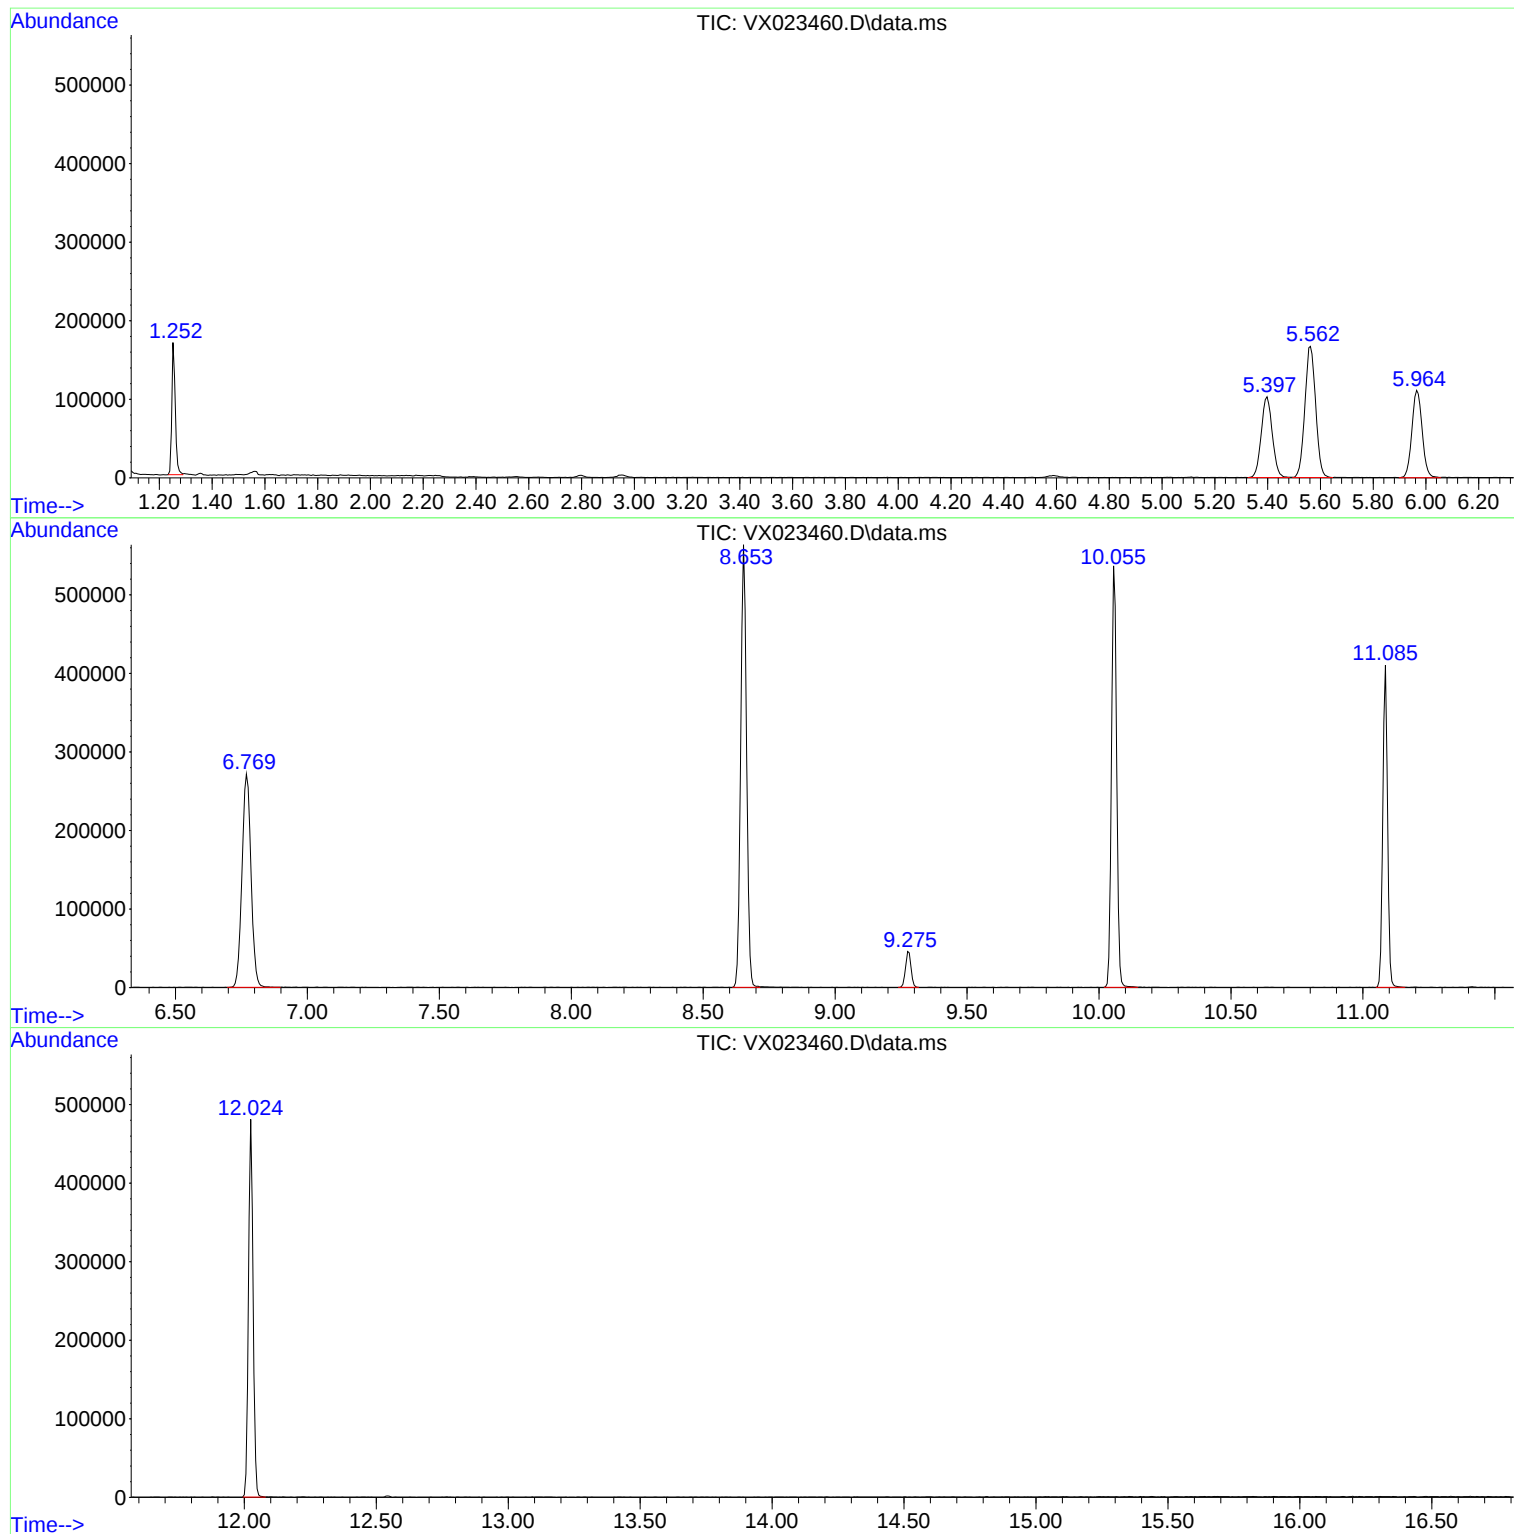

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023460.D
Acq On : 26 Jul 2021 18:46
Operator : JC/MD
Sample : M3146-12 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-3-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023460.D
Acq On : 26 Jul 2021 18:46
Operator : JC/MD
Sample : M3146-12 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-3-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
