

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
 Data File : VX023461.D
 Acq On : 26 Jul 2021 19:10
 Operator : JC/MD
 Sample : M3146-15 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-4-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023461.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	36	rVB	175246	157576	17.86%	3.394%
2	1.569	71	79	82	rBV3	5610	10521	1.19%	0.227%
3	5.397	691	707	721	rBV	104250	306385	34.73%	6.599%
4	5.562	721	734	747	rVB	172801	489177	55.44%	10.537%
5	5.964	790	800	815	rBV	116966	301980	34.23%	6.504%
6	6.769	921	932	944	rBV	275323	647394	73.37%	13.944%
7	8.653	1234	1241	1253	rBV	579500	882313	100.00%	19.004%
8	9.275	1337	1343	1348	rBV3	6607	10093	1.14%	0.217%
9	10.055	1465	1471	1488	rBV	542988	738198	83.67%	15.900%
10	11.085	1634	1640	1649	rBV	416697	516334	58.52%	11.121%
11	12.024	1789	1794	1803	rBV	469488	582701	66.04%	12.551%




Sum of corrected areas: 4642672

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023461.D
Acq On : 26 Jul 2021 19:10
Operator : JC/MD
Sample : M3146-15 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

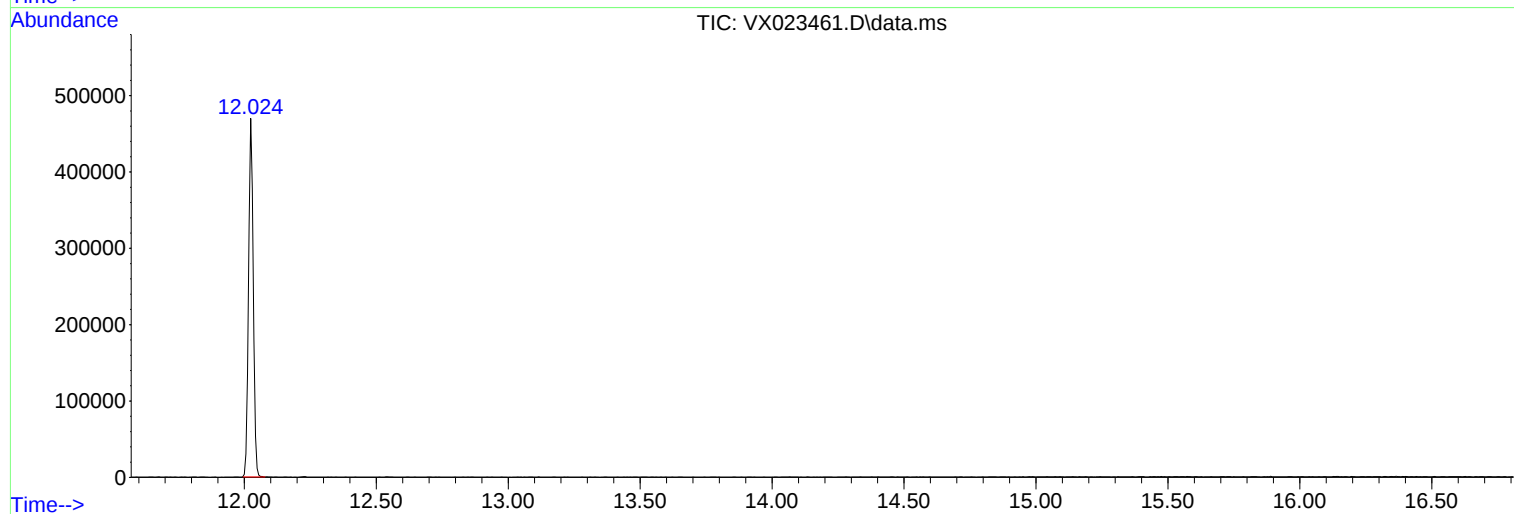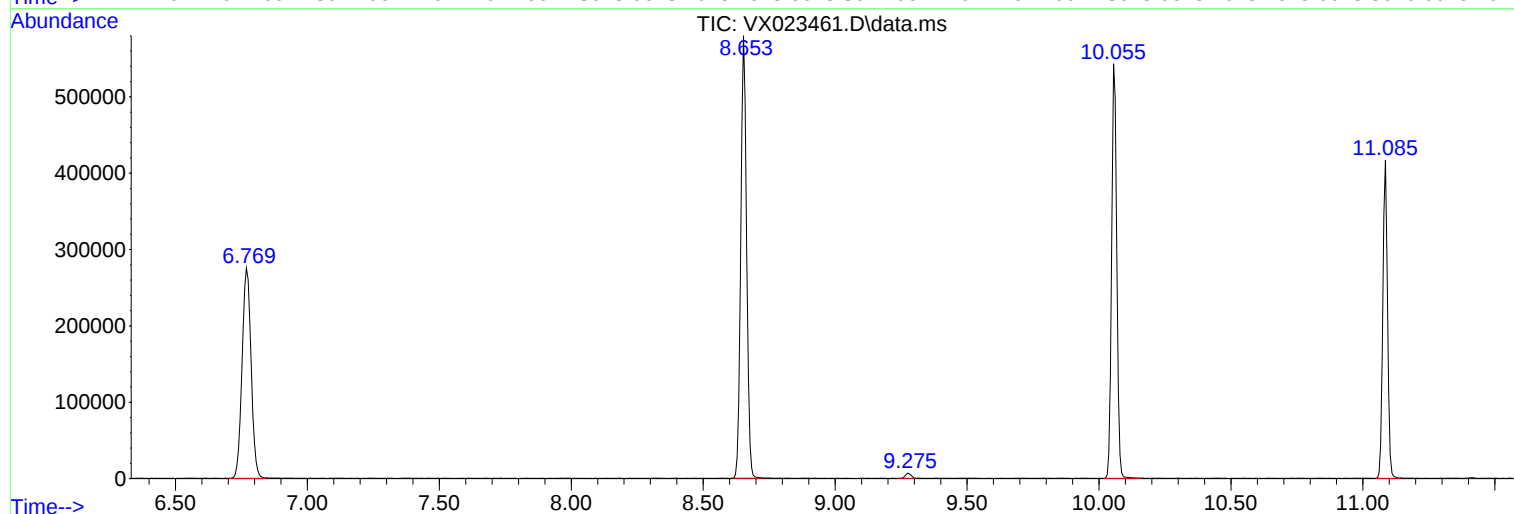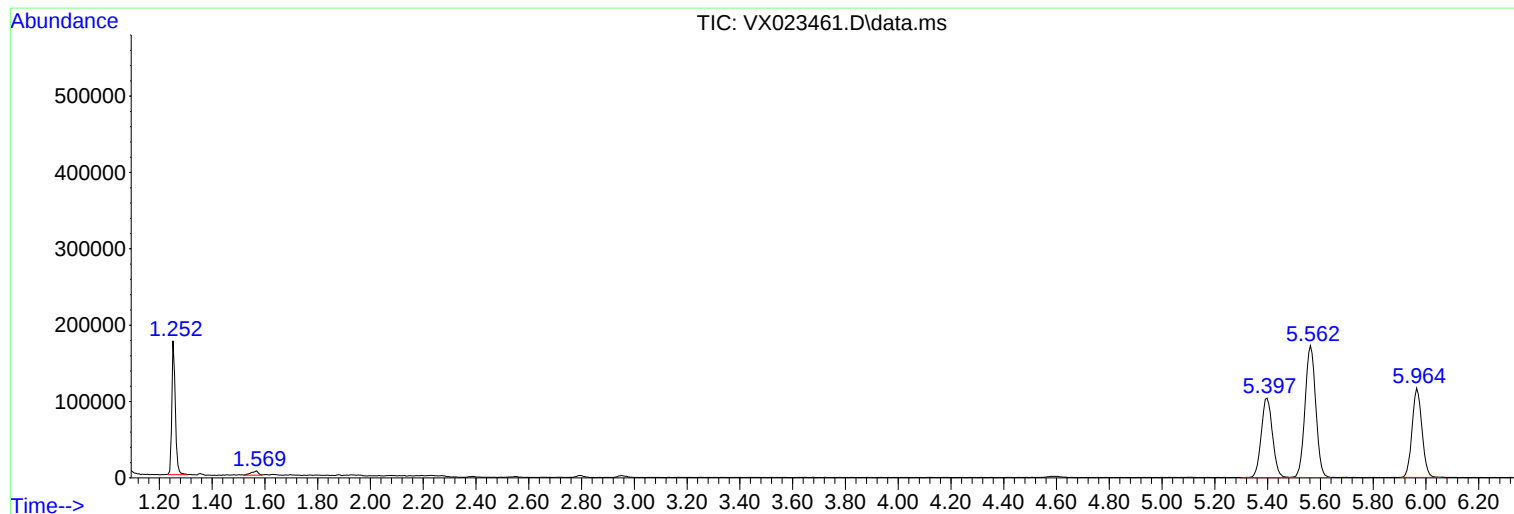

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023461.D
Acq On : 26 Jul 2021 19:10
Operator : JC/MD
Sample : M3146-15 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072621\
Data File : VX023461.D
Acq On : 26 Jul 2021 19:10
Operator : JC/MD
Sample : M3146-15 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------