

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072622\  
 Data File : VX030211.D  
 Acq On : 26 Jul 2022 15:40  
 Operator : JC/MD  
 Sample : N3876-05  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 EB-07-07192022

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030211.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.575       | 71            | 80          | 84           | rBV6     | 5476           | 13809         | 1.34%           | 0.290%        |
| 2         | 2.386       | 206           | 213         | 220          | rBV      | 11462          | 19630         | 1.91%           | 0.412%        |
| 3         | 2.544       | 235           | 239         | 246          | rVB2     | 6344           | 13166         | 1.28%           | 0.276%        |
| 4         | 5.391       | 691           | 706         | 719          | rBV      | 116155         | 340218        | 33.10%          | 7.144%        |
| 5         | 5.556       | 722           | 733         | 747          | rVV2     | 133366         | 378231        | 36.80%          | 7.943%        |
| 6         | 5.958       | 789           | 799         | 810          | rBV2     | 139936         | 374727        | 36.46%          | 7.869%        |
| 7         | 6.763       | 922           | 931         | 943          | rBV      | 217850         | 522121        | 50.80%          | 10.964%       |
| 8         | 8.653       | 1234          | 1241        | 1251         | rBV      | 656605         | 1027743       | 100.00%         | 21.582%       |
| 9         | 9.275       | 1338          | 1343        | 1349         | rVB3     | 10437          | 15801         | 1.54%           | 0.332%        |
| 10        | 9.525       | 1379          | 1384        | 1391         | rBV2     | 9928           | 15222         | 1.48%           | 0.320%        |
| 11        | 10.055      | 1464          | 1471        | 1487         | rBV      | 520647         | 673600        | 65.54%          | 14.145%       |
| 12        | 11.085      | 1634          | 1640        | 1647         | rBV      | 472924         | 614239        | 59.77%          | 12.899%       |
| 13        | 12.024      | 1788          | 1794        | 1802         | rBV      | 629874         | 753568        | 73.32%          | 15.824%       |




Sum of corrected areas: 4762075

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072622\  
Data File : VX030211.D  
Acq On : 26 Jul 2022 15:40  
Operator : JC/MD  
Sample : N3876-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-07-07192022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

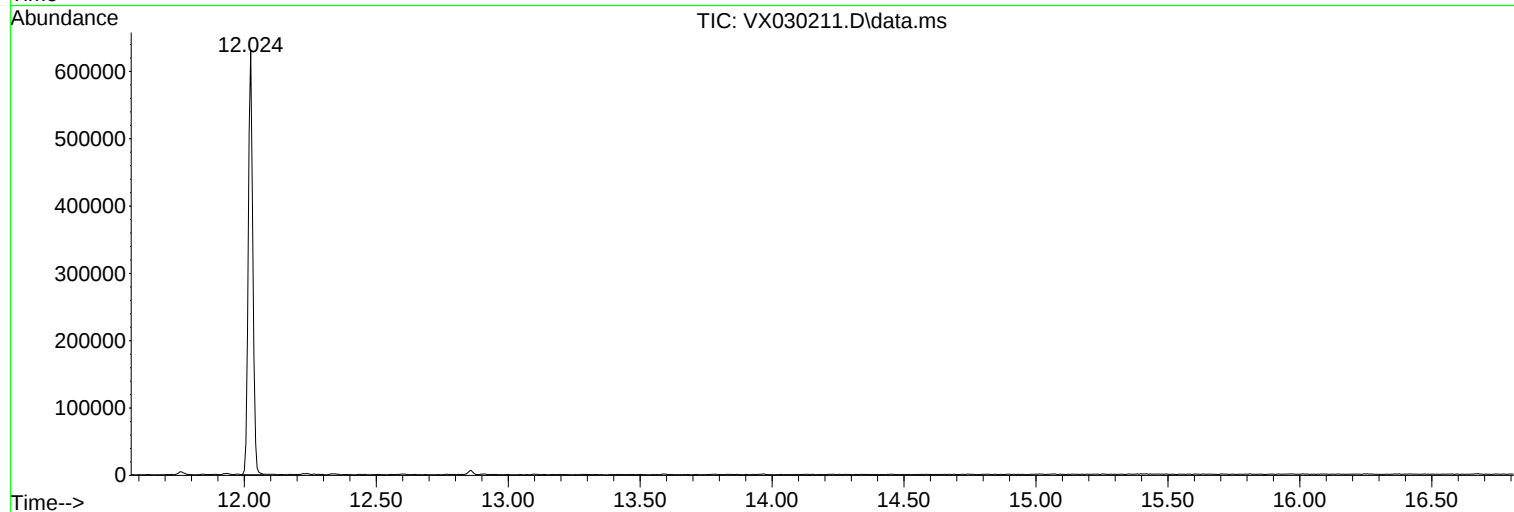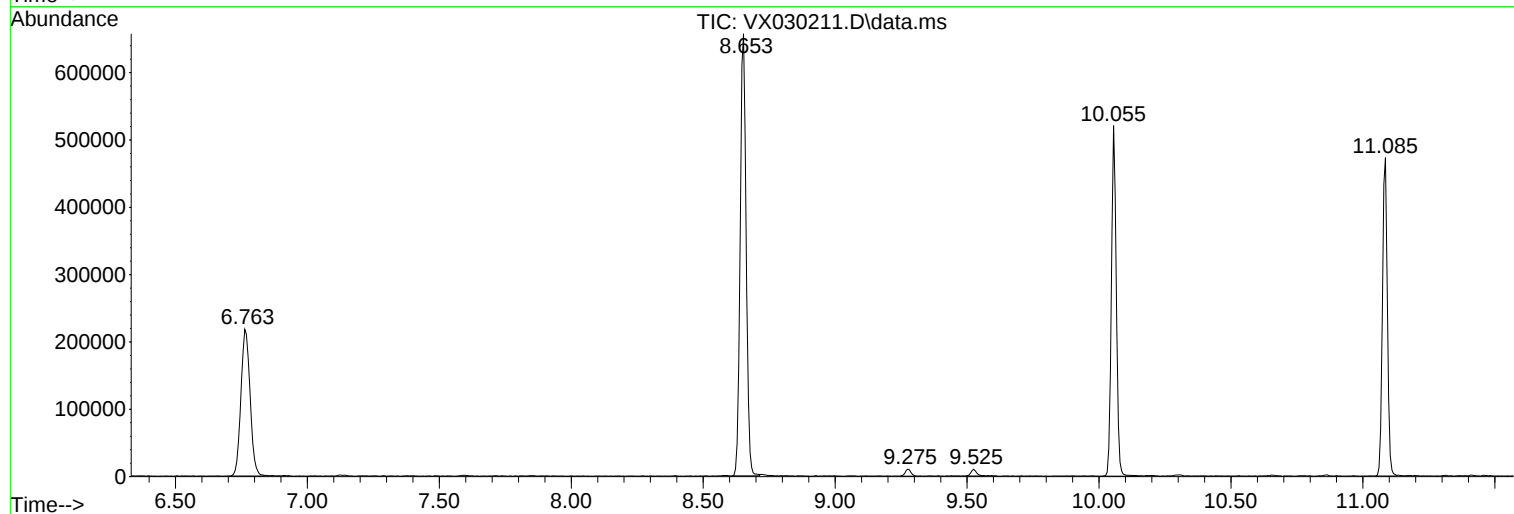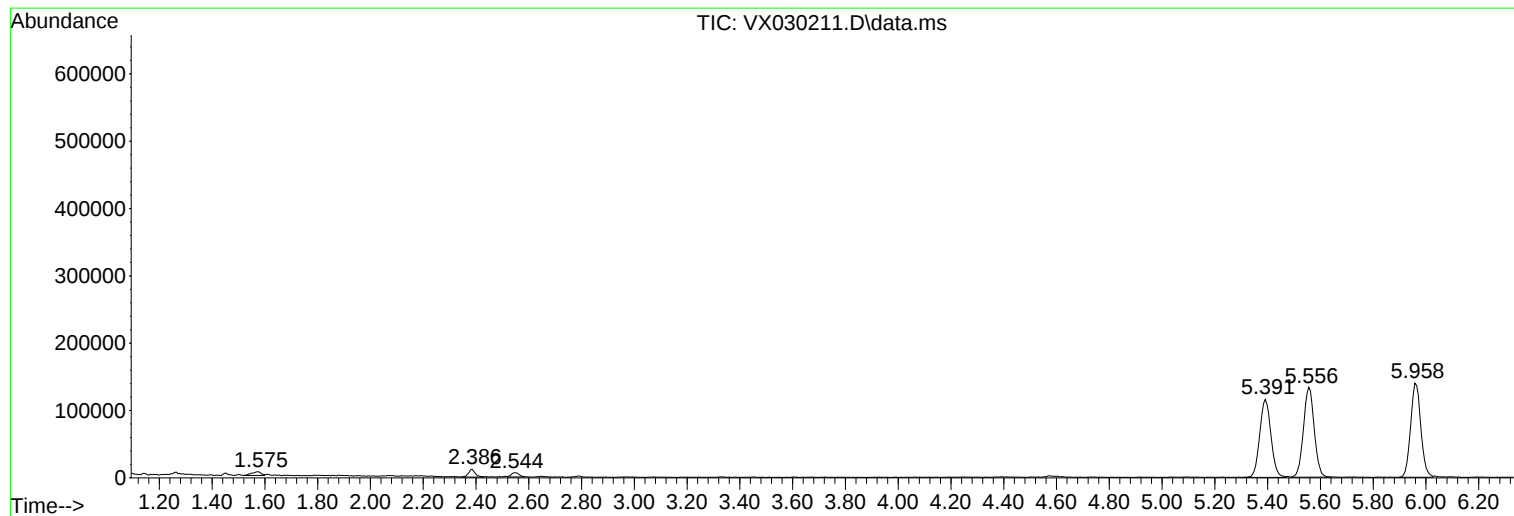

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072622\  
Data File : VX030211.D  
Acq On : 26 Jul 2022 15:40  
Operator : JC/MD  
Sample : N3876-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-07-07192022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072622\  
Data File : VX030211.D  
Acq On : 26 Jul 2022 15:40  
Operator : JC/MD  
Sample : N3876-05  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-07-07192022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|