

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072622\  
Data File : VX030213.D  
Acq On : 26 Jul 2022 16:26  
Operator : JC/MD  
Sample : N3876-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-08-07202022

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030213.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.385       | 207           | 213         | 223          | rVB      | 20528          | 35764         | 3.23%           | 0.707%        |
| 2         | 5.391       | 693           | 706         | 720          | rBV2     | 127143         | 369102        | 33.32%          | 7.300%        |
| 3         | 5.556       | 723           | 733         | 747          | rVB      | 138870         | 396509        | 35.79%          | 7.842%        |
| 4         | 5.958       | 789           | 799         | 814          | rBV      | 152352         | 410520        | 37.06%          | 8.119%        |
| 5         | 6.769       | 922           | 932         | 945          | rBV      | 226408         | 546835        | 49.36%          | 10.815%       |
| 6         | 8.653       | 1234          | 1241        | 1250         | rBV      | 724901         | 1107793       | 100.00%         | 21.910%       |
| 7         | 9.524       | 1380          | 1384        | 1391         | rBV3     | 8532           | 13056         | 1.18%           | 0.258%        |
| 8         | 10.055      | 1465          | 1471        | 1485         | rBV      | 533769         | 716928        | 64.72%          | 14.179%       |
| 9         | 11.085      | 1634          | 1640        | 1652         | rBV      | 517312         | 665605        | 60.08%          | 13.164%       |
| 10        | 12.024      | 1788          | 1794        | 1802         | rBV      | 643938         | 794002        | 71.67%          | 15.704%       |




Sum of corrected areas: 5056114

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072622\  
Data File : VX030213.D  
Acq On : 26 Jul 2022 16:26  
Operator : JC/MD  
Sample : N3876-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-08-072022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

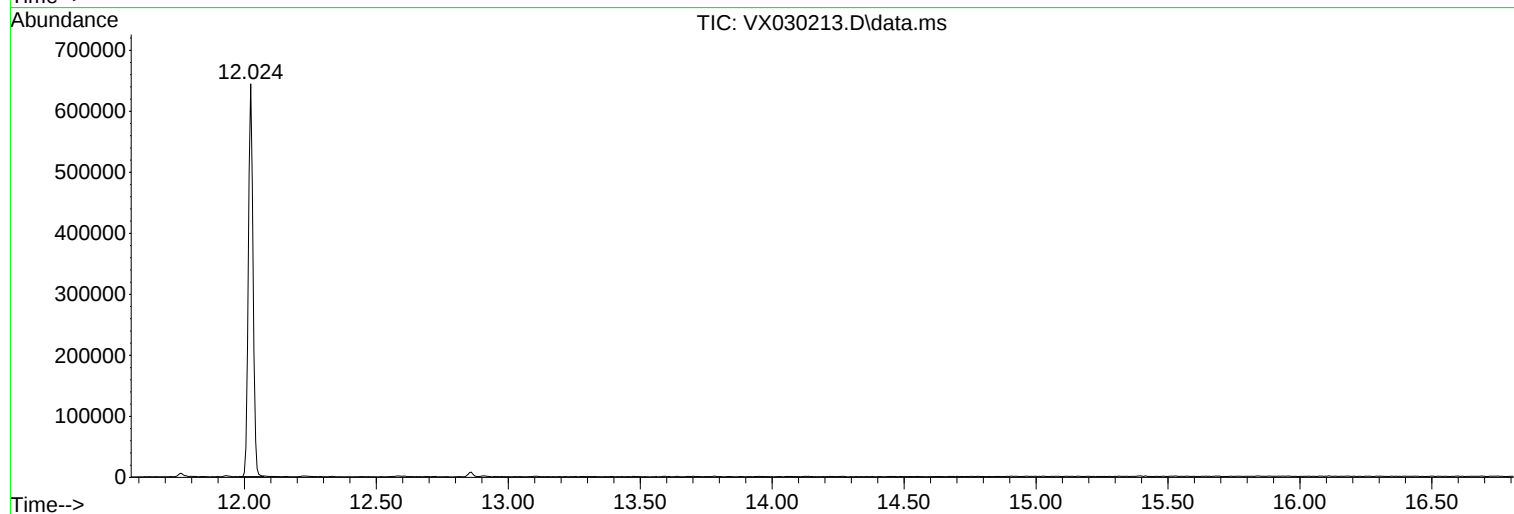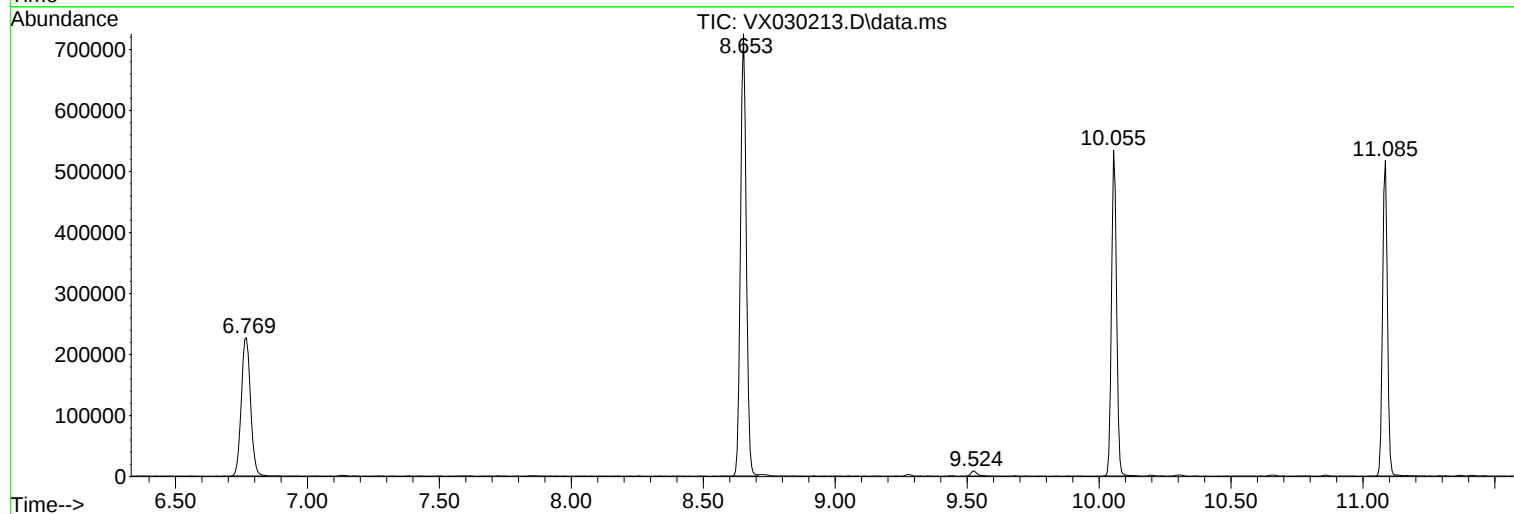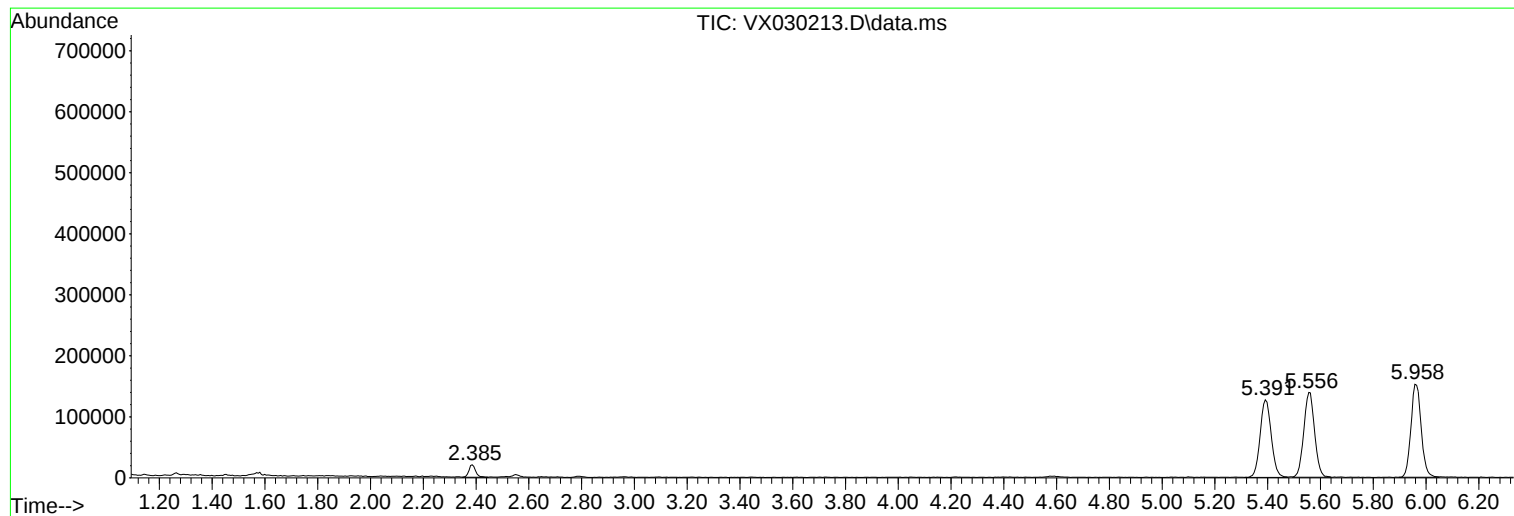

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072622\  
Data File : VX030213.D  
Acq On : 26 Jul 2022 16:26  
Operator : JC/MD  
Sample : N3876-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-08-07202022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX072622\  
Data File : VX030213.D  
Acq On : 26 Jul 2022 16:26  
Operator : JC/MD  
Sample : N3876-06  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
EB-08-07202022

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X072522W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|