

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072622\
 Data File : VX030218.D
 Acq On : 26 Jul 2022 18:24
 Operator : JC/MD
 Sample : N3876-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SPC-07-84

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
 Title : SW846 8260

Signal : TIC: VX030218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	16	rVB	44865	36757	3.70%	0.750%
2	1.264	27	29	35	rVB4	8671	10478	1.06%	0.214%
3	1.368	41	46	53	rVB3	12061	19248	1.94%	0.393%
4	2.544	229	239	246	rBV3	8416	16898	1.70%	0.345%
5	5.397	691	707	720	rBV2	112161	329294	33.18%	6.718%
6	5.556	723	733	746	rVV	143353	403832	40.69%	8.238%
7	5.964	789	800	812	rBV	133096	363854	36.67%	7.423%
8	6.769	922	932	944	rBV	233891	560463	56.48%	11.434%
9	7.129	985	991	1000	rBV6	5230	11695	1.18%	0.239%
10	8.653	1234	1241	1248	rBV	640126	992354	100.00%	20.245%
11	9.275	1338	1343	1349	rVB3	7317	10698	1.08%	0.218%
12	10.055	1465	1471	1484	rBV	541319	729721	73.53%	14.887%
13	11.086	1634	1640	1650	rBV	466548	597070	60.17%	12.181%
14	12.024	1789	1794	1803	rBV	668020	819413	82.57%	16.717%




Sum of corrected areas: 4901775

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072622\
Data File : VX030218.D
Acq On : 26 Jul 2022 18:24
Operator : JC/MD
Sample : N3876-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-07-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

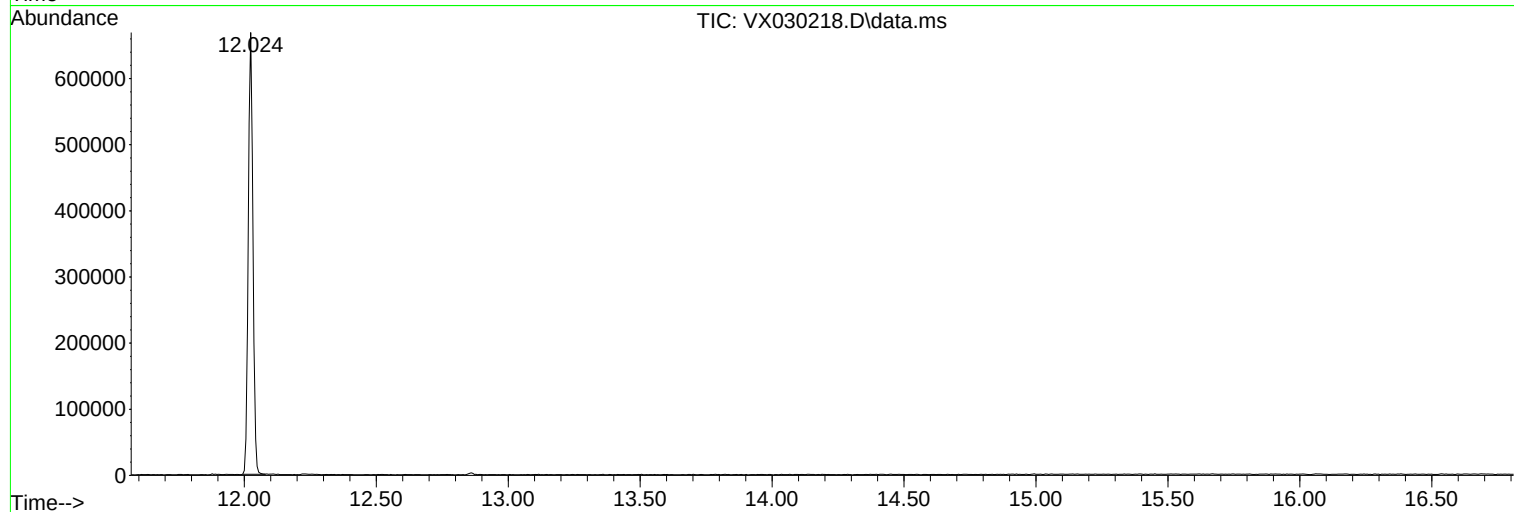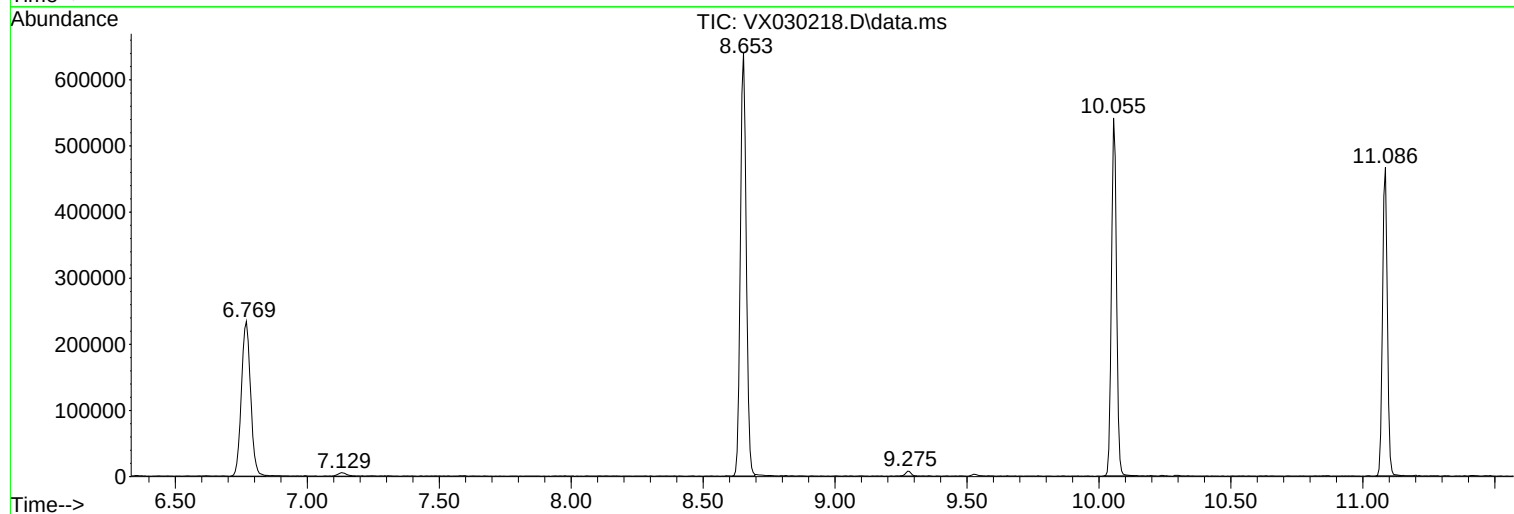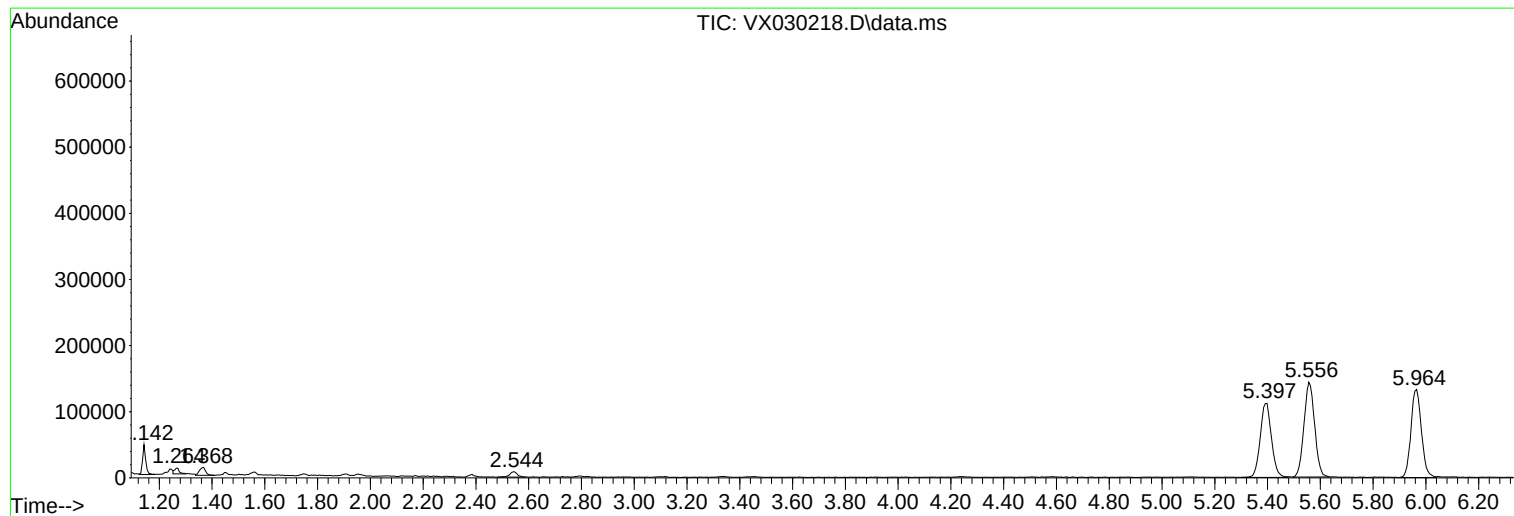

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072622\
Data File : VX030218.D
Acq On : 26 Jul 2022 18:24
Operator : JC/MD
Sample : N3876-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-07-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072622\
Data File : VX030218.D
Acq On : 26 Jul 2022 18:24
Operator : JC/MD
Sample : N3876-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-07-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------