


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072718\
Data File : VX003712.D
Acq On : 27 Jul 2018 12:56
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X072718W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Jul 27 16:17:43 2018

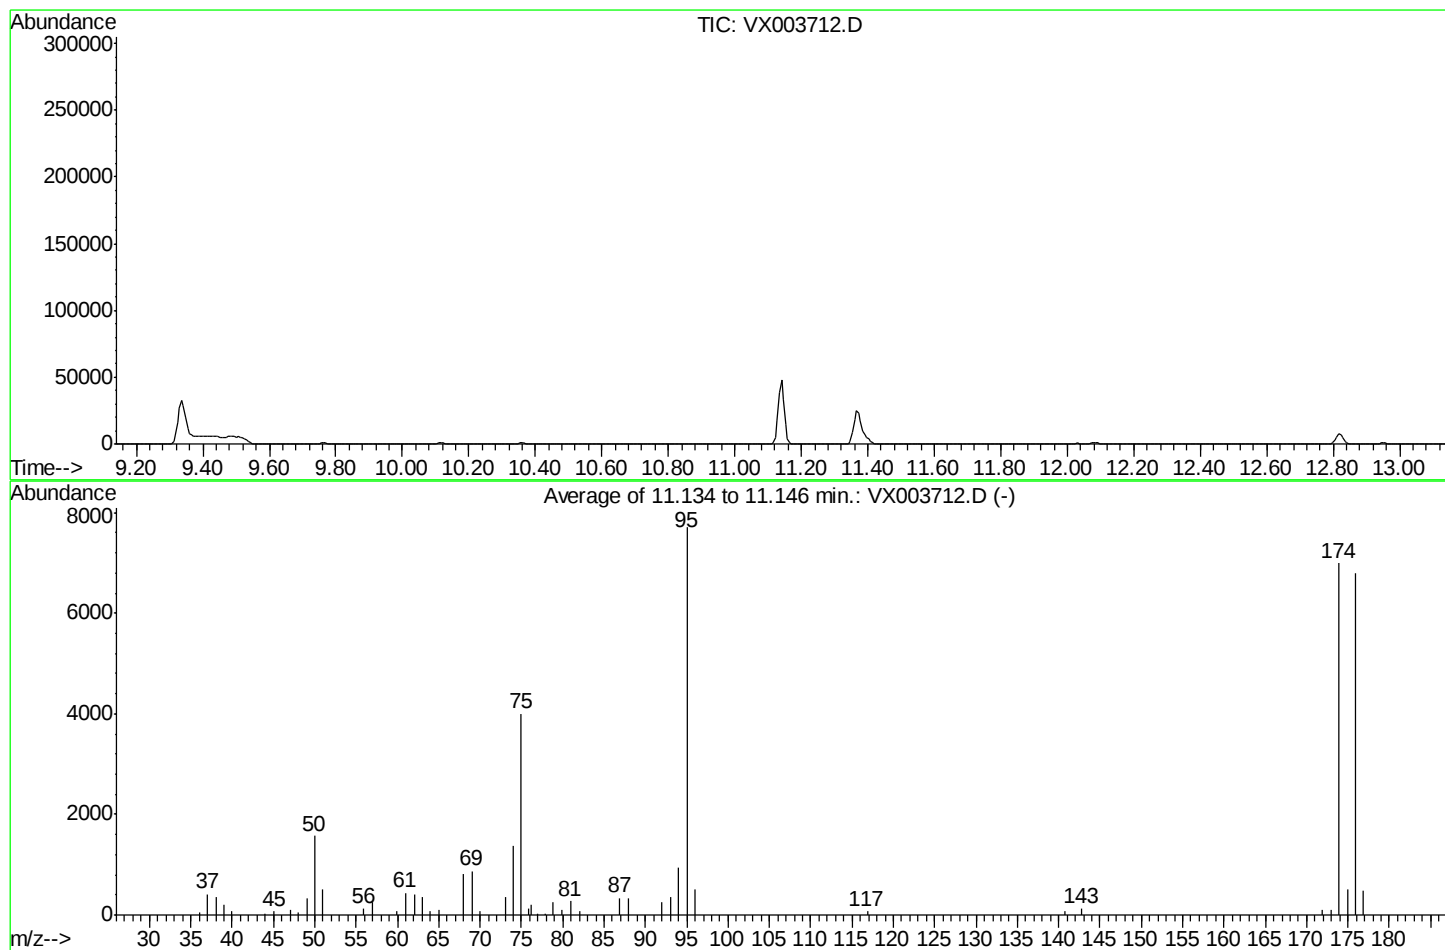

AutoFind: Scans 1730, 1731, 1732; Background Corrected with Scan 1725

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	1566	PASS
75	95	30	60	51.9	4003	PASS
95	95	100	100	100.0	7707	PASS
96	95	5	9	6.8	521	PASS
173	174	0.00	2	1.3	91	PASS
174	95	50	100	90.7	6988	PASS
175	174	5	9	7.2	500	PASS
176	174	95	101	97.2	6794	PASS
177	176	5	9	7.3	495	PASS