

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX072720\
 Data File : VX017615.D
 Acq On : 27 Jul 2020 14:05
 Operator : JC/SP
 Sample : L3450-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TT-016-IDWGW-20200723

Quant Time: Aug 06 03:33:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X072720W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Mon Jul 27 11:38:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	4.98	128	117817	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.84	114	579079	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.10	117	552302	30.00	ug/l	0.00

System Monitoring Compounds

27) 1,2-Dichloroethane-d4	6.03	65	265477	29.32	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	97.73%
60) 4-Bromofluorobenzene	11.12	95	272020	29.08	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	96.93%
63) Toluene-d8	8.70	98	735022	30.07	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	100.23%


Target Compounds					Qvalue
37) Trichloroethene	7.19	130	101963	14.270 ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX072720\
Data File : VX017615.D
Acq On : 27 Jul 2020 14:05
Operator : JC/SP
Sample : L3450-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TT-016-IDW/GW-20200723

Quant Time: Aug 06 03:33:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\624X072720W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Mon Jul 27 11:38:31 2020
Response via : Initial Calibration

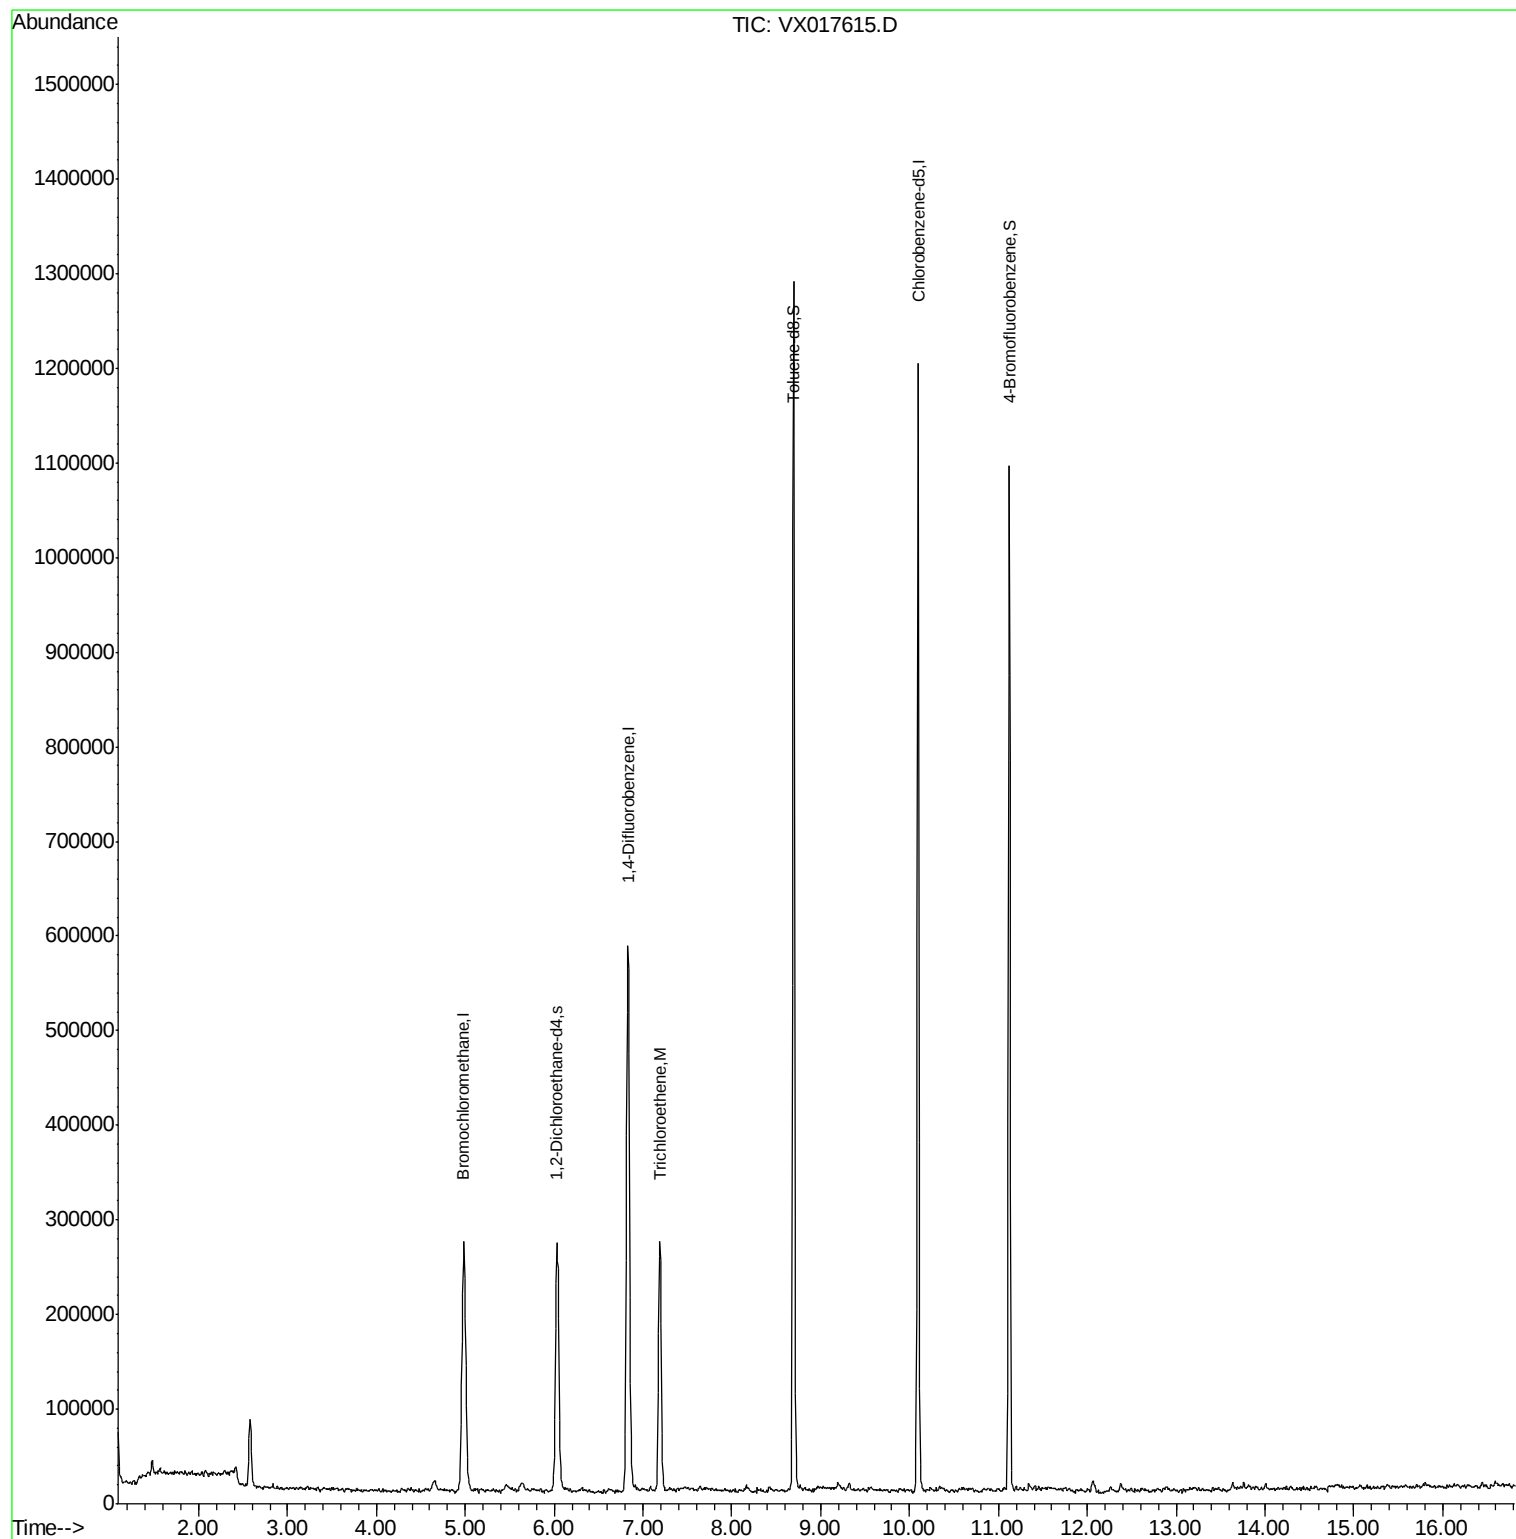

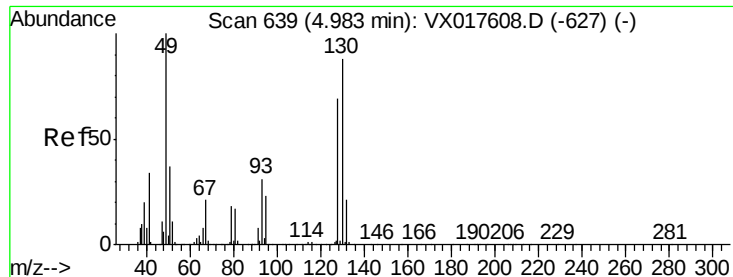

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 4.98 min Scan# 639

Delta R.T. -0.00 min

Lab File: VX017615.D

Acq: 27 Jul 2020 14:05





Instrument :

MSVOA_X

ClientSampleId :

TT-016-IDW/GW-20200723

Tgt Ion:	128	Resp:	117817
Ion	Ratio	Lower	Upper
128	100		
49	152.5	0.0	376.0
130	129.4	0.0	323.0

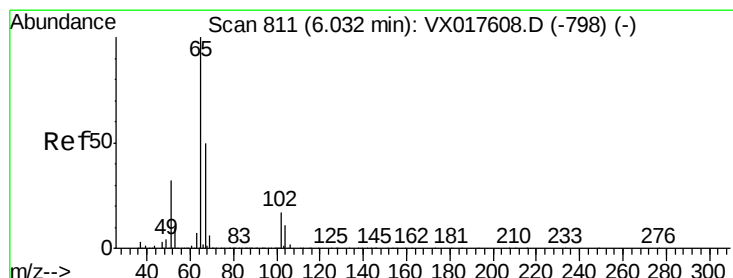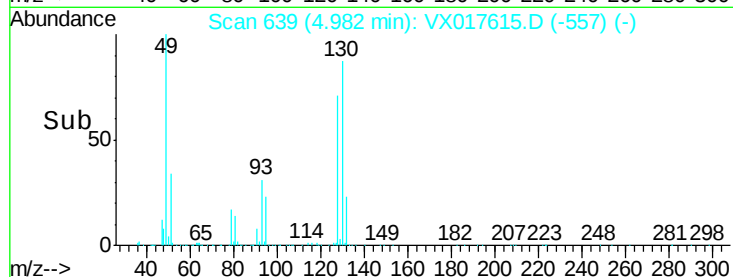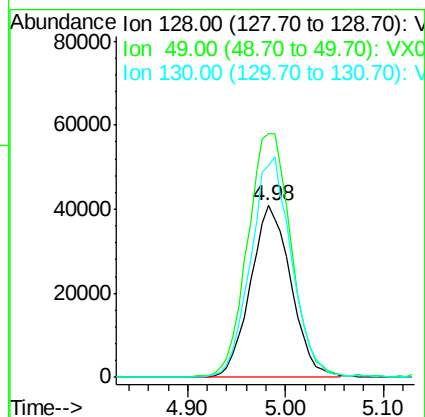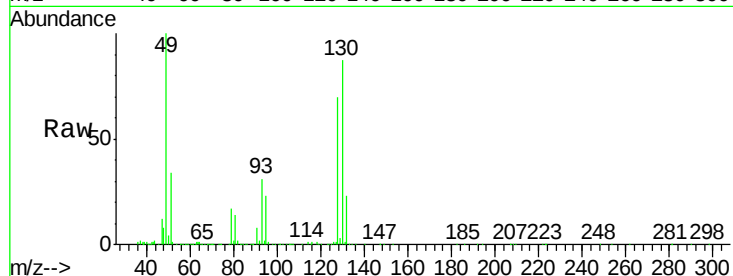

#27

1,2-Dichloroethane-d4

Concen: 29.323 ug/l




RT: 6.03 min Scan# 811


Delta R.T. -0.00 min

Lab File: VX017615.D

Acq: 27 Jul 2020 14:05

Tgt Ion:	65	Resp:	265477
Ion	Ratio	Lower	Upper
65	100		
67	50.4	40.6	61.0

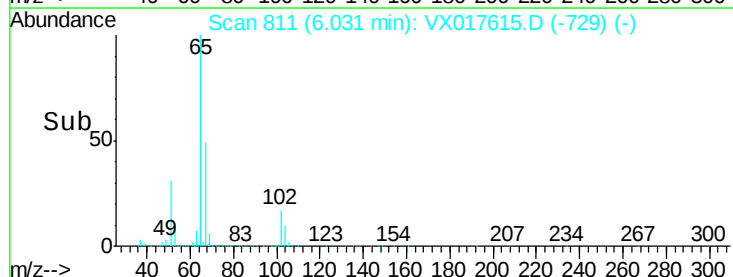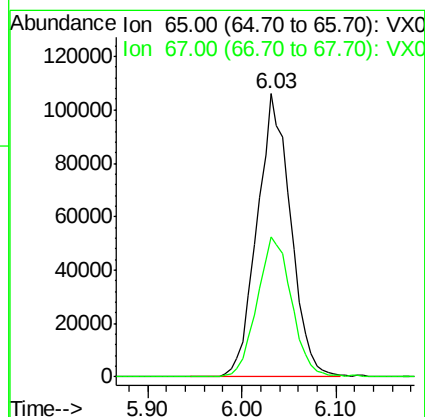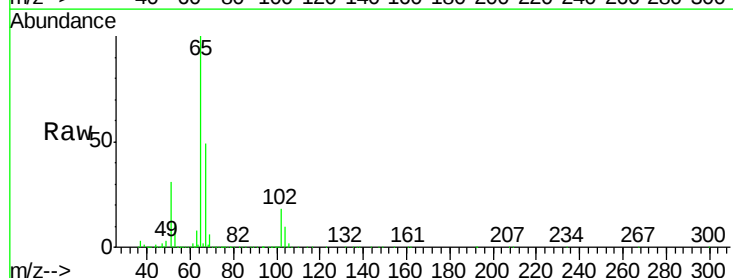

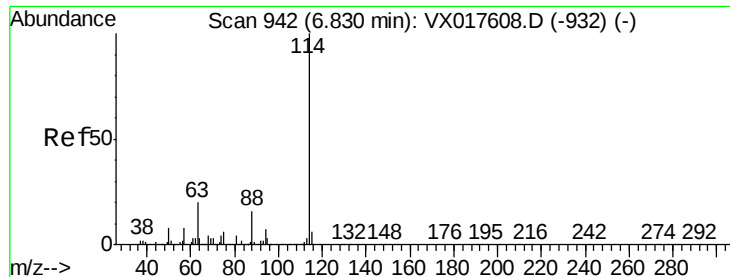

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 6.84 min Scan# 943

Delta R.T. 0.01 min

Lab File: VX017615.D

Acq: 27 Jul 2020 14:05

Instrument :

MSVOA_X

ClientSampleId :

TT-016-IDW/GW-20200723


Tgt Ion:114 Resp: 579079

Ion Ratio Lower Upper

114 100

63 20.7 16.3 24.5




88 16.1 12.6 18.8

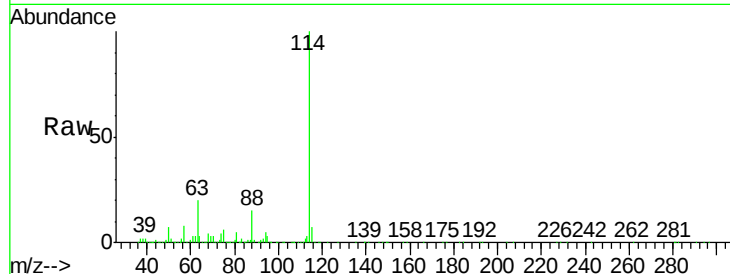

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 88.00 (87.70 to 88.70): VX0

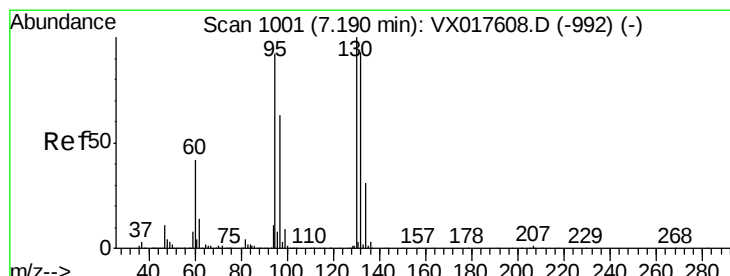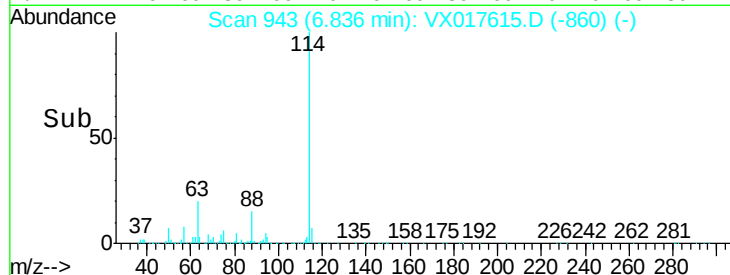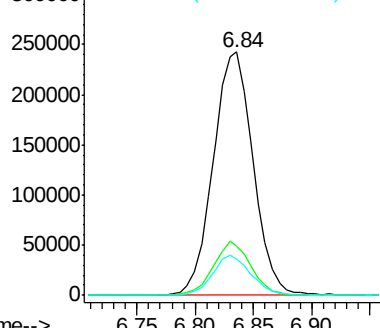

#37

Trichloroethene

Concen: 14.270 ug/l

RT: 7.19 min Scan# 1001

Delta R.T. -0.00 min

Lab File: VX017615.D


Acq: 27 Jul 2020 14:05

Tgt Ion:130 Resp: 101963

Ion Ratio Lower Upper



130 100


95 90.2 73.9 110.9

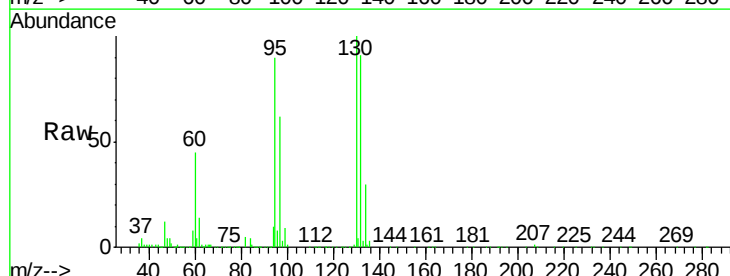

Abundance Ion 129.90 (129.60 to 130.60): V

Ion 94.90 (94.60 to 95.60): VX0



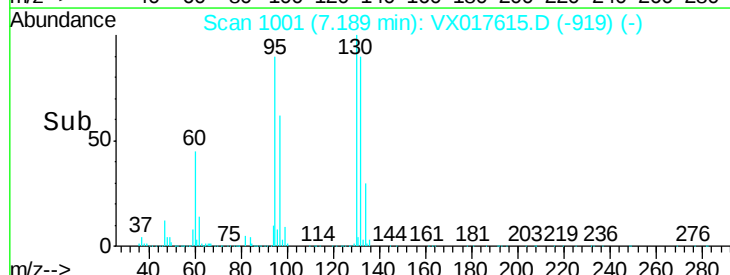
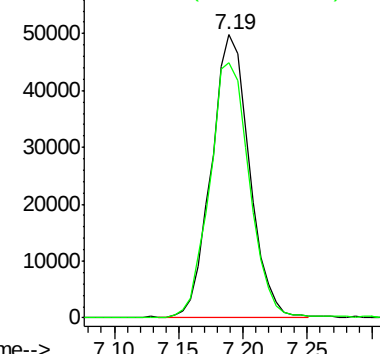


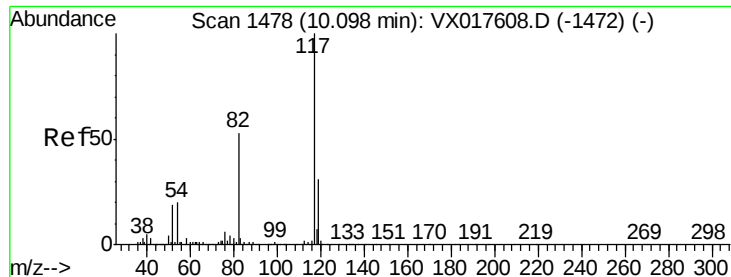

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX017615.D
Acq: 27 Jul 2020 14:05




Instrument :
MSVOA_X
ClientSampleId :
TT-016-IDW/GW-20200723


Tgt Ion: 117 Resp: 552302
Ion Ratio Lower Upper
117 100
82 54.2 43.6 65.4
119 31.4 25.7 38.5

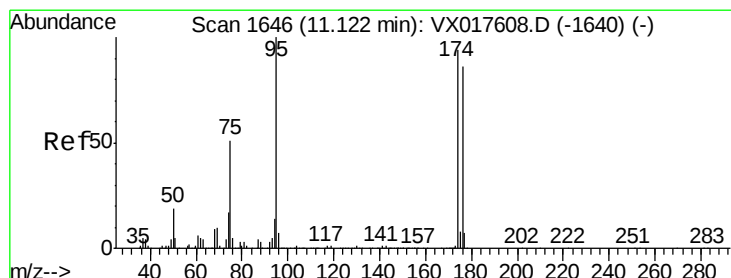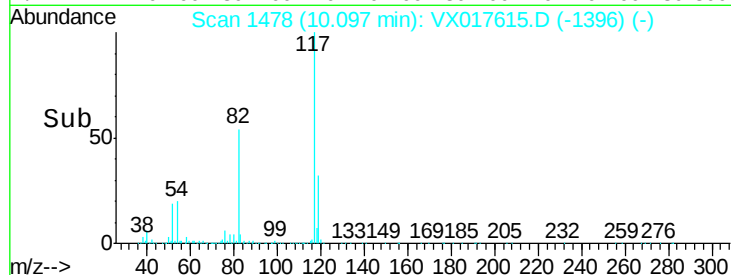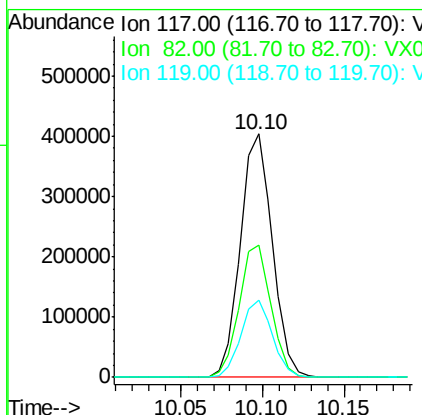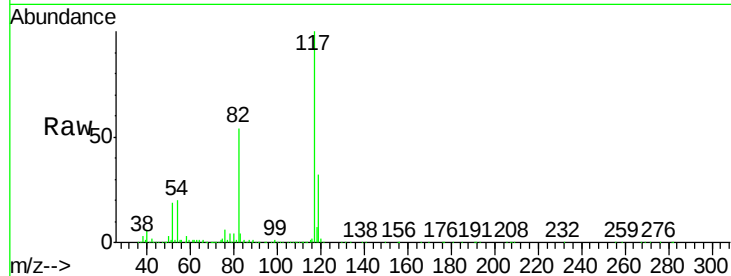

#60
4-Bromofluorobenzene
Concen: 29.083 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX017615.D
Acq: 27 Jul 2020 14:05

Tgt Ion: 95 Resp: 272020
Ion Ratio Lower Upper
95 100
174 84.6 70.2 105.2
176 80.9 65.6 98.4

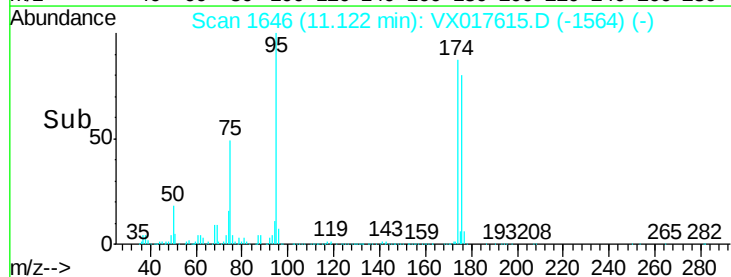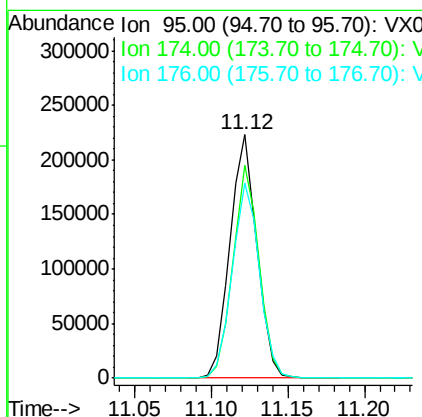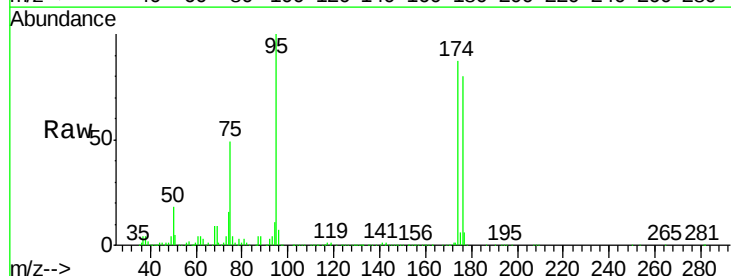

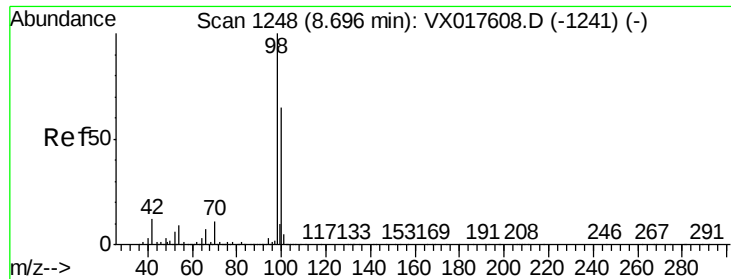

#63

Toluene-d8

Concen: 30.074 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX017615.D

Acq: 27 Jul 2020 14:05

Instrument :

MSVOA_X

ClientSampleId :

TT-016-IDW/GW-20200723

Tgt Ion: 98 Resp: 735022

Ion Ratio Lower Upper

98 100

100 65.0 51.9 77.9

