


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX072720\
Data File : VX017606.D
Acq On : 27 Jul 2020 08:54
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Title : SW846 8260
Last Update : Fri Jul 24 05:48:09 2020

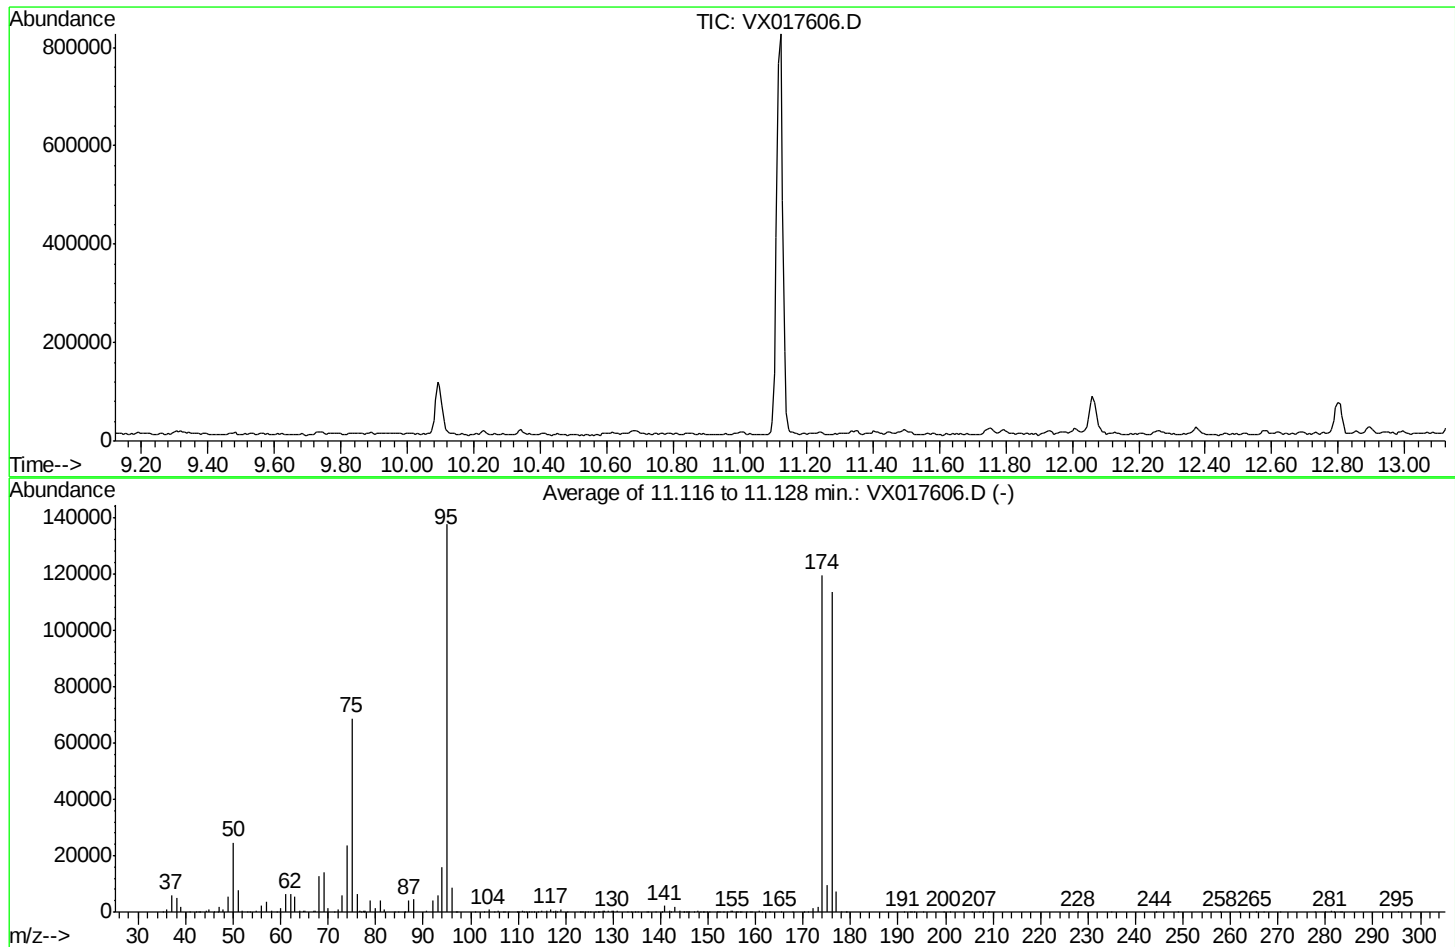

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	24638	PASS
75	95	30	60	50.0	68705	PASS
95	95	100	100	100.0	137544	PASS
96	95	5	9	6.4	8776	PASS
173	174	0.00	2	1.5	1761	PASS
174	95	50	100	86.8	119453	PASS
175	174	5	9	8.0	9550	PASS
176	174	95	101	95.1	113549	PASS
177	176	5	9	6.3	7191	PASS