


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX072720\
Data File : VX017622.D
Acq On : 27 Jul 2020 16:44
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X072320W.M
Title : SW846 8260
Last Update : Fri Jul 24 05:48:09 2020

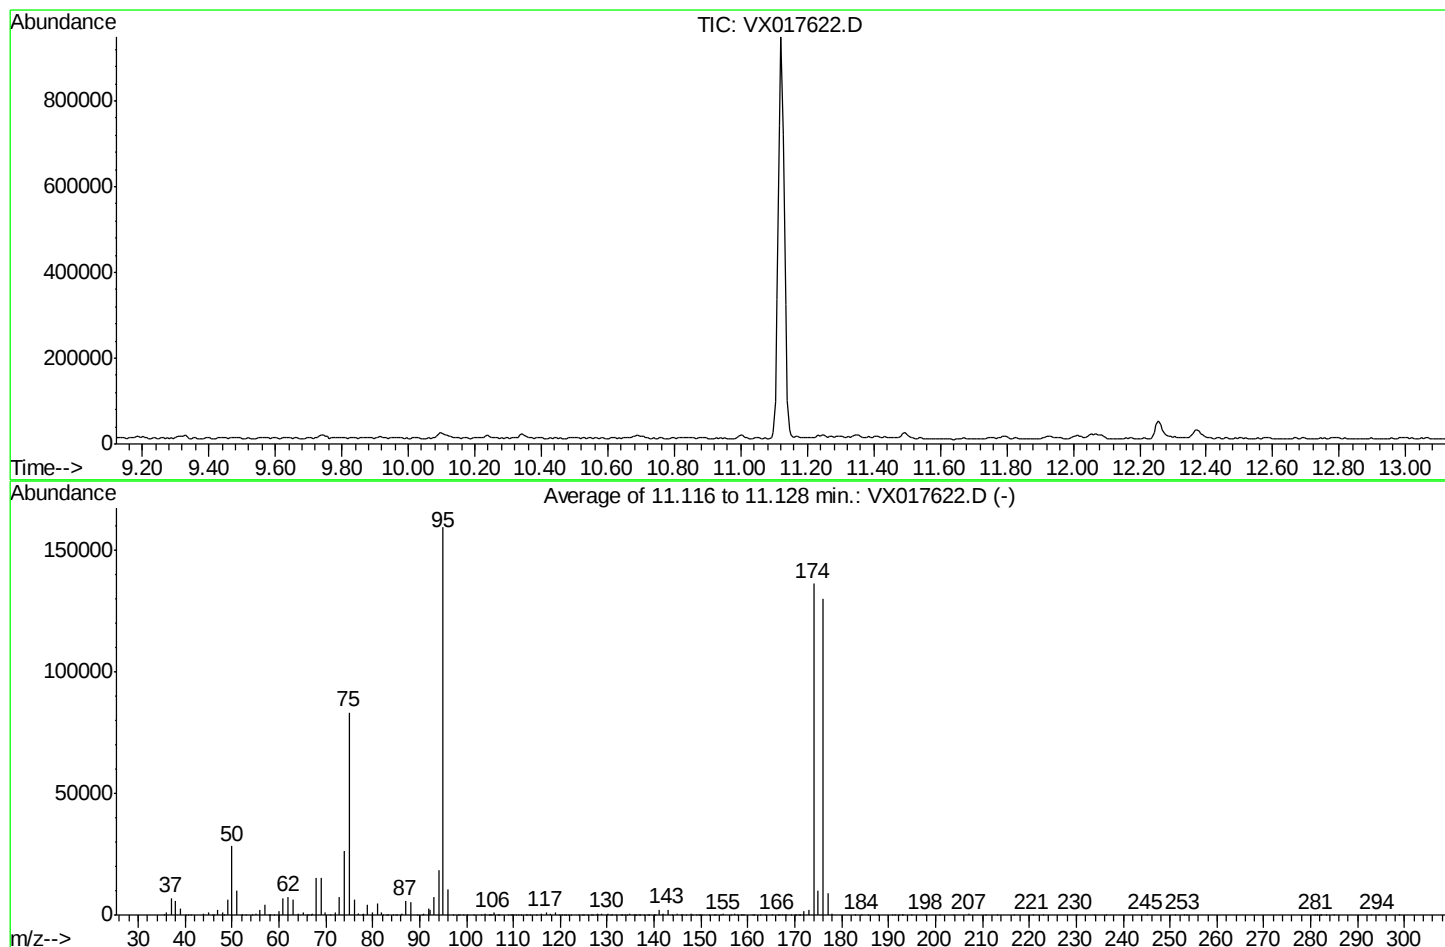

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	28423	PASS
75	95	30	60	52.3	83463	PASS
95	95	100	100	100.0	159445	PASS
96	95	5	9	6.7	10718	PASS
173	174	0.00	2	1.5	2011	PASS
174	95	50	100	85.5	136352	PASS
175	174	5	9	7.4	10035	PASS
176	174	95	101	95.6	130306	PASS
177	176	5	9	7.0	9155	PASS