

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
 Data File : VX023471.D
 Acq On : 27 Jul 2021 12:52
 Operator : JC/MD
 Sample : M3146-21 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-4-PD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.252	24	27	32	rBV	113595	99714	10.83%	2.091%
2	1.569	71	79	81	rBV4	6098	10129	1.10%	0.212%
3	5.397	695	707	722	rBV2	106237	310343	33.70%	6.507%
4	5.562	722	734	746	rVV	179998	504320	54.76%	10.574%
5	5.964	789	800	814	rBV	118389	313332	34.02%	6.569%
6	6.769	922	932	949	rBV	290103	677288	73.54%	14.200%
7	8.653	1234	1241	1250	rBV	601109	921016	100.00%	19.310%
8	10.055	1465	1471	1483	rBV	563003	774106	84.05%	16.230%
9	11.085	1634	1640	1651	rBV	431507	546417	59.33%	11.456%
10	12.024	1788	1794	1802	rBV	501175	612894	66.55%	12.850%




Sum of corrected areas: 4769559

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023471.D
Acq On : 27 Jul 2021 12:52
Operator : JC/MD
Sample : M3146-21 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

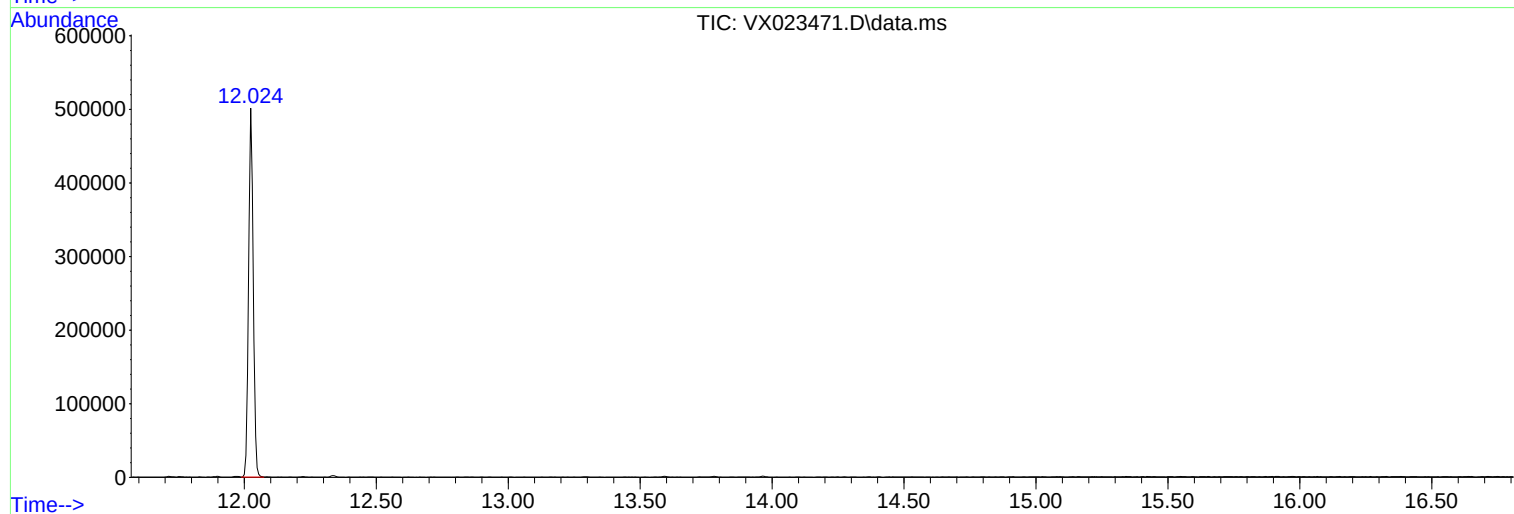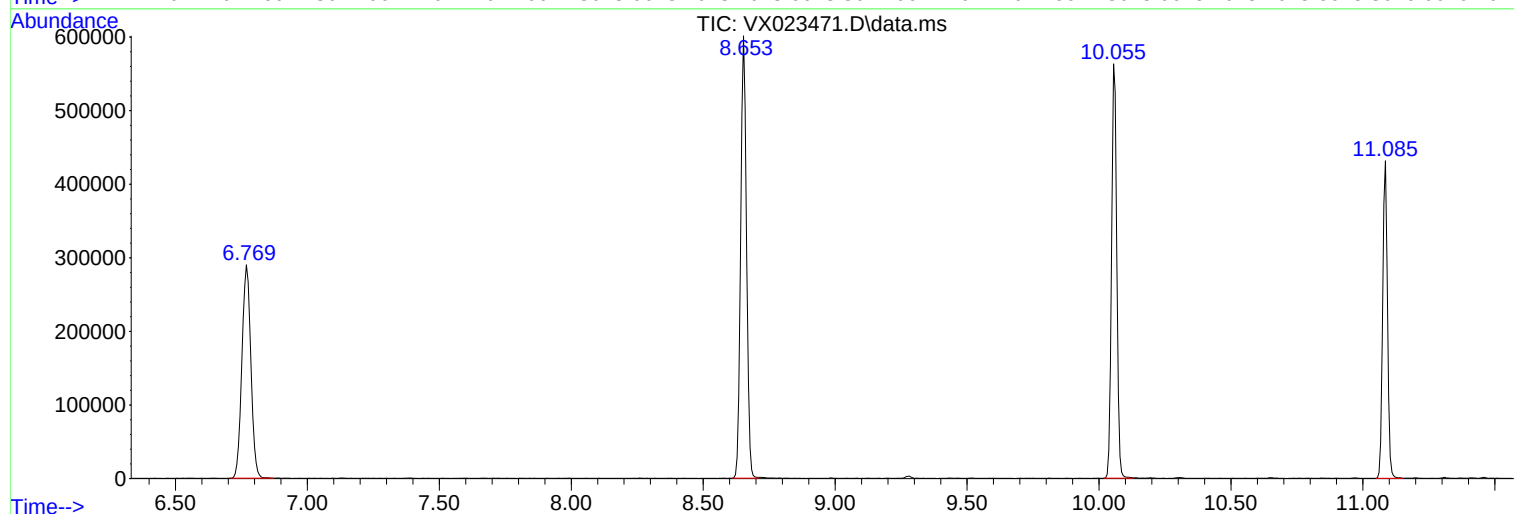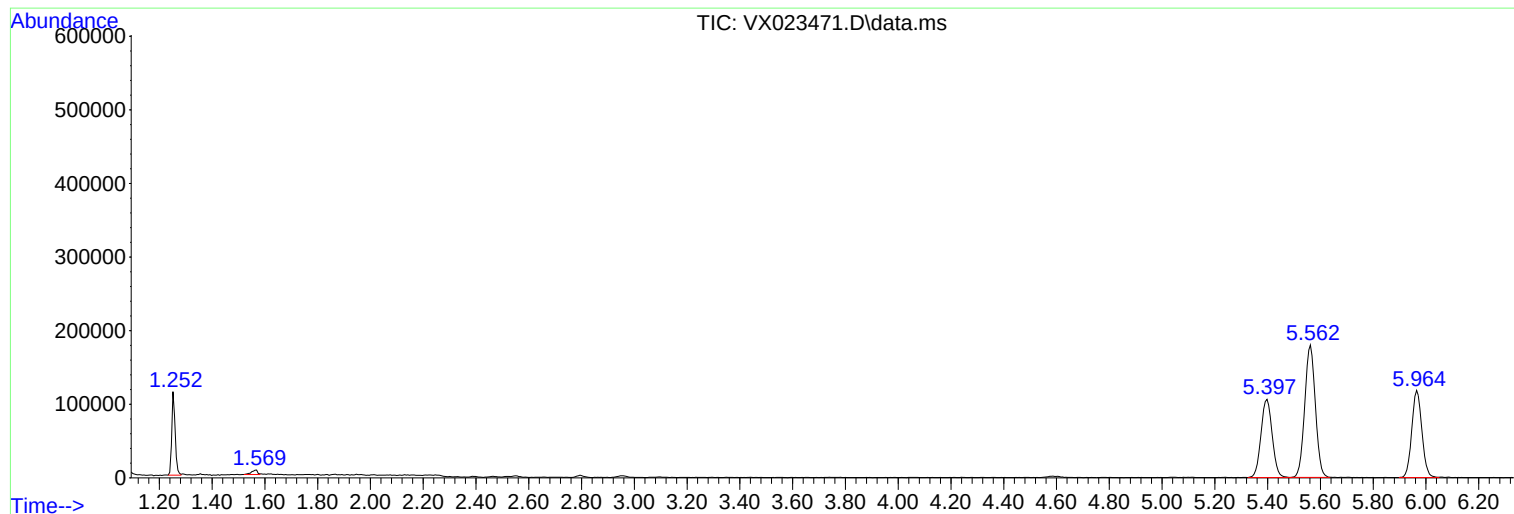

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023471.D
Acq On : 27 Jul 2021 12:52
Operator : JC/MD
Sample : M3146-21 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023471.D
Acq On : 27 Jul 2021 12:52
Operator : JC/MD
Sample : M3146-21 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
