

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
 Data File : VX023474.D
 Acq On : 27 Jul 2021 14:02
 Operator : JC/MD
 Sample : M3146-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-6-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023474.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.569	72	79	84	rVB3	5809	10984	1.27%	0.248%
2	2.550	233	240	246	rVB	5436	9741	1.12%	0.220%
3	4.501	550	560	571	rBV2	16221	43624	5.03%	0.986%
4	5.398	694	707	719	rBV	101779	289115	33.32%	6.534%
5	5.562	721	734	749	rVB2	169915	472112	54.40%	10.669%
6	5.964	790	800	814	rBV2	111304	289105	33.31%	6.533%
7	6.769	920	932	942	rBV	270518	628309	72.40%	14.199%
8	8.653	1234	1241	1250	rBV	569368	867822	100.00%	19.611%
9	10.055	1465	1471	1482	rBV	542391	733934	84.57%	16.586%
10	11.086	1634	1640	1649	rBV	418939	518399	59.74%	11.715%
11	12.024	1789	1794	1801	rBV	455592	561968	64.76%	12.700%


Sum of corrected areas: 4425113

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023474.D
Acq On : 27 Jul 2021 14:02
Operator : JC/MD
Sample : M3146-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

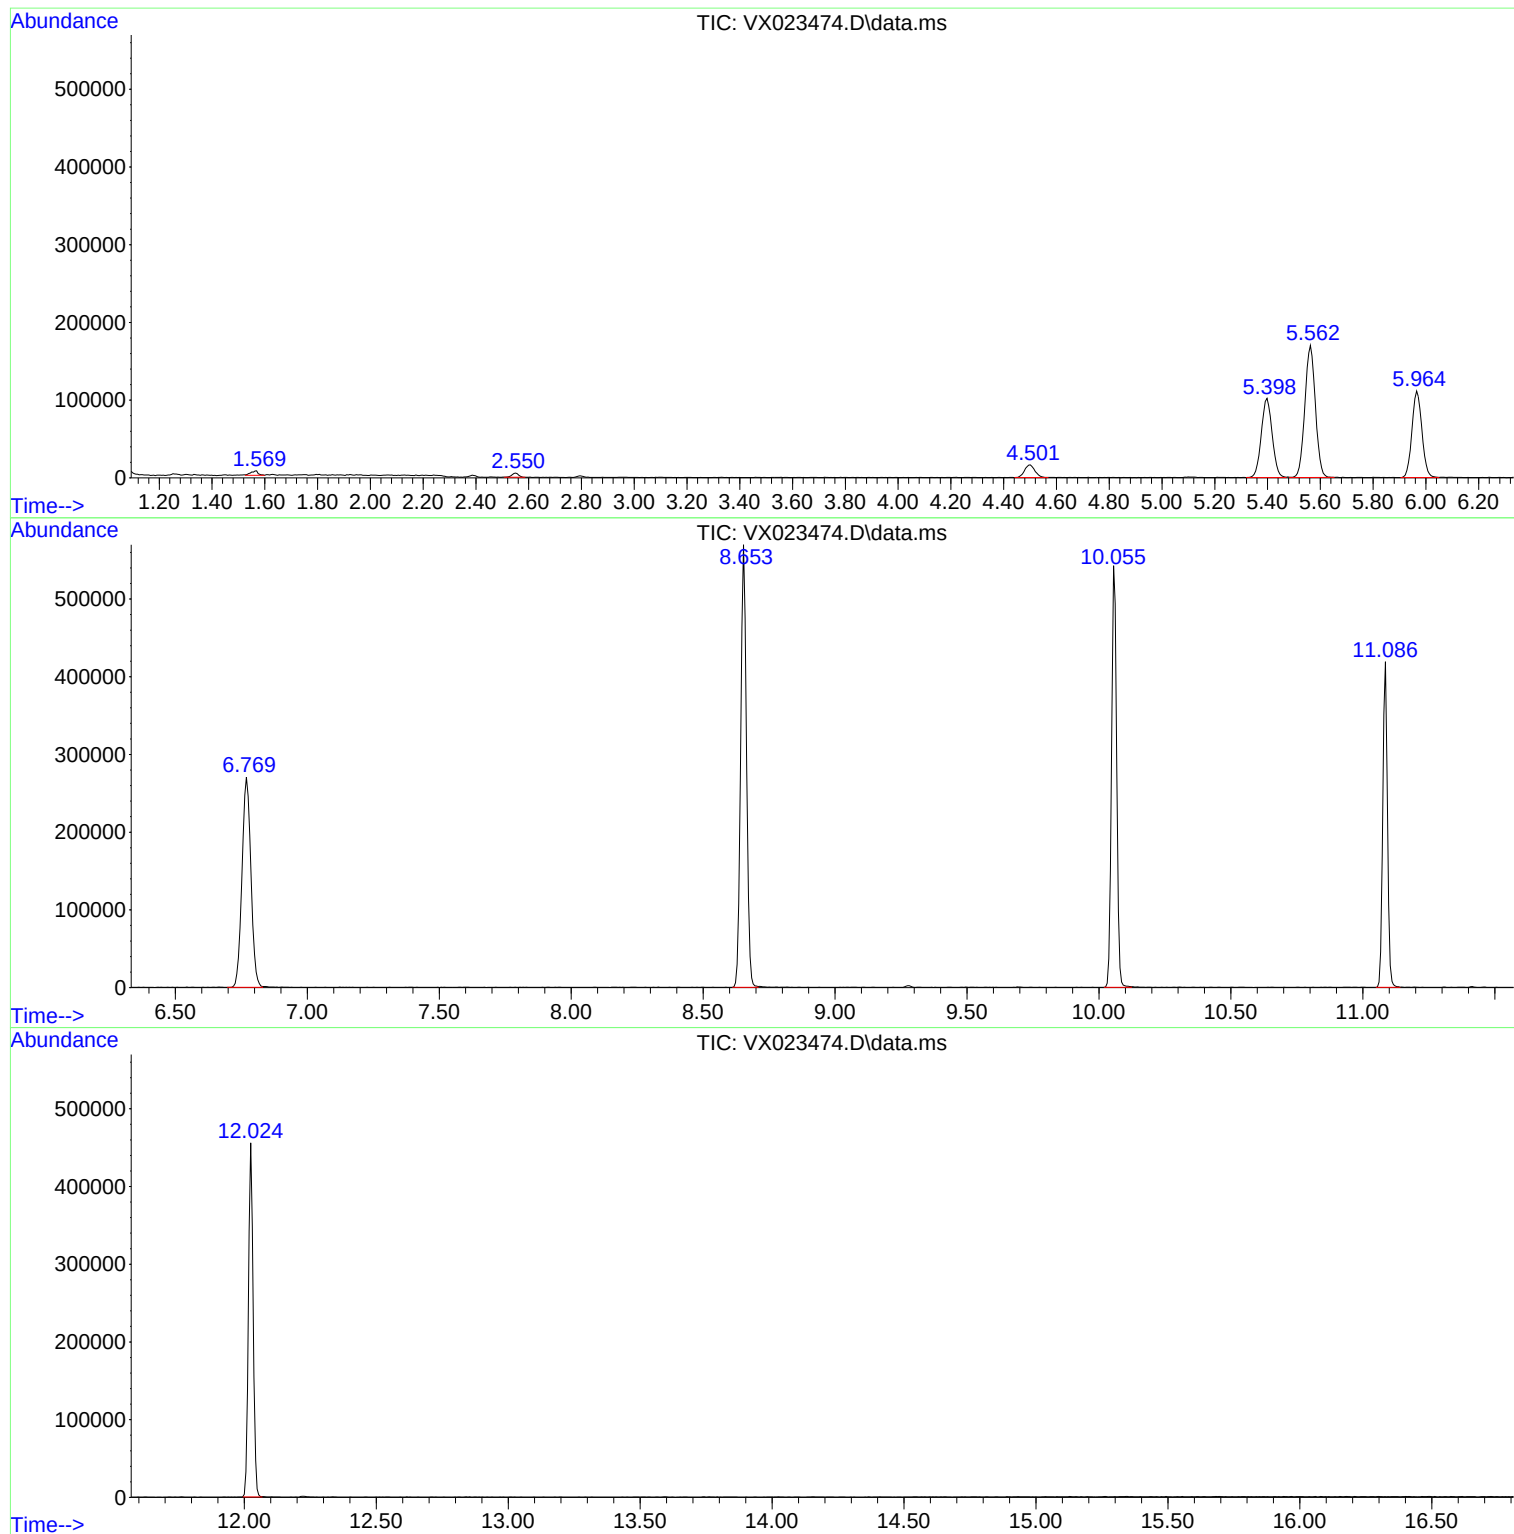

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023474.D
Acq On : 27 Jul 2021 14:02
Operator : JC/MD
Sample : M3146-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023474.D
Acq On : 27 Jul 2021 14:02
Operator : JC/MD
Sample : M3146-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-6-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------