

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
 Data File : VX023475.D
 Acq On : 27 Jul 2021 14:26
 Operator : JC/MD
 Sample : M3146-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-9-PD

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023475.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	70	78	84	rBV	6033	11993	1.35%	0.267%
2	2.386	206	213	220	rVB	5247	9644	1.08%	0.214%
3	2.550	231	240	248	rBV	7923	15447	1.74%	0.343%
4	5.397	694	707	719	rBV	102910	296348	33.30%	6.586%
5	5.562	722	734	749	rVB	173955	483350	54.31%	10.743%
6	5.964	787	800	819	rBV	113957	300877	33.81%	6.687%
7	6.769	921	932	950	rBV	279205	655711	73.68%	14.573%
8	8.653	1234	1241	1252	rBV	574663	889915	100.00%	19.779%
9	10.055	1465	1471	1479	rBV	547803	747437	83.99%	16.612%
10	11.085	1634	1640	1651	rBV	418693	518875	58.31%	11.532%
11	12.024	1789	1794	1803	rVB	472788	569744	64.02%	12.663%




Sum of corrected areas: 4499341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023475.D
Acq On : 27 Jul 2021 14:26
Operator : JC/MD
Sample : M3146-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-9-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

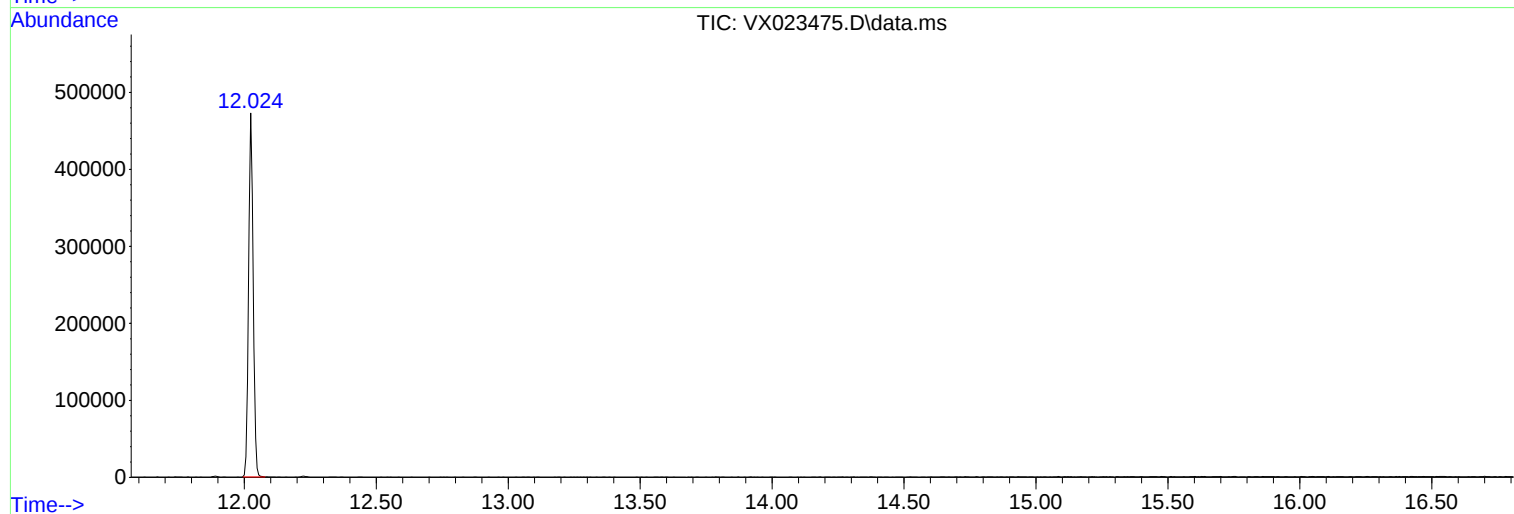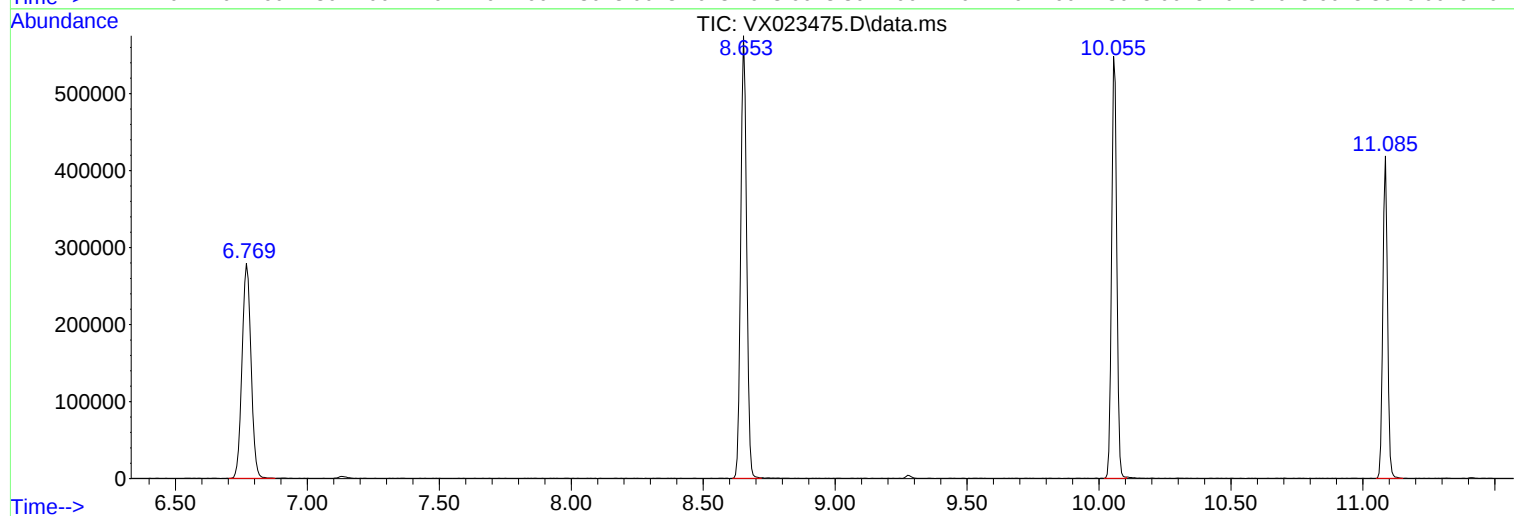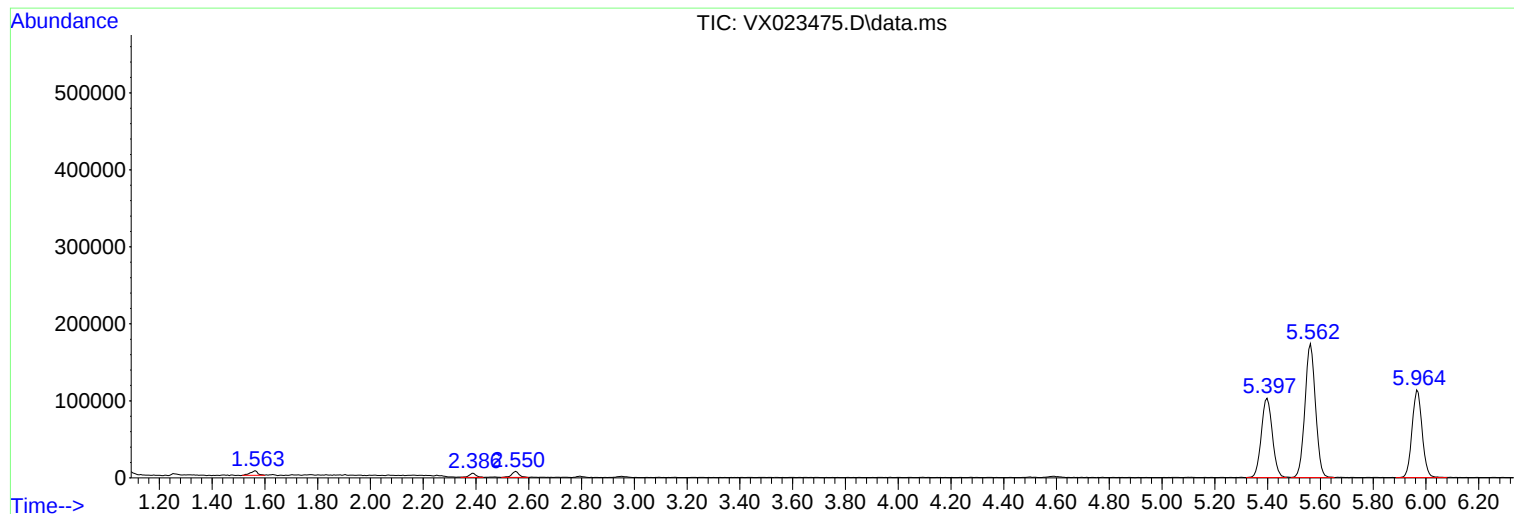

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023475.D
Acq On : 27 Jul 2021 14:26
Operator : JC/MD
Sample : M3146-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-9-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023475.D
Acq On : 27 Jul 2021 14:26
Operator : JC/MD
Sample : M3146-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-9-PD

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------