

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
 Data File : VX023476.D
 Acq On : 27 Jul 2021 14:49
 Operator : JC/MD
 Sample : M3146-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-8-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	72	78	84	rVB3	4838	8806	1.02%	0.197%
2	2.550	231	240	249	rBV	9856	18168	2.10%	0.406%
3	4.495	551	559	568	rBV	15454	40618	4.70%	0.909%
4	5.397	693	707	721	rBV3	99133	286386	33.15%	6.406%
5	5.562	723	734	747	rVB	167299	468496	54.23%	10.480%
6	5.964	790	800	814	rBV2	108397	289603	33.52%	6.478%
7	6.769	922	932	949	rBV	264679	624786	72.33%	13.976%
8	8.653	1234	1241	1251	rBV	561767	863848	100.00%	19.323%
9	10.055	1465	1471	1488	rBV	545132	738830	85.53%	16.527%
10	11.085	1634	1640	1650	rBV	427496	534449	61.87%	11.955%
11	12.024	1789	1794	1803	rVB	484165	596473	69.05%	13.343%


Sum of corrected areas: 4470463

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023476.D
Acq On : 27 Jul 2021 14:49
Operator : JC/MD
Sample : M3146-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-8-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

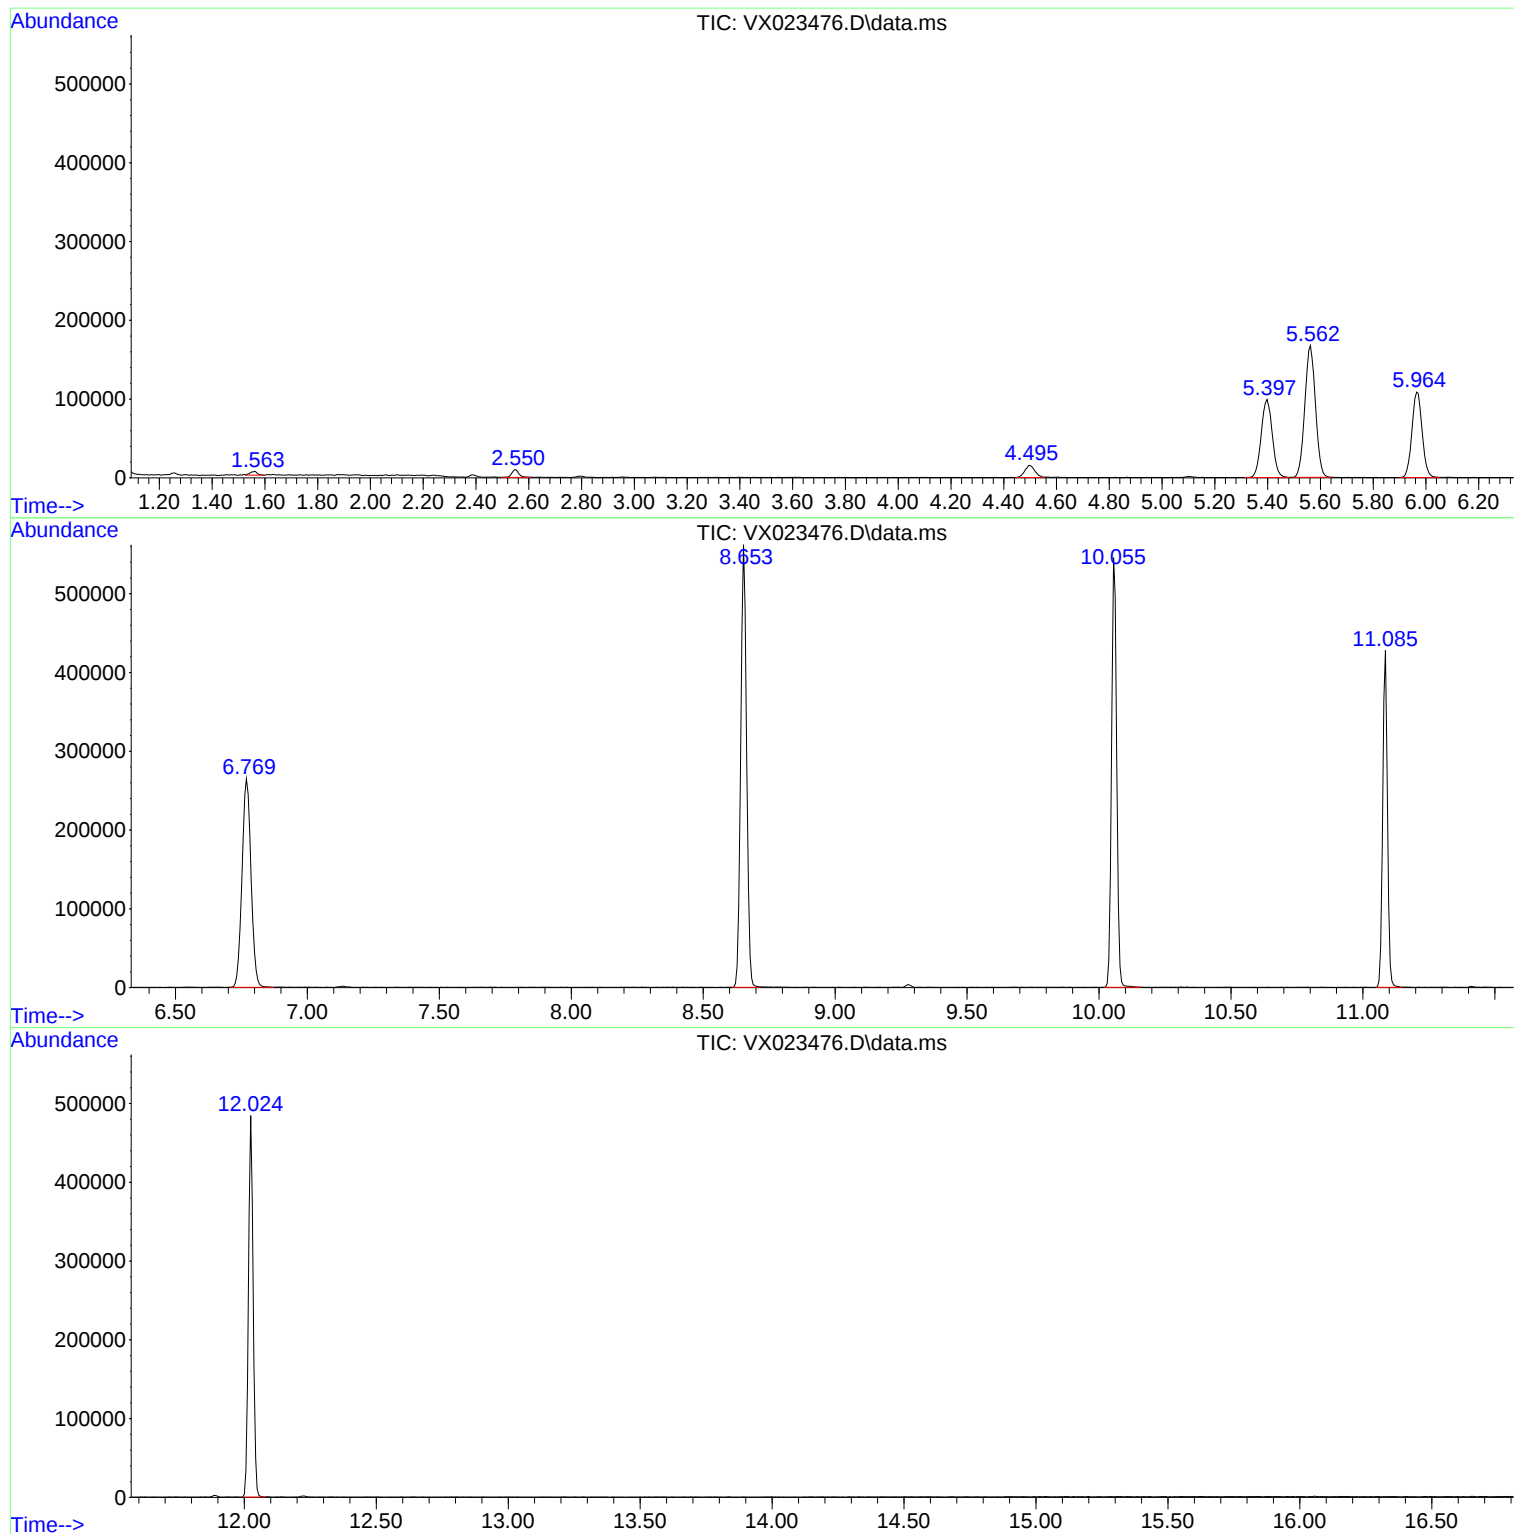

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023476.D
Acq On : 27 Jul 2021 14:49
Operator : JC/MD
Sample : M3146-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-8-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023476.D
Acq On : 27 Jul 2021 14:49
Operator : JC/MD
Sample : M3146-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-8-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
