

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
 Data File : VX023478.D
 Acq On : 27 Jul 2021 15:37
 Operator : JC/MD
 Sample : M3146-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-3-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	70	78	84	rBV3	5188	9097	1.03%	0.176%
2	2.550	234	240	248	rVB	11594	20338	2.29%	0.394%
3	5.397	695	707	720	rBV	103731	302183	34.07%	5.859%
4	5.562	723	734	747	rVB	172842	484104	54.58%	9.386%
5	5.964	789	800	812	rBV	113159	307897	34.71%	5.970%
6	6.769	922	932	945	rBV	277116	657780	74.16%	12.753%
7	8.653	1234	1241	1250	rBV	571441	887004	100.00%	17.198%
8	9.275	1335	1343	1354	rBV	449219	644029	72.61%	12.487%
9	10.055	1466	1471	1478	rBV	540174	731683	82.49%	14.186%
10	11.085	1634	1640	1654	rVB	414621	514782	58.04%	9.981%
11	12.024	1789	1794	1801	rBV	467851	578774	65.25%	11.222%
12	12.542	1874	1879	1889	rVB3	15588	20041	2.26%	0.389%


Sum of corrected areas: 5157712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023478.D
Acq On : 27 Jul 2021 15:37
Operator : JC/MD
Sample : M3146-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-3-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

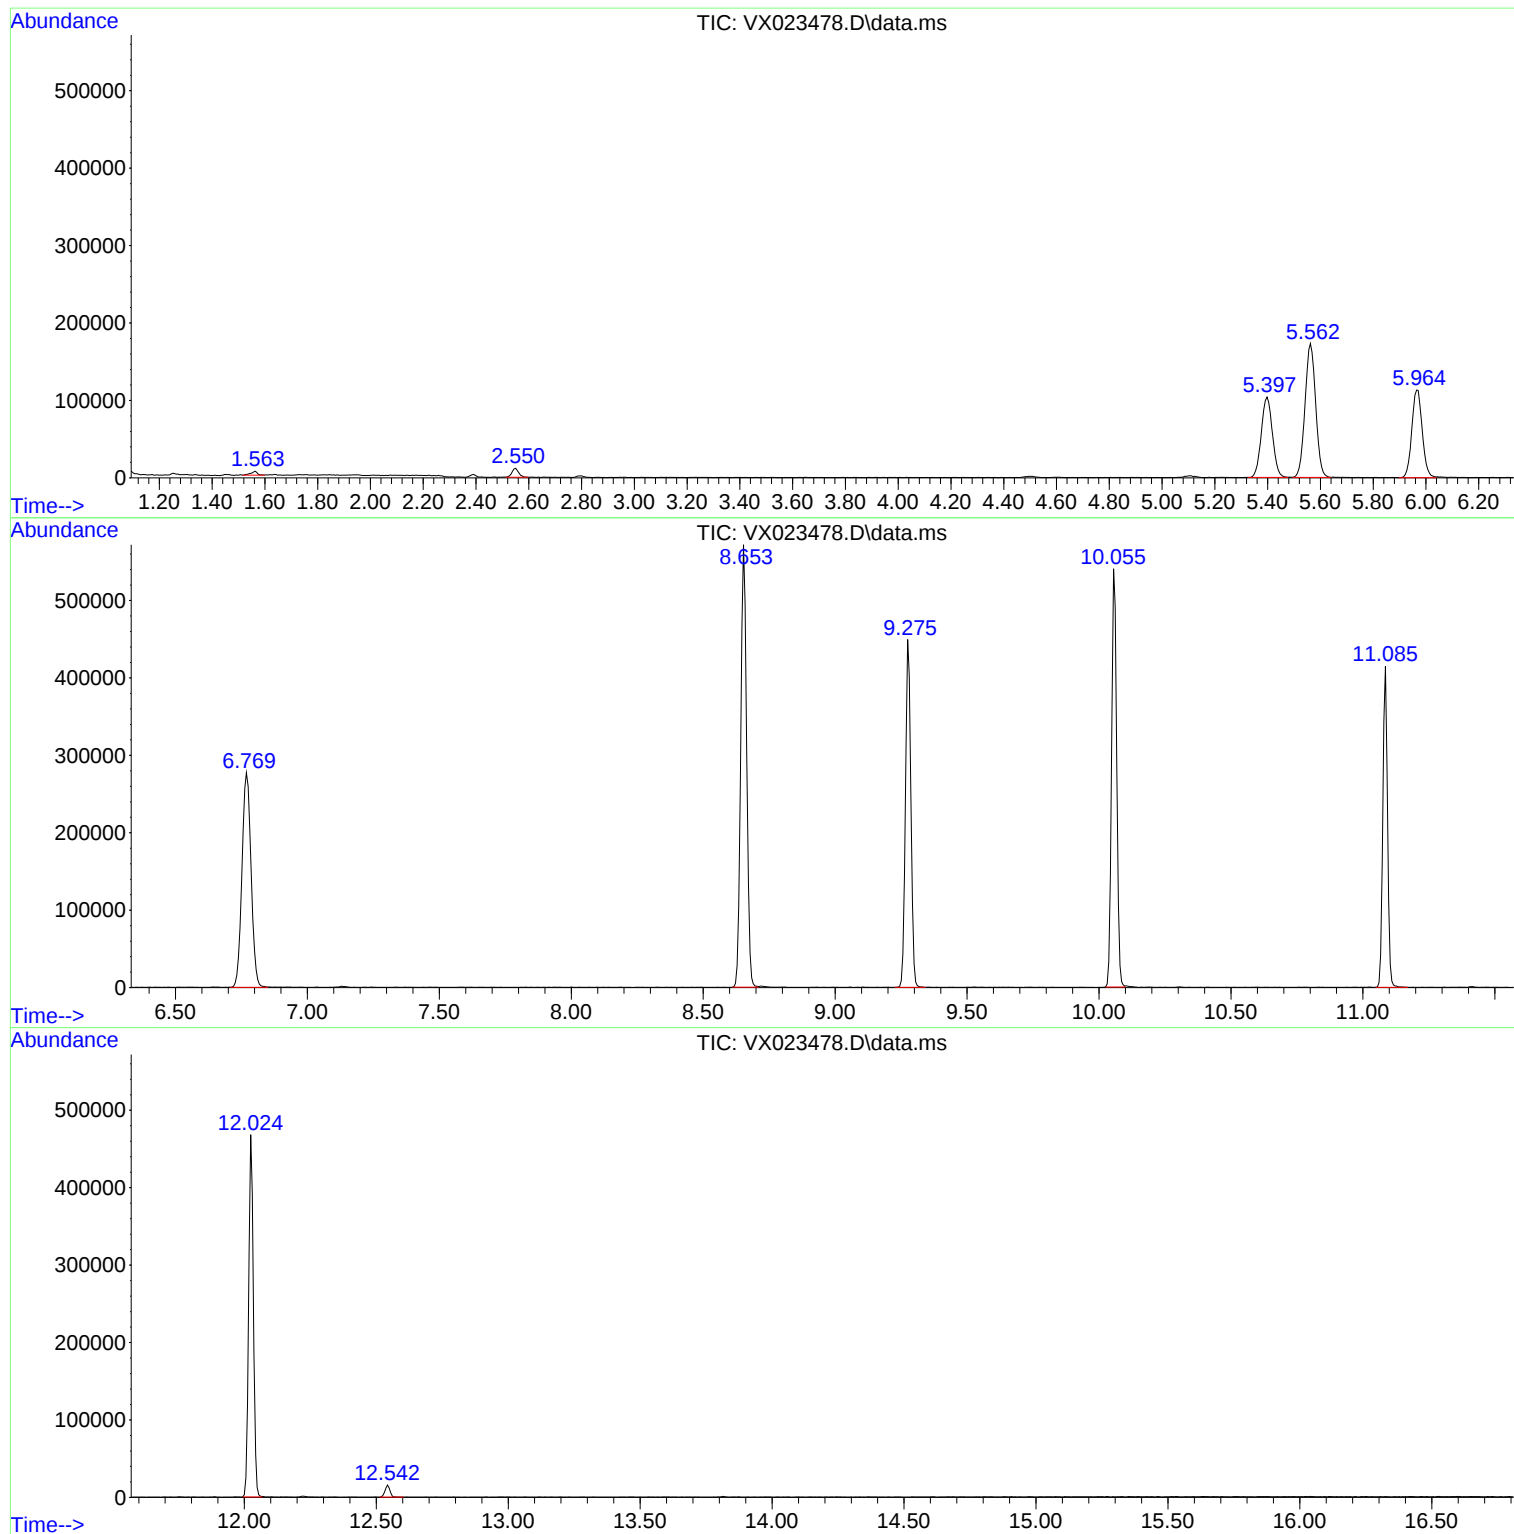

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023478.D
Acq On : 27 Jul 2021 15:37
Operator : JC/MD
Sample : M3146-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-3-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023478.D
Acq On : 27 Jul 2021 15:37
Operator : JC/MD
Sample : M3146-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-3-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------