

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
 Data File : VX023479.D
 Acq On : 27 Jul 2021 16:00
 Operator : JC/MD
 Sample : M3146-15
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 152140-DDC-4-PS

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M

Title : SW846 8260

Signal : TIC: VX023479.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	71	78	84	rVB	5782	10239	1.16%	0.225%
2	2.550	233	240	247	rVB	5997	11034	1.25%	0.243%
3	5.397	695	707	722	rBV	102913	292342	33.11%	6.426%
4	5.562	722	734	749	rVB	169439	473093	53.59%	10.400%
5	5.964	790	800	812	rBV2	113081	296429	33.58%	6.516%
6	6.769	922	932	944	rBV	272170	641609	72.68%	14.104%
7	8.653	1234	1241	1252	rBV	583037	882842	100.00%	19.407%
8	9.275	1337	1343	1350	rBV	53507	81632	9.25%	1.794%
9	10.055	1465	1471	1486	rVB	548298	748249	84.75%	16.448%
10	11.085	1634	1640	1651	rVB	421301	529425	59.97%	11.638%
11	12.024	1789	1794	1804	rBV	470031	573027	64.91%	12.596%
12	12.543	1875	1879	1883	rBV2	7245	9208	1.04%	0.202%


Sum of corrected areas: 4549129

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023479.D
Acq On : 27 Jul 2021 16:00
Operator : JC/MD
Sample : M3146-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

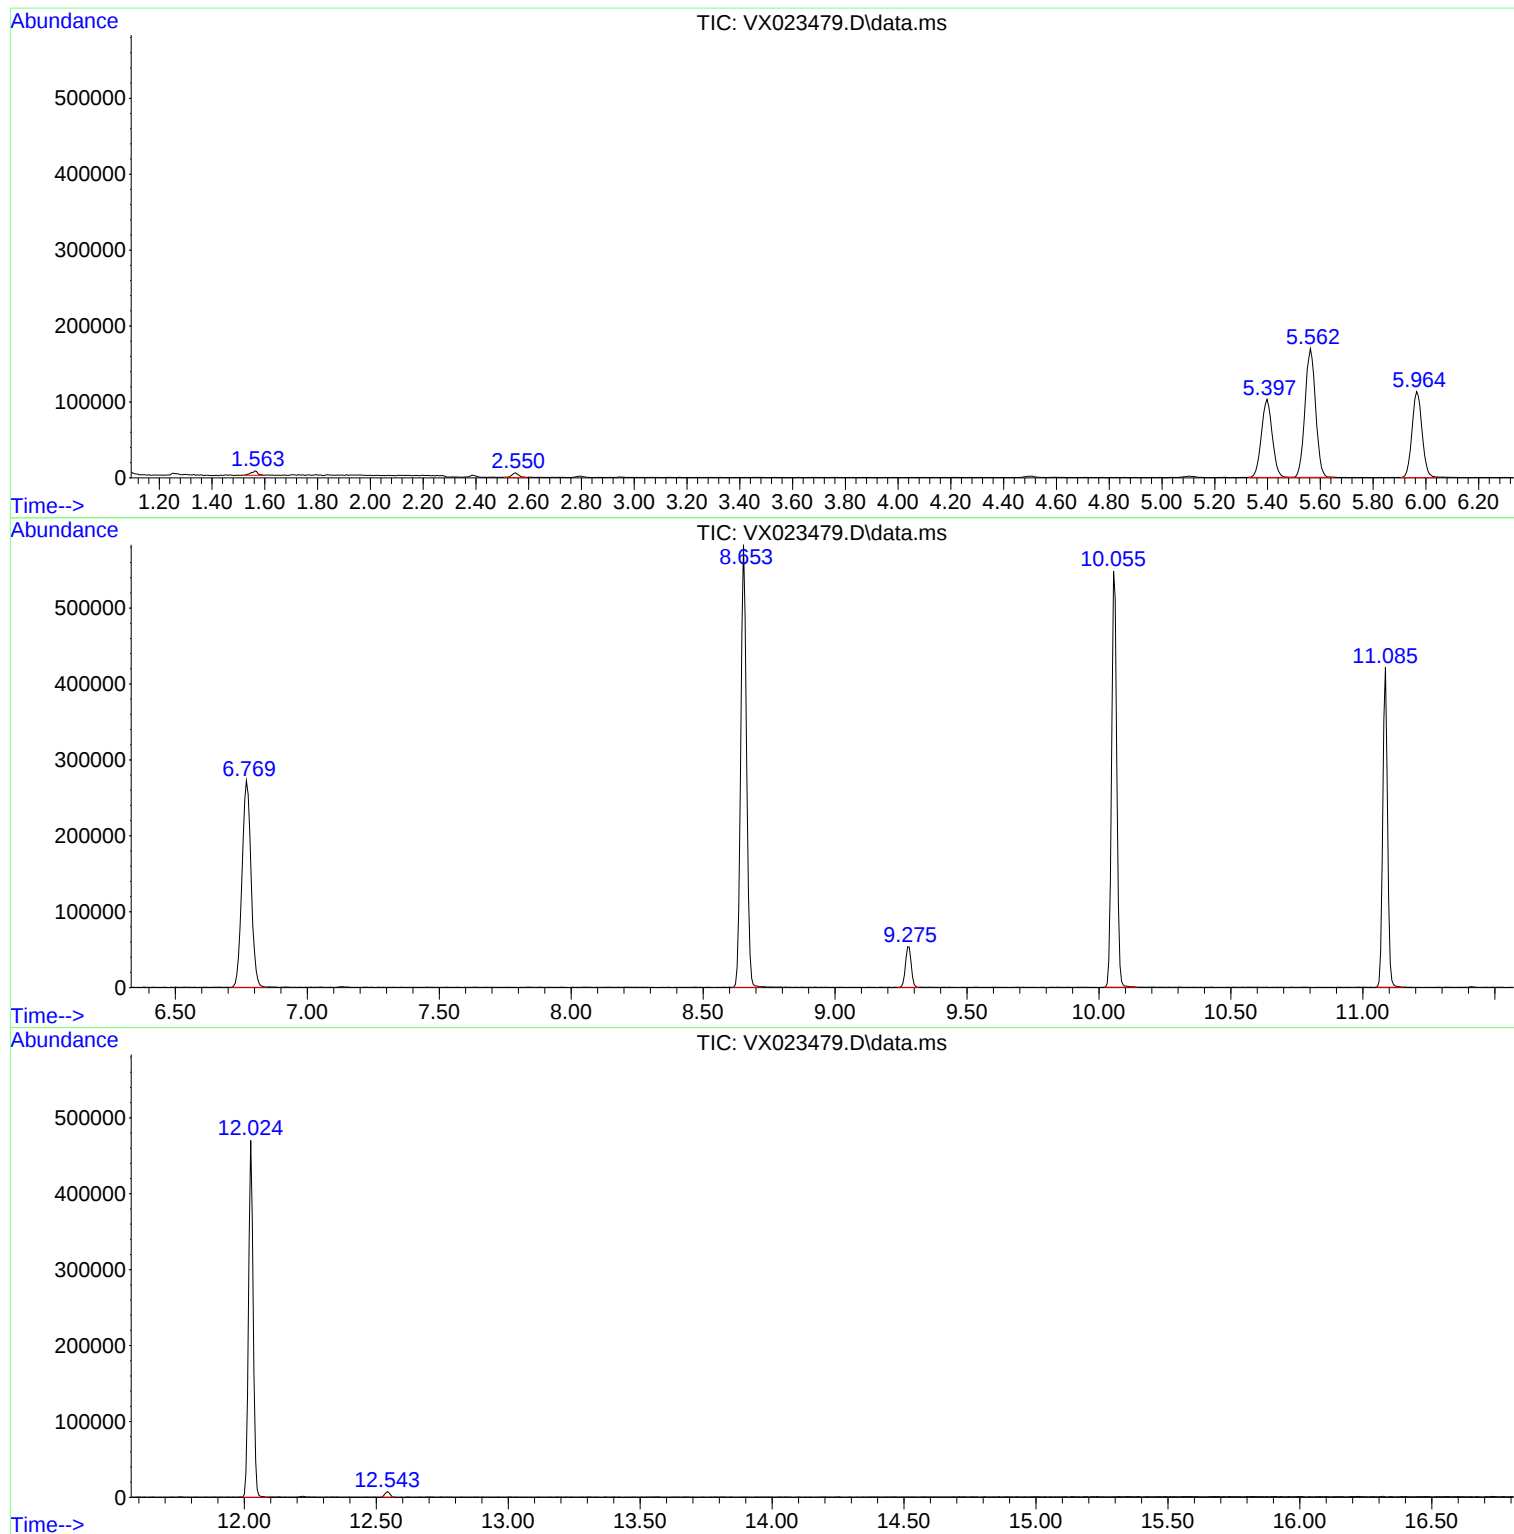

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023479.D
Acq On : 27 Jul 2021 16:00
Operator : JC/MD
Sample : M3146-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072721\
Data File : VX023479.D
Acq On : 27 Jul 2021 16:00
Operator : JC/MD
Sample : M3146-15
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
152140-DDC-4-PS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072221W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
