

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
 Data File : VX030229.D
 Acq On : 27 Jul 2022 14:17
 Operator : JC/MD
 Sample : N3876-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SPC-07-84

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	14	rVB	31343	26977	2.53%	0.539%
2	1.368	41	46	51	rVB3	9003	13041	1.22%	0.261%
3	2.544	229	239	244	rBV2	9016	19653	1.84%	0.393%
4	5.391	694	706	720	rBV	122051	360467	33.79%	7.204%
5	5.556	722	733	749	rVB2	137536	405159	37.98%	8.097%
6	5.964	789	800	817	rBV	147374	399935	37.49%	7.992%
7	6.769	922	932	944	rBV	224410	540344	50.66%	10.798%
8	7.135	983	992	1002	rBV4	5602	13747	1.29%	0.275%
9	8.653	1234	1241	1250	rBV	686664	1066638	100.00%	21.316%
10	10.055	1464	1471	1482	rBV	529266	714800	67.01%	14.285%
11	11.085	1633	1640	1650	rBV	504438	651907	61.12%	13.028%
12	12.024	1789	1794	1803	rBV	637833	791301	74.19%	15.813%




Sum of corrected areas: 5003969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
Data File : VX030229.D
Acq On : 27 Jul 2022 14:17
Operator : JC/MD
Sample : N3876-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-07-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

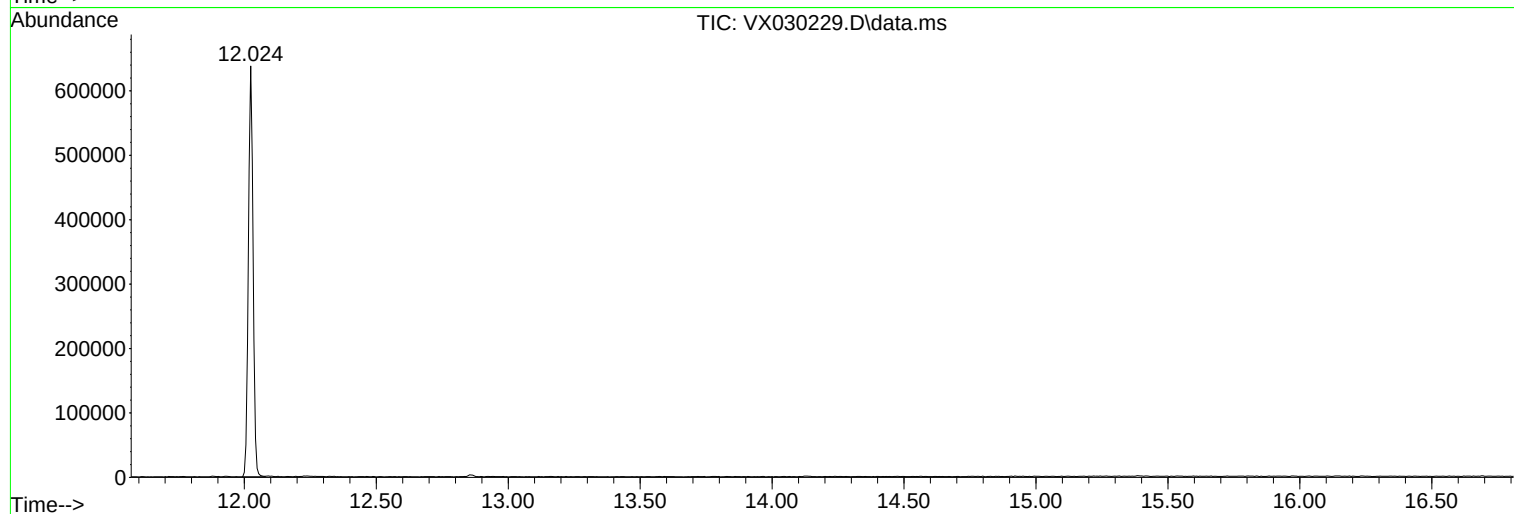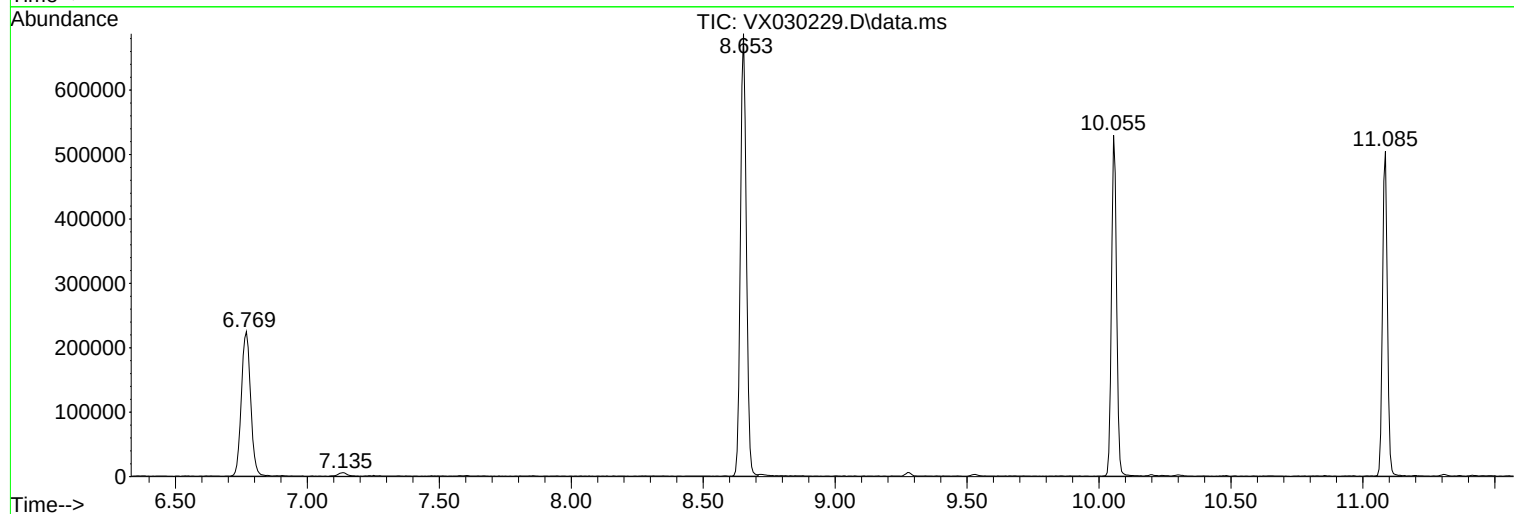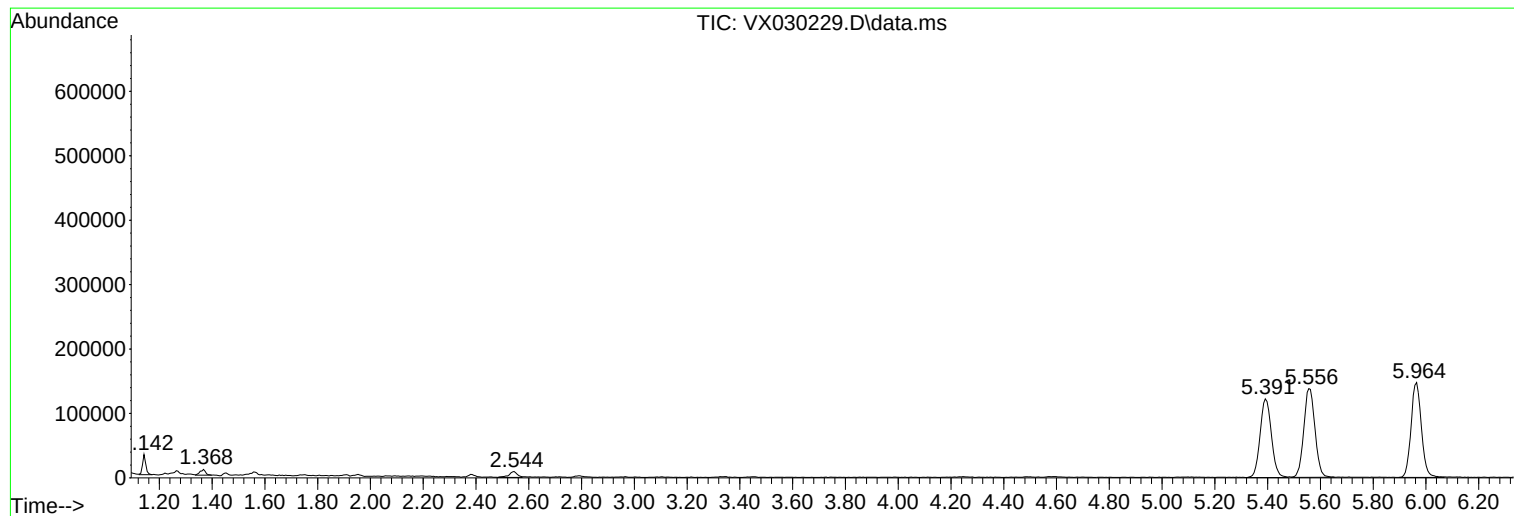

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
Data File : VX030229.D
Acq On : 27 Jul 2022 14:17
Operator : JC/MD
Sample : N3876-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-07-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
Data File : VX030229.D
Acq On : 27 Jul 2022 14:17
Operator : JC/MD
Sample : N3876-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SPC-07-84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc