

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
 Data File : VX030242.D
 Acq On : 27 Jul 2022 19:22
 Operator : JC/MD
 Sample : N3884-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-2022-07-25

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M

Title : SW846 8260

Signal : TIC: VX030242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.581	72	81	84	rBV7	5549	13929	1.41%	0.294%
2	2.544	229	239	250	rBV	19115	38974	3.95%	0.824%
3	2.947	297	305	313	rBV	5718	14118	1.43%	0.298%
4	5.391	694	706	721	rBV2	116068	336954	34.18%	7.124%
5	5.556	721	733	748	rVV	133480	379030	38.45%	8.014%
6	5.958	786	799	814	rBV	141119	378297	38.37%	7.998%
7	6.769	921	932	945	rBV	222110	531236	53.89%	11.232%
8	8.653	1234	1241	1250	rBV	640934	985807	100.00%	20.842%
9	10.055	1466	1471	1481	rBV	500576	679688	68.95%	14.370%
10	11.085	1634	1640	1650	rBV	470196	614476	62.33%	12.991%
11	12.024	1789	1794	1801	rBV	620881	757349	76.83%	16.012%




Sum of corrected areas: 4729858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
Data File : VX030242.D
Acq On : 27 Jul 2022 19:22
Operator : JC/MD
Sample : N3884-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-2022-07-25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

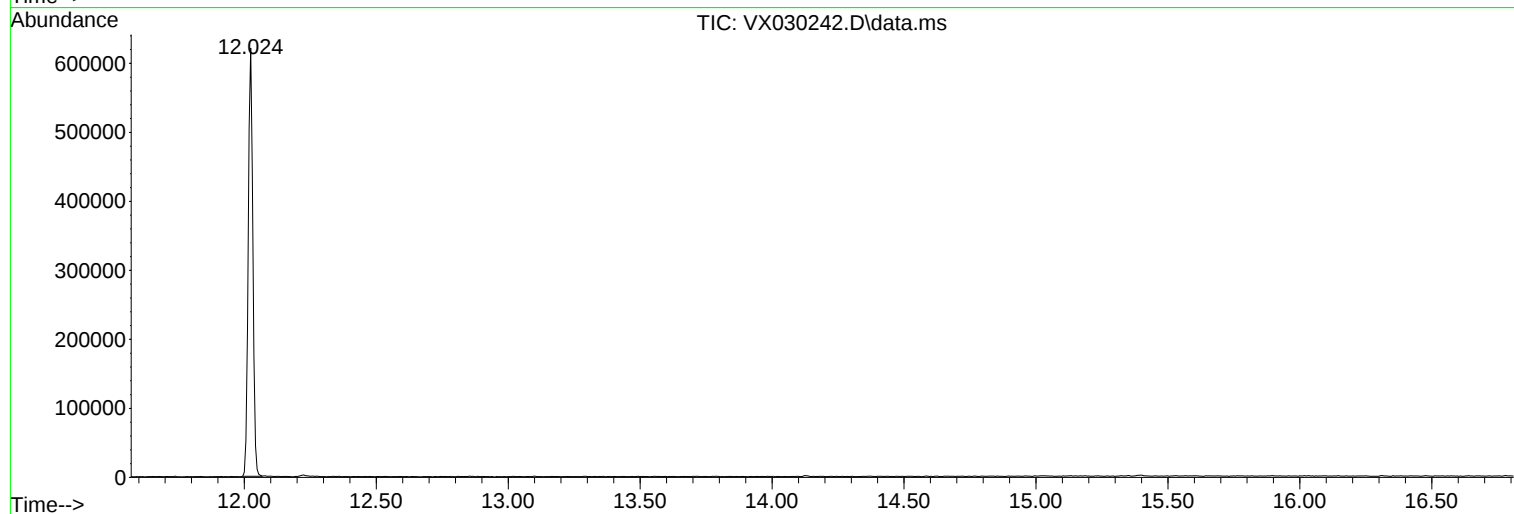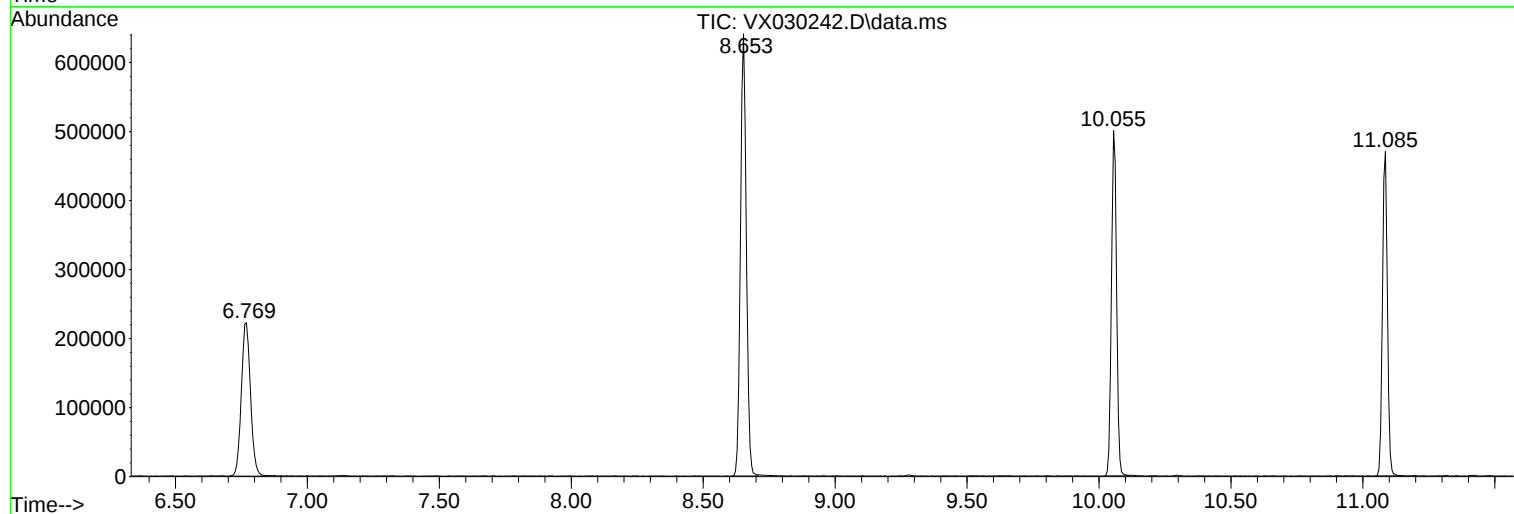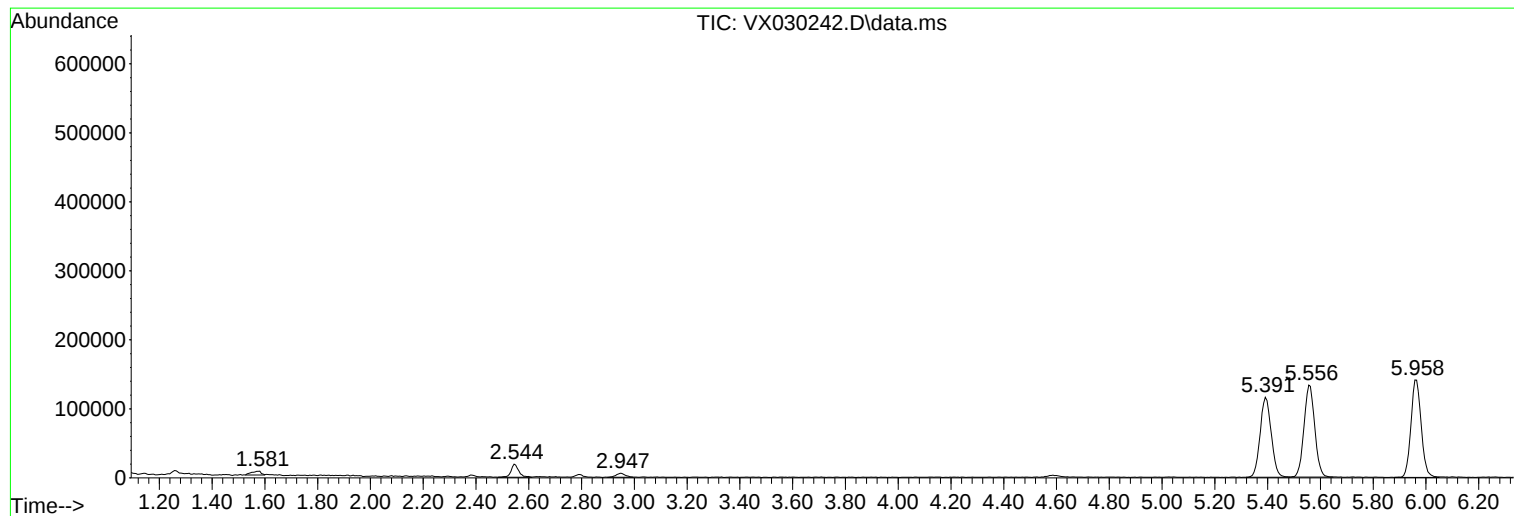

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
Data File : VX030242.D
Acq On : 27 Jul 2022 19:22
Operator : JC/MD
Sample : N3884-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-2022-07-25










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.544	5.14 ug/l	38974	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	40
3			Formamide	45	CH3NO	000075-12-7	5
4			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	4
5			Propanoic acid, 2-hydroxy-, meth...	104	C4H8O3	000547-64-8	4

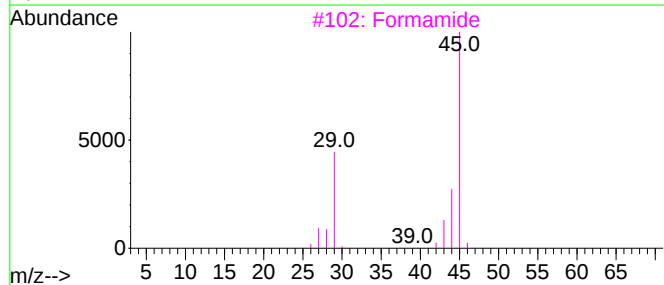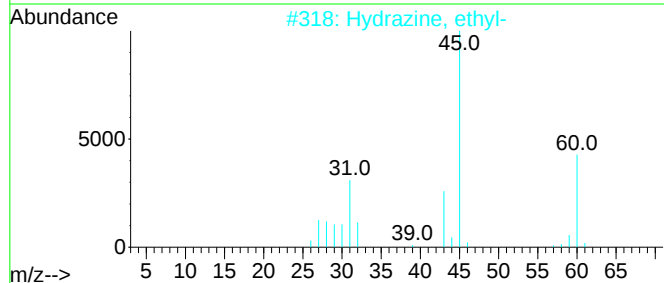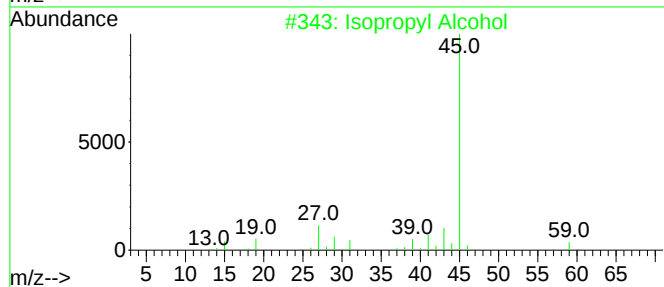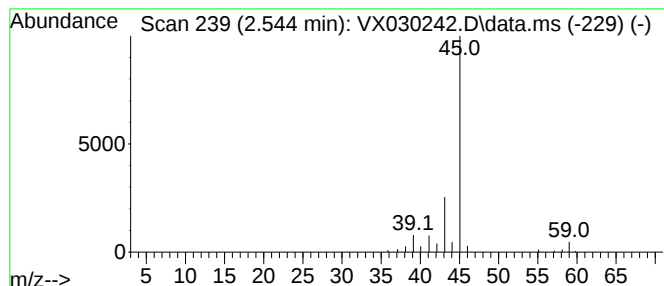

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
Data File : VX030242.D
Acq On : 27 Jul 2022 19:22
Operator : JC/MD
Sample : N3884-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-2022-07-25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.544	5.1	ug/l	38974	1	5.562	379030	50.0