
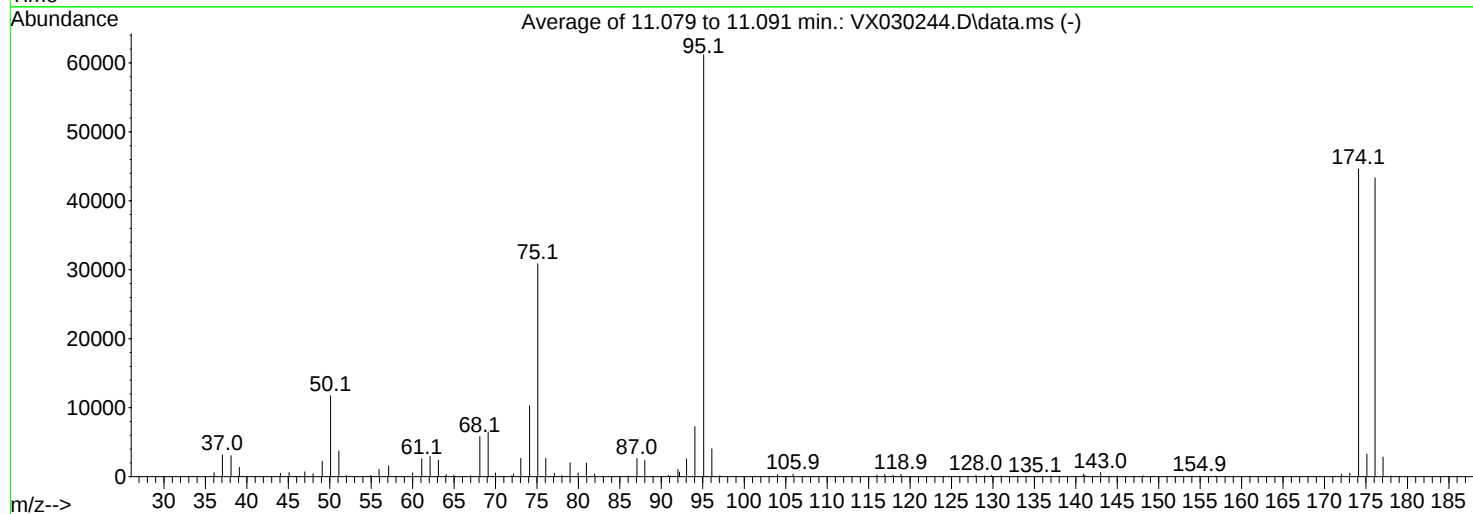


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072722\
Data File : VX030244.D
Acq On : 27 Jul 2022 20:09
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072522W.M
Title : SW846 8260
Last Update : Mon Jul 25 16:49:17 2022

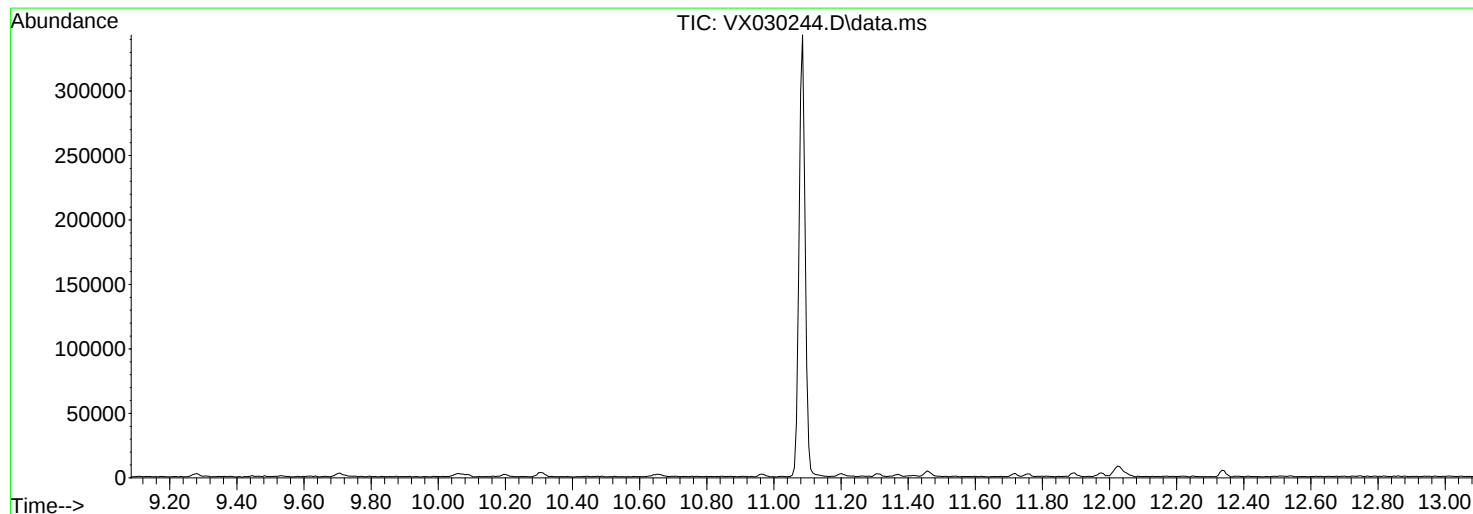

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	11733	PASS
75	95	30	60	50.5	30899	PASS
95	95	100	100	100.0	61173	PASS
96	95	5	9	6.6	4049	PASS
173	174	0.00	2	1.1	501	PASS
174	95	50	100	72.9	44616	PASS
175	174	5	9	7.3	3278	PASS
176	174	95	101	97.1	43339	PASS
177	176	5	9	6.6	2847	PASS