

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072723\
 Data File : VX036672.D
 Acq On : 27 Jul 2023 13:27
 Operator : JC/MD
 Sample : 03767-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MMC-COMP

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M

Title : SW846 8260

Signal : TIC: VX036672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.575	69	80	81	rBV6	6633	16991	1.83%	0.349%
2	2.386	205	213	222	rVB	21139	36932	3.98%	0.758%
3	5.099	649	658	667	rVB	17881	54341	5.85%	1.115%
4	5.385	694	705	720	rBV	114504	334428	36.03%	6.860%
5	5.550	720	732	748	rVB	211339	601558	64.81%	12.340%
6	5.958	789	799	816	rBV2	115698	309000	33.29%	6.339%
7	6.763	921	931	945	rBV	307418	735564	79.24%	15.089%
8	8.647	1233	1240	1248	rBV	586497	928253	100.00%	19.042%
9	10.055	1465	1471	1487	rBV	532295	722412	77.82%	14.820%
10	11.079	1634	1639	1651	rBV	409864	517737	55.78%	10.621%
11	12.024	1788	1794	1802	rBV	469993	617499	66.52%	12.667%




Sum of corrected areas: 4874715

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072723\
Data File : VX036672.D
Acq On : 27 Jul 2023 13:27
Operator : JC/MD
Sample : 03767-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MMC-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

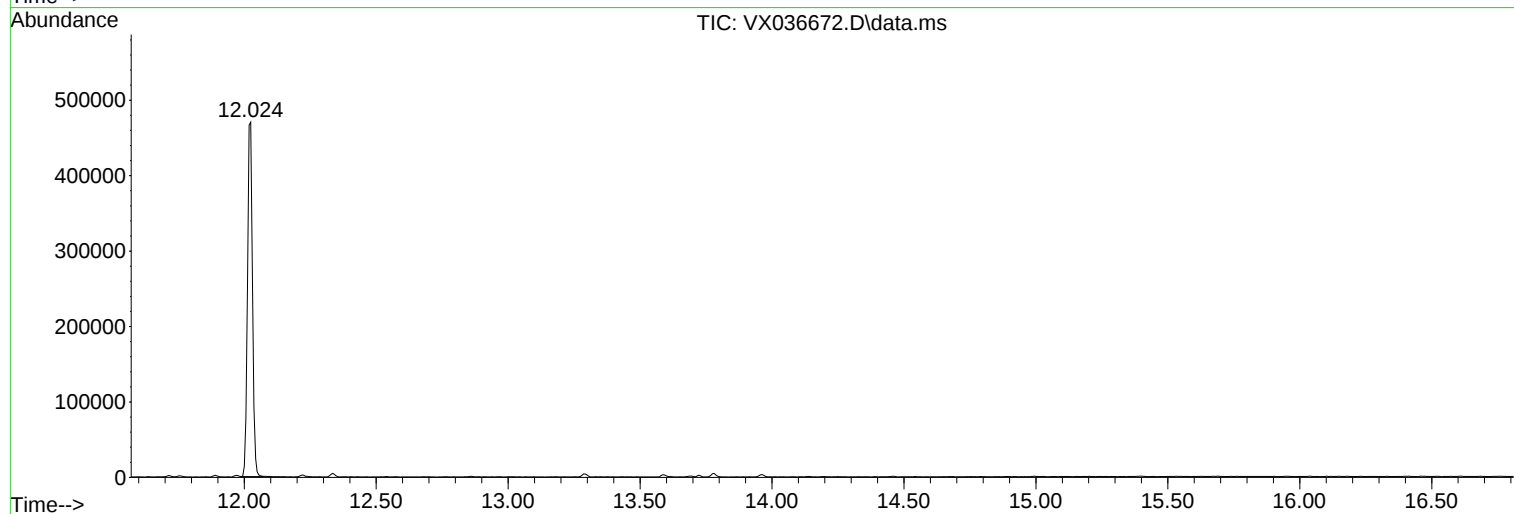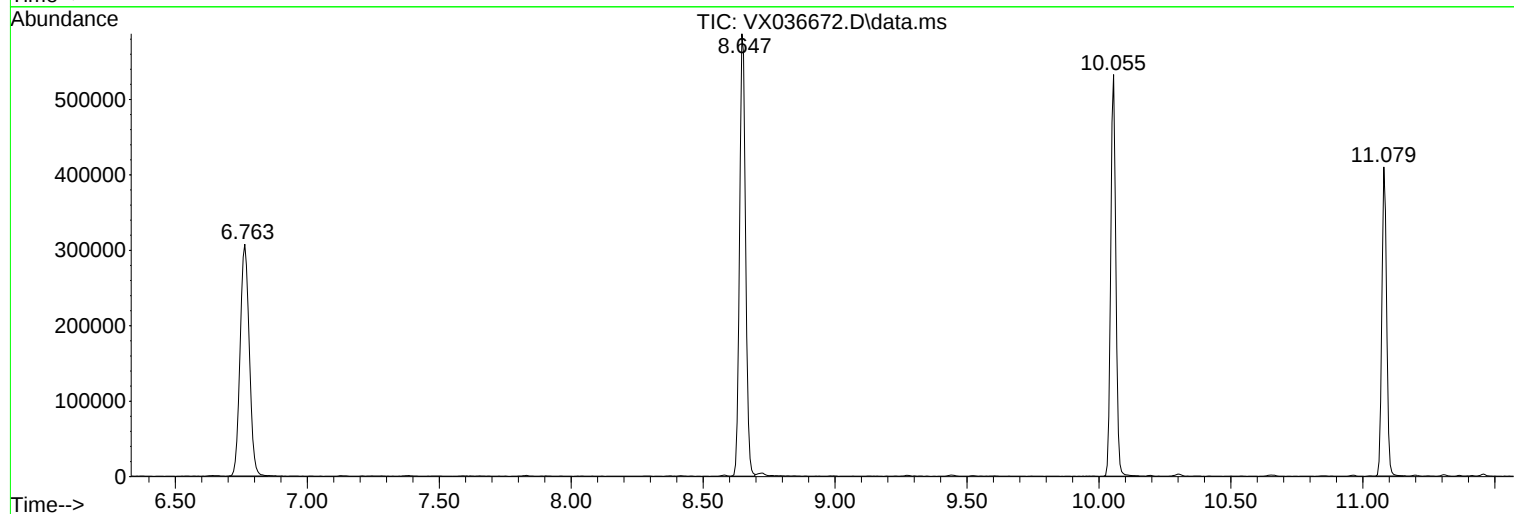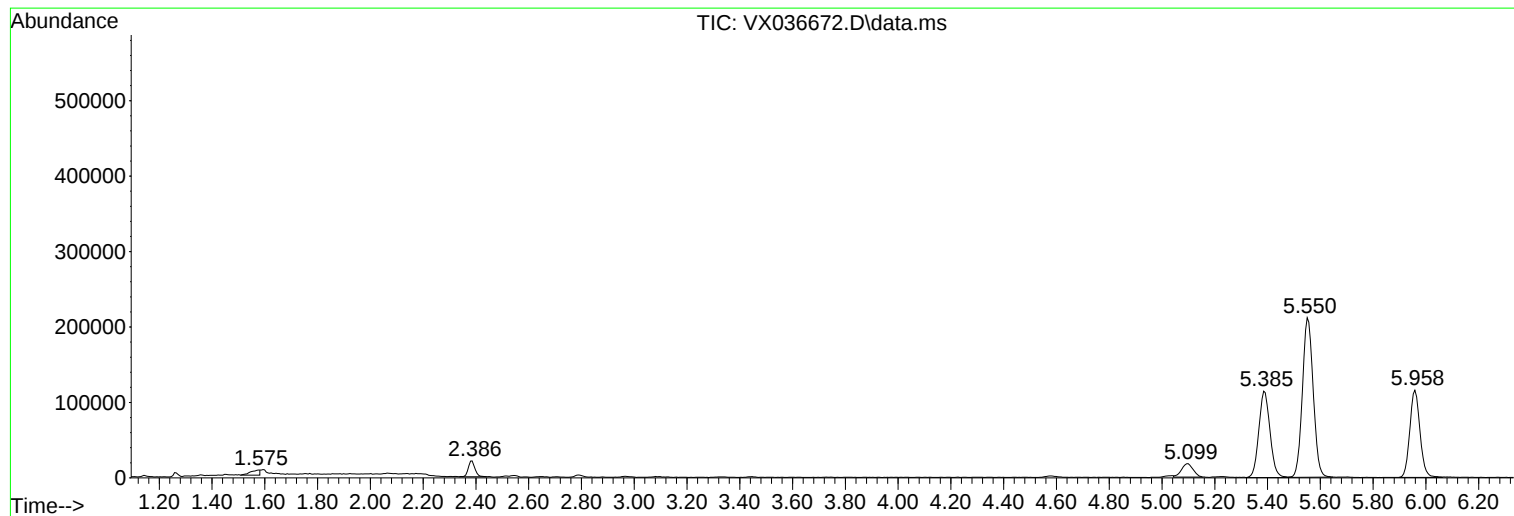

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072723\
Data File : VX036672.D
Acq On : 27 Jul 2023 13:27
Operator : JC/MD
Sample : 03767-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MMC-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072723\
Data File : VX036672.D
Acq On : 27 Jul 2023 13:27
Operator : JC/MD
Sample : 03767-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MMC-COMP

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------