



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072723\
Data File : VX036666.D
Acq On : 27 Jul 2023 09:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072123W.M
Title : SW846 8260
Last Update : Fri Jul 21 12:14:12 2023

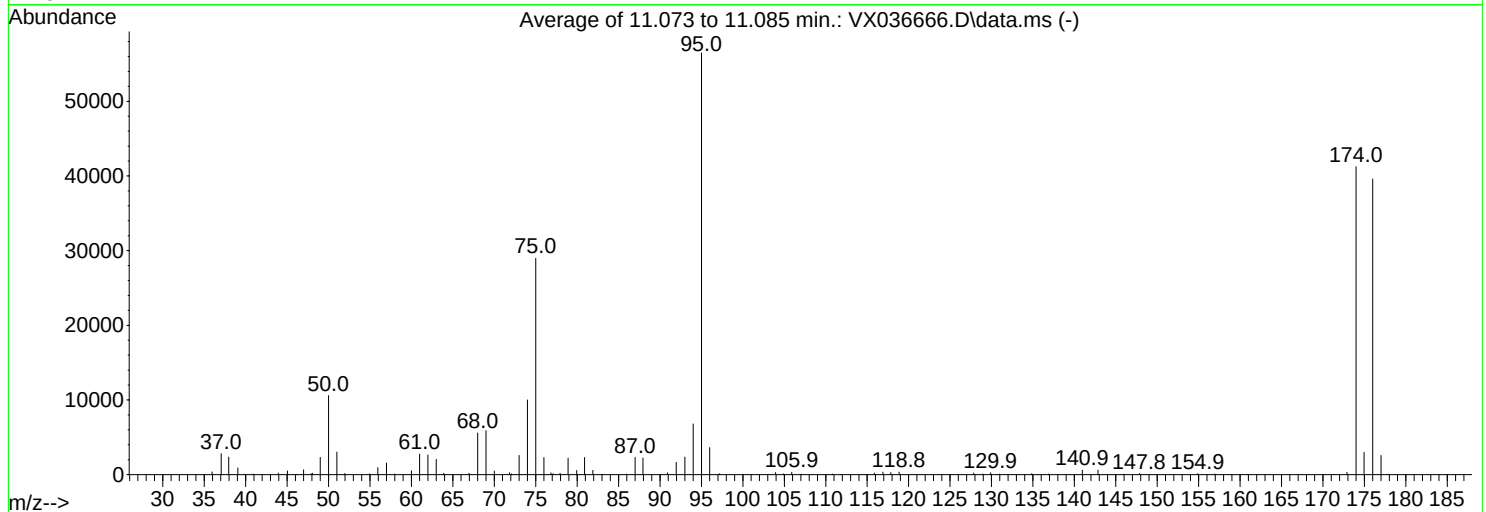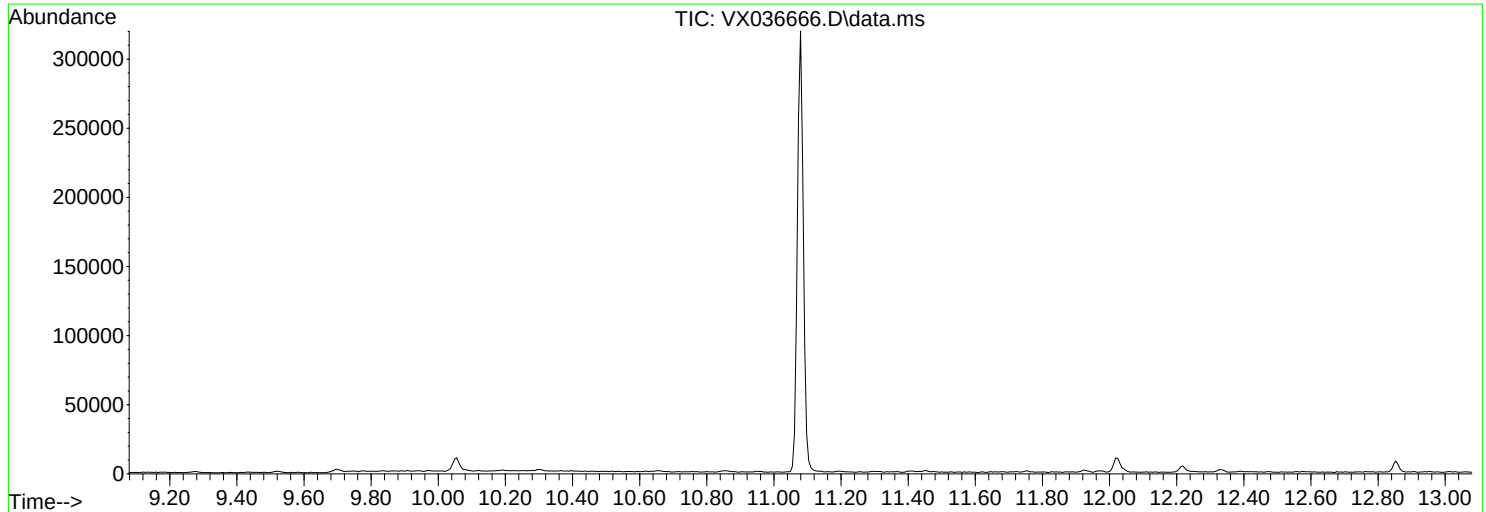

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	10593	PASS
75	95	30	60	51.3	28976	PASS
95	95	100	100	100.0	56491	PASS
96	95	5	9	6.4	3633	PASS
173	174	0.00	2	0.8	326	PASS
174	95	50	100	73.0	41248	PASS
175	174	5	9	7.2	2971	PASS
176	174	95	101	96.0	39595	PASS
177	176	5	9	6.5	2583	PASS