

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072724\
 Data File : VX042587.D
 Acq On : 25 Jul 2024 23:09
 Operator : JC/MD
 Sample : P3328-06ME 20X
 Misc : 8.62g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Jul 26 01:51:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jul 26 00:18:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.763	114	186922	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	167370	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	73540	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	37324	34.305	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	68.620%
7) Chloroethane-d5	1.648	69	25981	37.926	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	75.860%
11) 1,1-Dichloroethene-d2	2.300	65	19491	40.933	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	81.860%
21) 2-Butanone-d5	4.465	46	77677	99.070	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.070%
24) Chloroform-d	5.056	84	98842	45.183	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.360%
26) 1,2-Dichloroethane-d4	5.952	65	63777	49.393	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.780%
32) Benzene-d6	5.971	84	198212	45.817	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.640%
36) 1,2-Dichloropropane-d6	7.306	67	62537	48.035	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.060%
41) Toluene-d8	8.647	98	170453	42.280	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.560%
43) trans-1,3-Dichloroprop...	8.952	79	23841	42.371	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.740%
47) 2-Hexanone-d5	9.385	63	56063	94.867	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.870%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	88192	45.820	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.640%
66) 1,2-Dichlorobenzene-d4	12.317	152	70307	49.221	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.440%
Target Compounds						
					Qvalue	
37) 1,2-Dichloropropane	7.306	63	6539	5.445	ug/L #	84
61) 1,2,3-Trichloropropane	12.024	75	6791	5.200	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072724\
Data File : VX042587.D
Acq On : 25 Jul 2024 23:09
Operator : JC/MD
Sample : P3328-06ME 20X
Misc : 8.62g/5.0mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Jul 26 01:51:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML070324WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Jul 26 00:18:59 2024
Response via : Initial Calibration

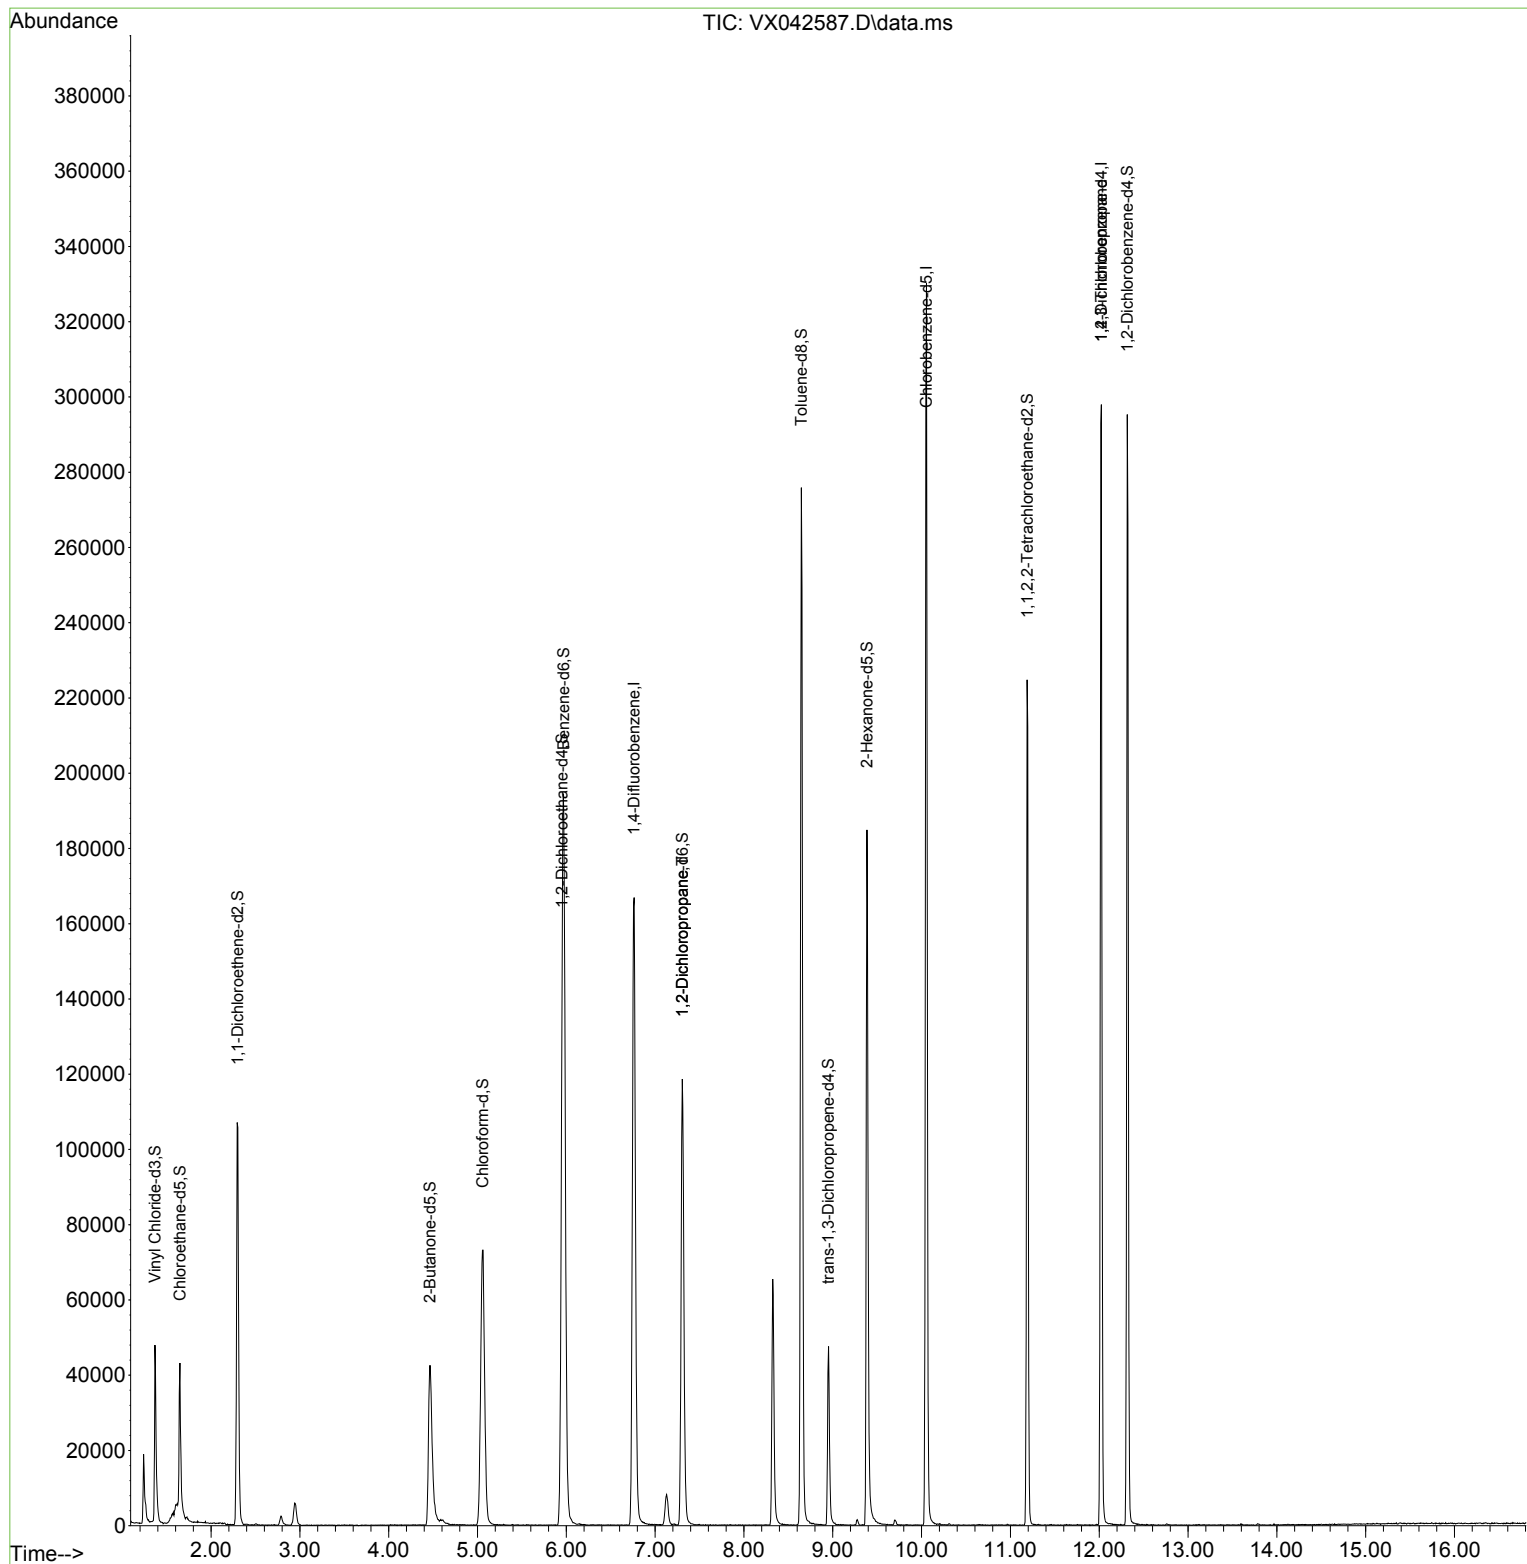

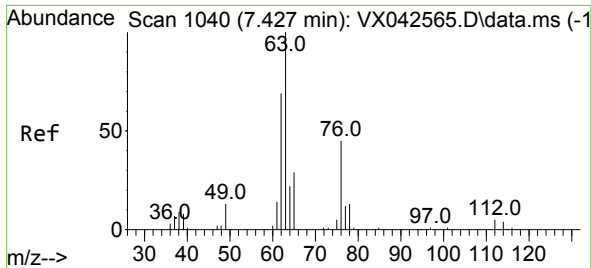

#37

1,2-Dichloropropane

Concen: 5.445 ug/L

RT: 7.306 min Scan# 1

Delta R.T. -0.122 min

Lab File: VX042587.D

Acq: 25 Jul 2024 23:09

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 63 Resp: 6539

Ion Ratio Lower Upper

63 100

112 0.0 4.3 6.5#

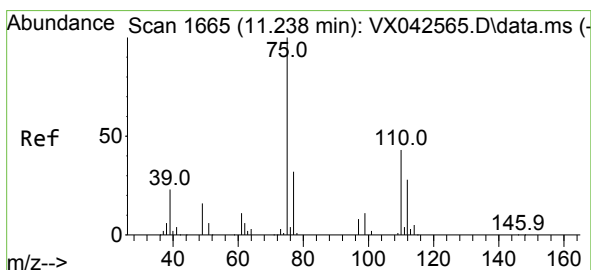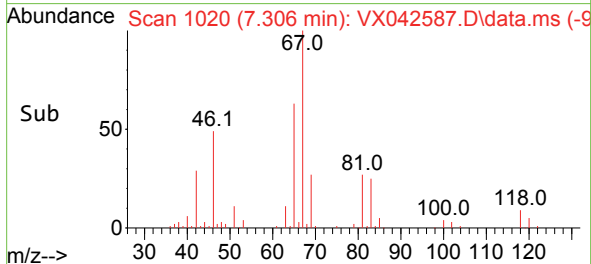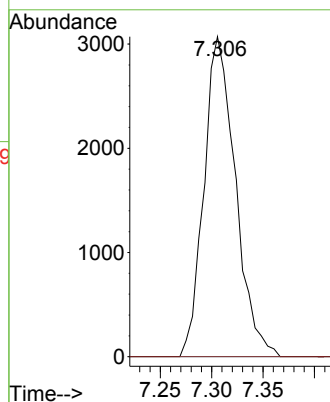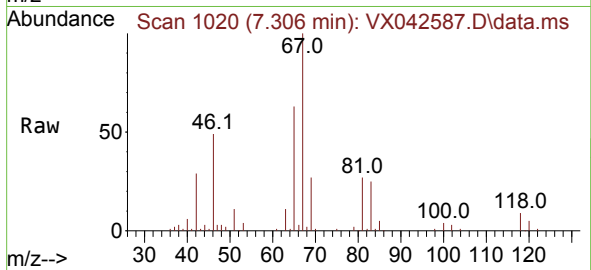

#61

1,2,3-Trichloropropane

Concen: 5.200 ug/L

RT: 12.024 min Scan# 1794

Delta R.T. 0.787 min

Lab File: VX042587.D

Acq: 25 Jul 2024 23:09

Tgt Ion: 75 Resp: 6791

Ion Ratio Lower Upper

75 100

77 32.5 25.8 38.8

110 3.0 35.4 53.0#

